


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081020\
 Data File : BF121233.D
 Acq On : 10 Aug 2020 12:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 29 14:55:43 2020

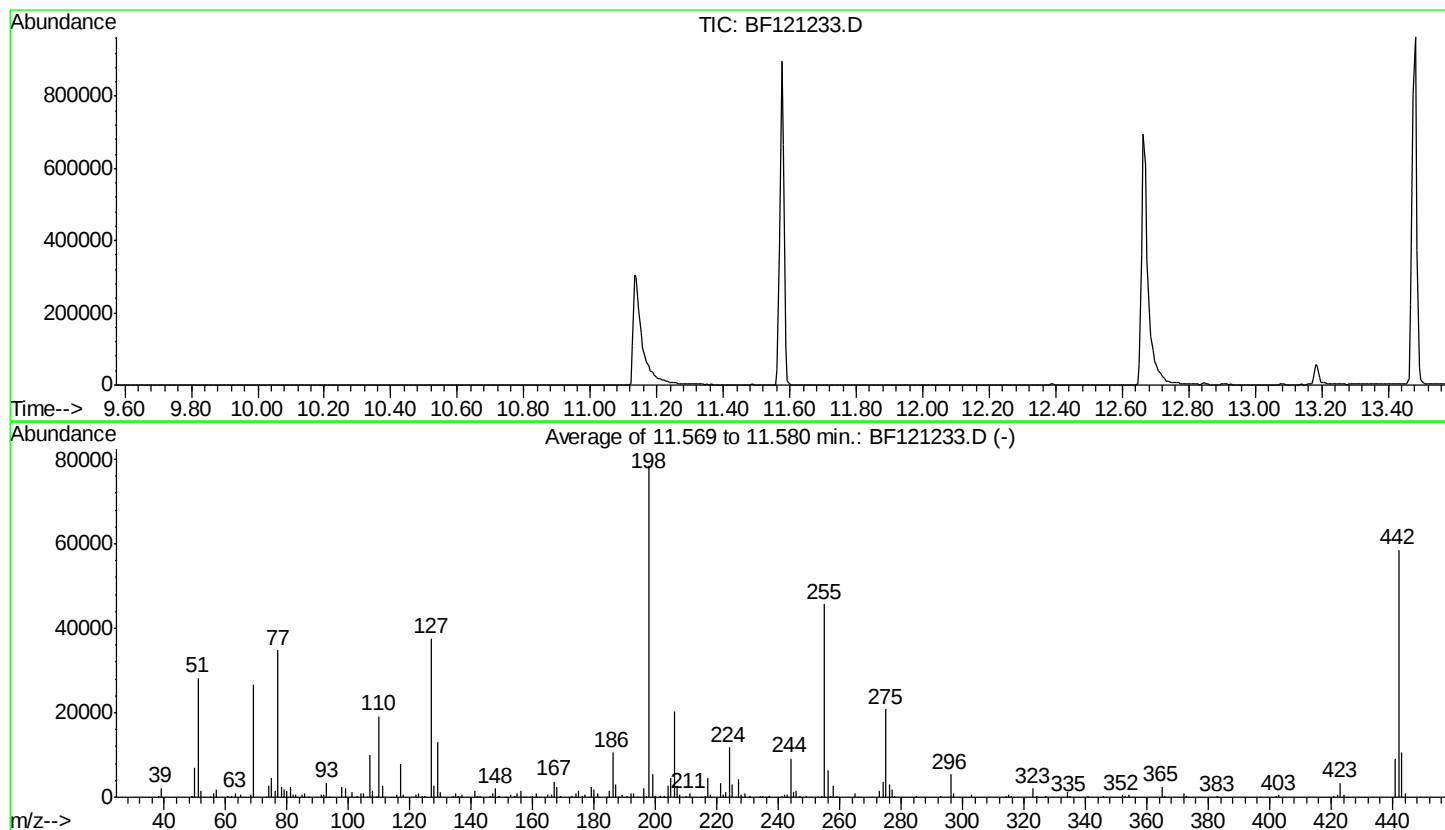

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	28218	PASS
68	69	0.00	2	1.9	508	PASS
69	198	0.00	100	34.1	26749	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	37549	PASS
197	198	0.00	2	0.4	342	PASS
198	198	100	100	100.0	78464	PASS
199	198	5	9	6.9	5395	PASS
275	198	10	60	26.6	20857	PASS
365	198	1	100	3.1	2450	PASS
441	198	0.01	100	11.6	9113	PASS
442	198	50	100	74.7	58609	PASS
443	442	15	24	18.1	10630	PASS