
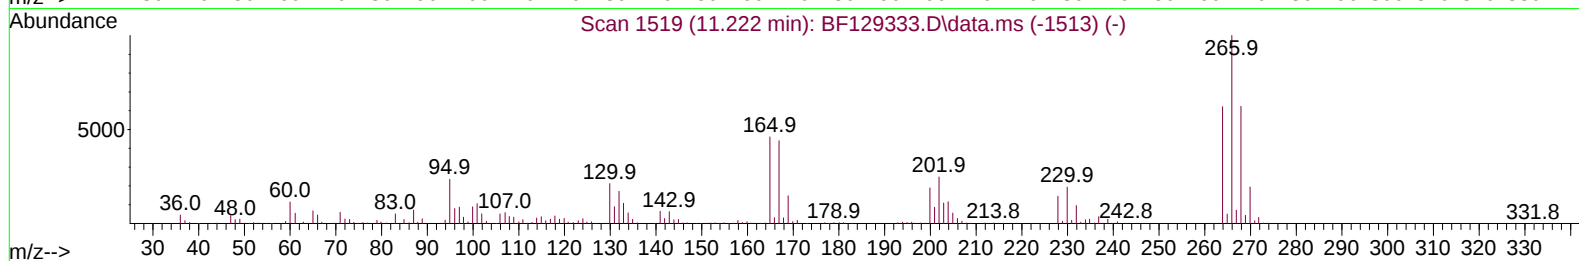
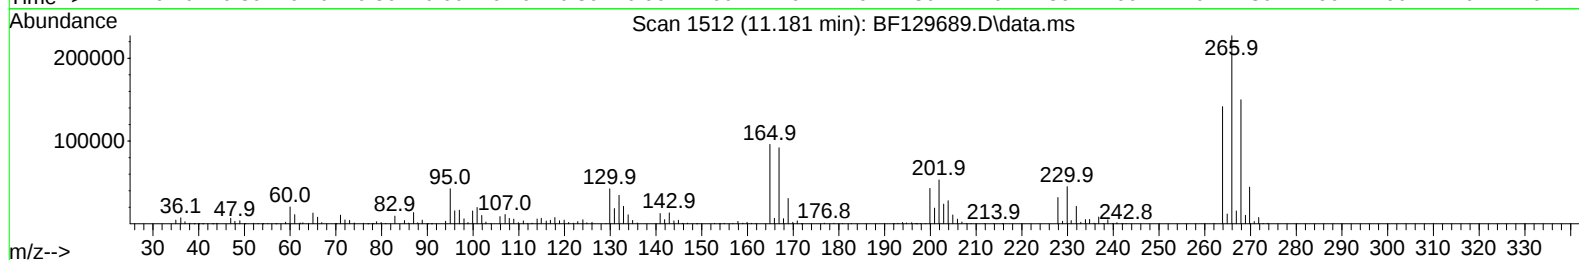


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081022\  
Data File : BF129689.D  
Acq On    : 10 Aug 2022  09:55  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Aug 10 21:26:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 15:26:57 2022
Response via : Initial Calibration

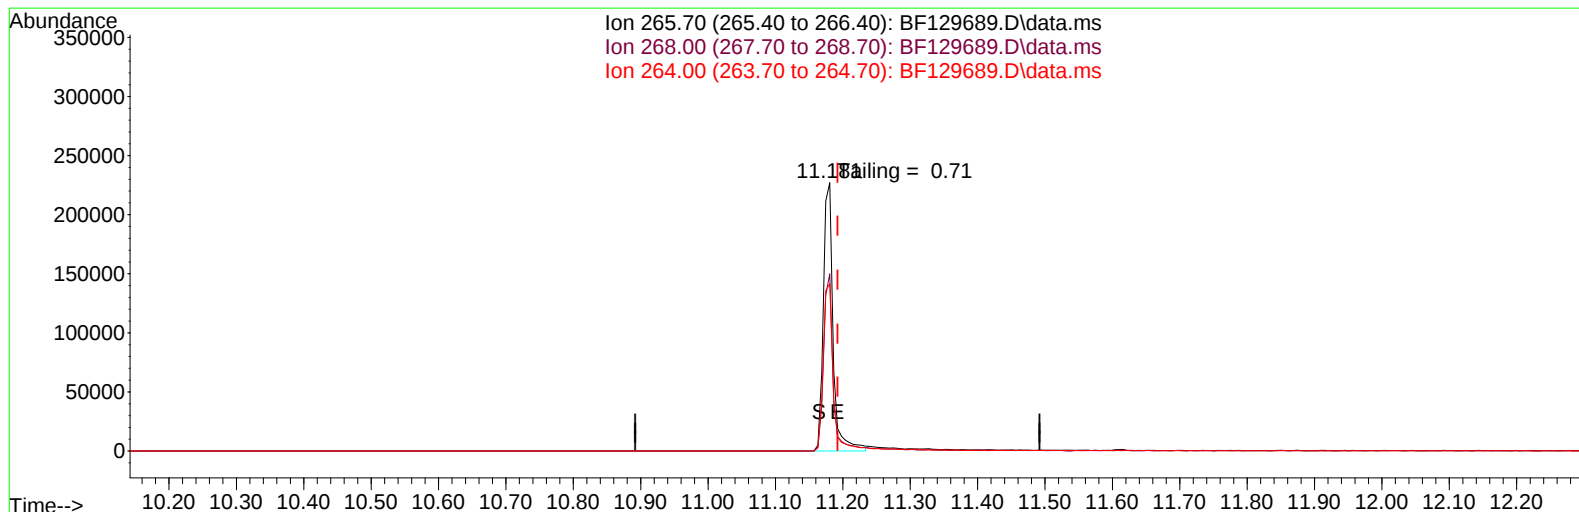

TIC: BF129689.D\data.ms

(70) Pentachlorophenol (C)




11.181min (-0.012) 79990.42 ng

response **237338**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	66.02
264.00	61.80	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081022\
Data File : BF129689.D
Acq On : 10 Aug 2022 09:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 21:26:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 15:26:57 2022
Response via : Initial Calibration

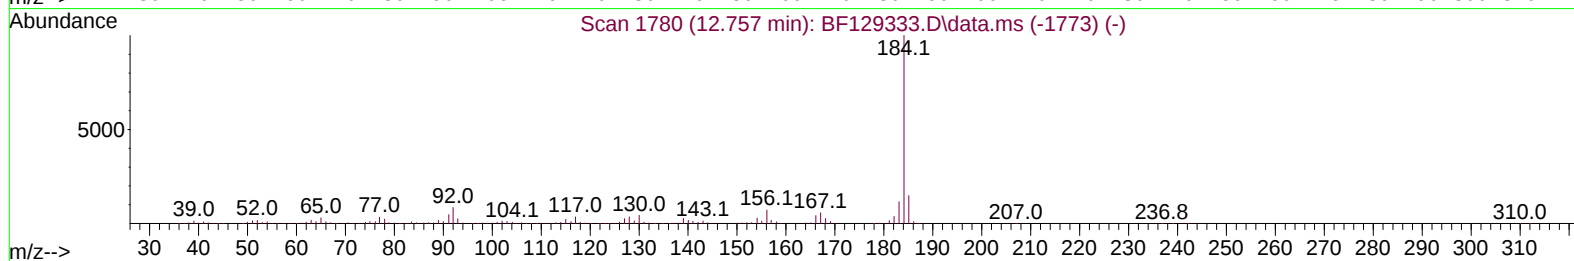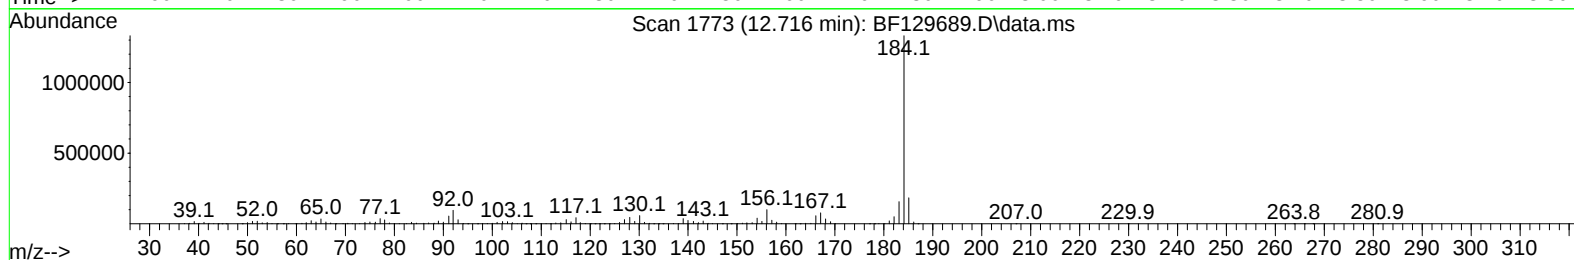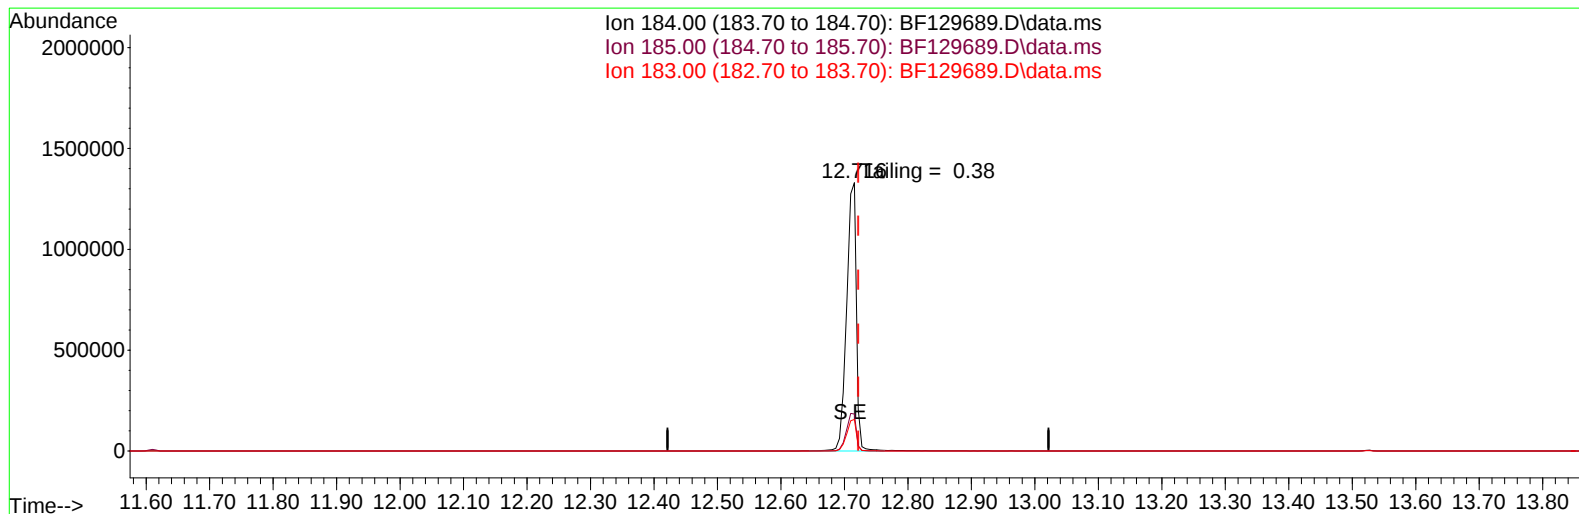

TIC: BF129689.D\data.ms

(77) Benzidine

12.716min (-0.006) 28578.26 ng

response 1430602

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.81
183.00	11.60	11.74
0.00	0.00	0.00