


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081022\  
 Data File : BF129689.D  
 Acq On : 10 Aug 2022 09:55  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Aug 10 15:26:57 2022

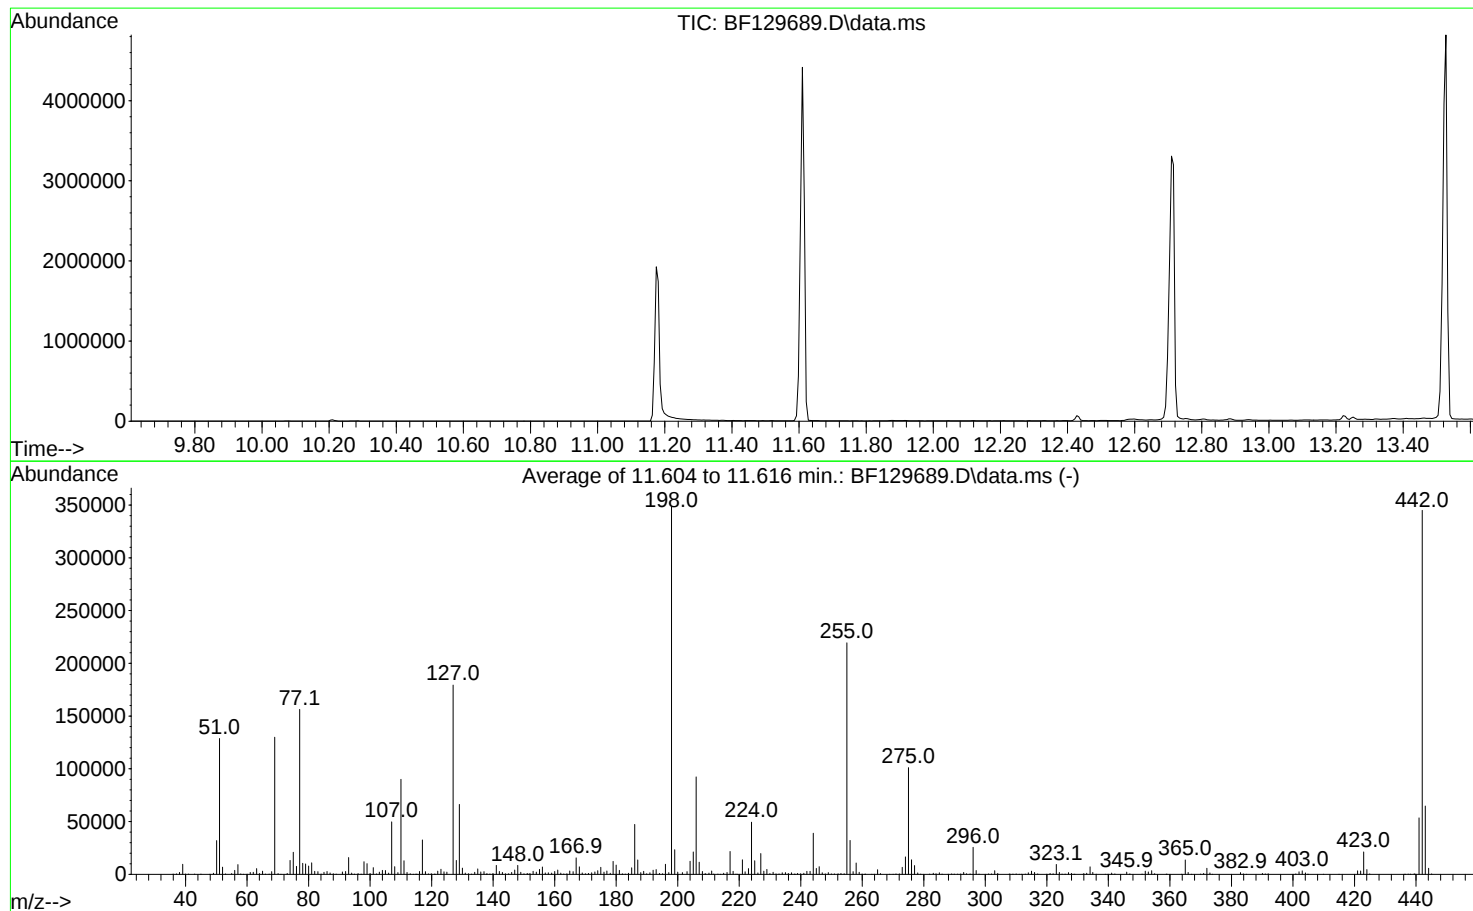




AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1578

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.9         | 128685     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 2490       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.2         | 129875     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 656        | PASS                |
| 127            | 198             | 10              | 80              | 51.4         | 179323     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 1578       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 348693     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 23227      | PASS                |
| 275            | 198             | 10              | 60              | 29.0         | 101141     | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 13605      | PASS                |
| 441            | 198             | 0.01            | 100             | 15.3         | 53523      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 344960     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 64752      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081022\  
Data File : BF129689.D  
Acq On : 10 Aug 2022 09:55  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 10 21:26:53 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 10 15:26:57 2022  
Response via : Initial Calibration

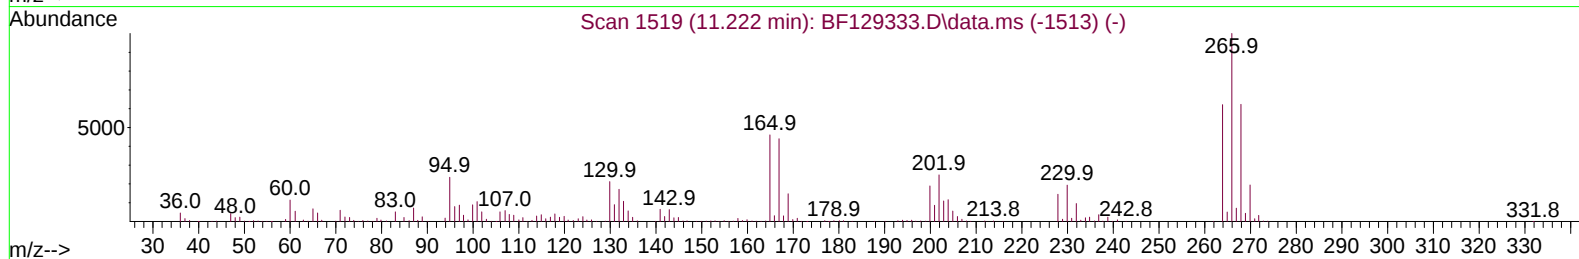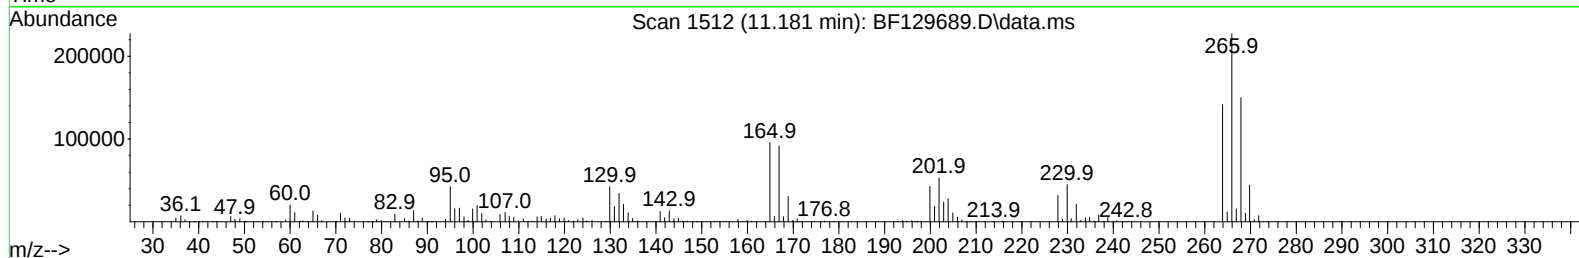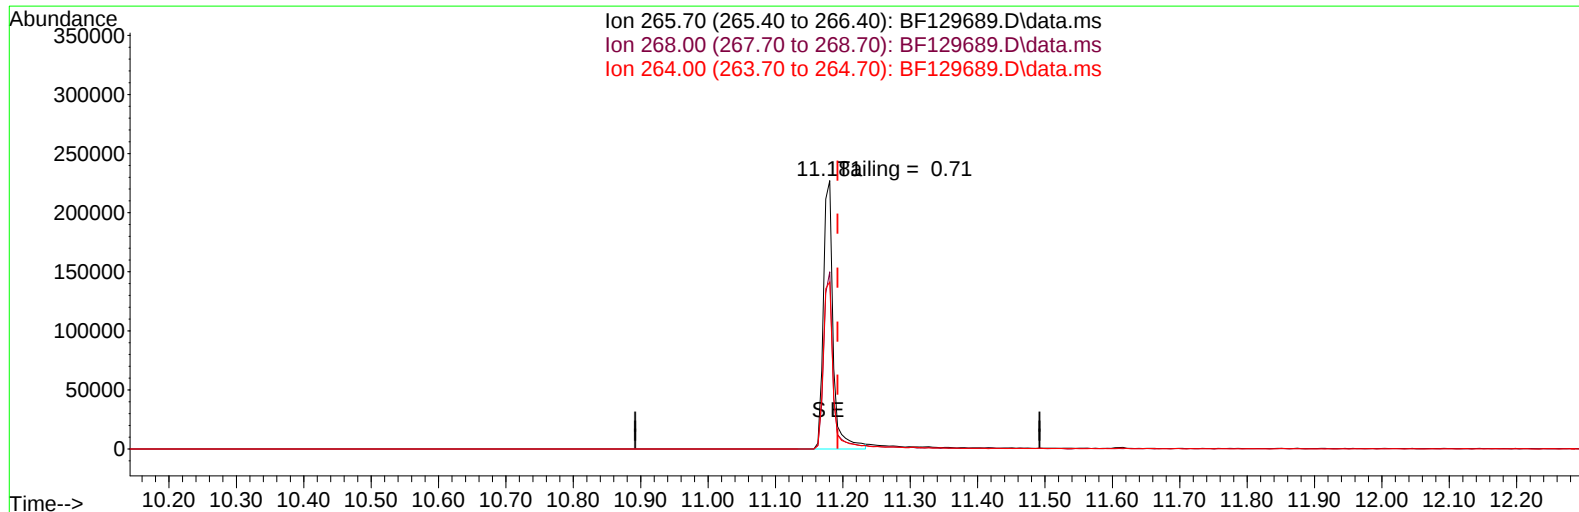

TIC: BF129689.D\data.ms

**(70) Pentachlorophenol (C)**

**11.181min (-0.012) 79990.42 ng**




**response 237338**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.70  | 66.02  |
| 264.00 | 61.80  | 62.30  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081022\  
Data File : BF129689.D  
Acq On : 10 Aug 2022 09:55  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 10 21:26:53 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 10 15:26:57 2022  
Response via : Initial Calibration

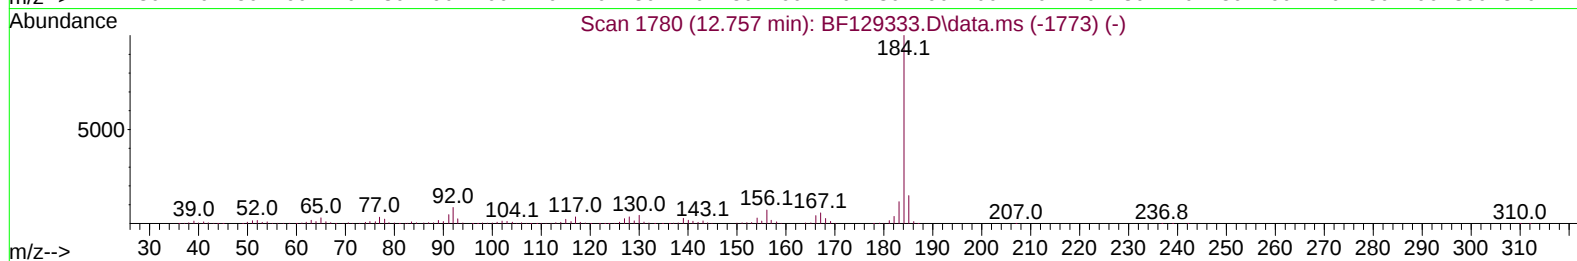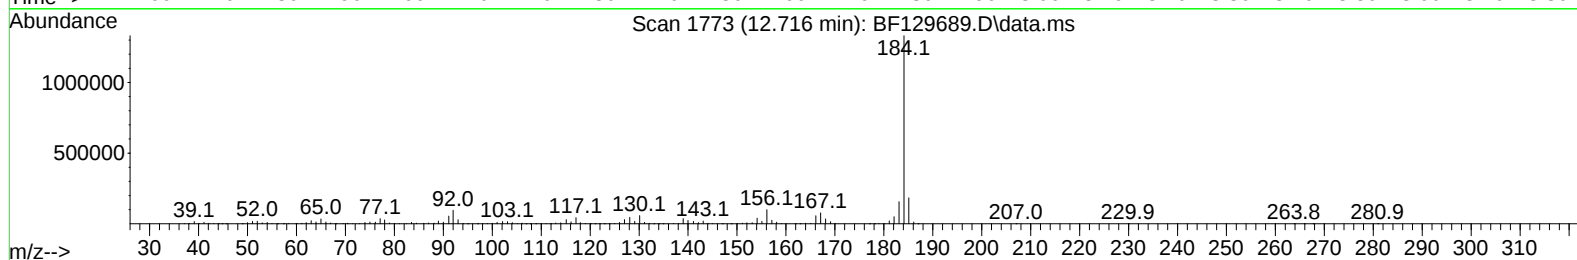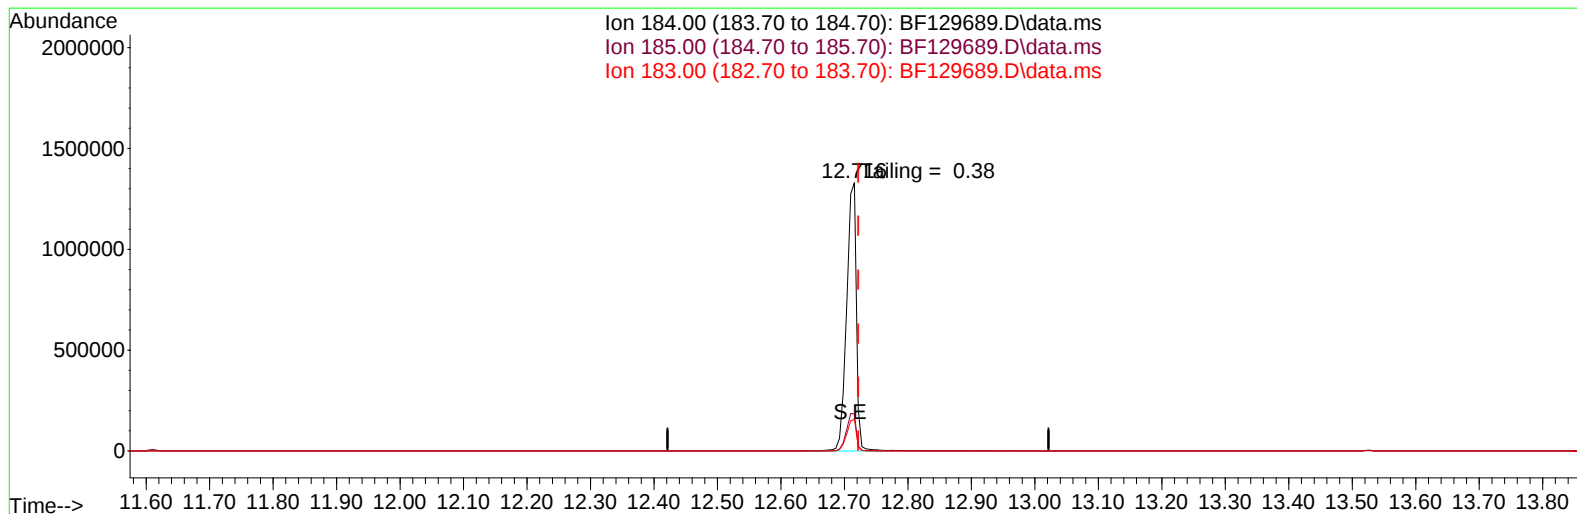

TIC: BF129689.D\data.ms

(77) Benzidine

12.716min (-0.006) 28578.26 ng

response 1430602

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 13.81  |
| 183.00 | 11.60  | 11.74  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/10/2022     | BNA_F            | <u>BF129689.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 821763           | 13.52              |
| DDD           | 9416             | 13.22              |
| DDE           | 2849             | 12.88              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 12265         | 834028           | 1.47               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP