
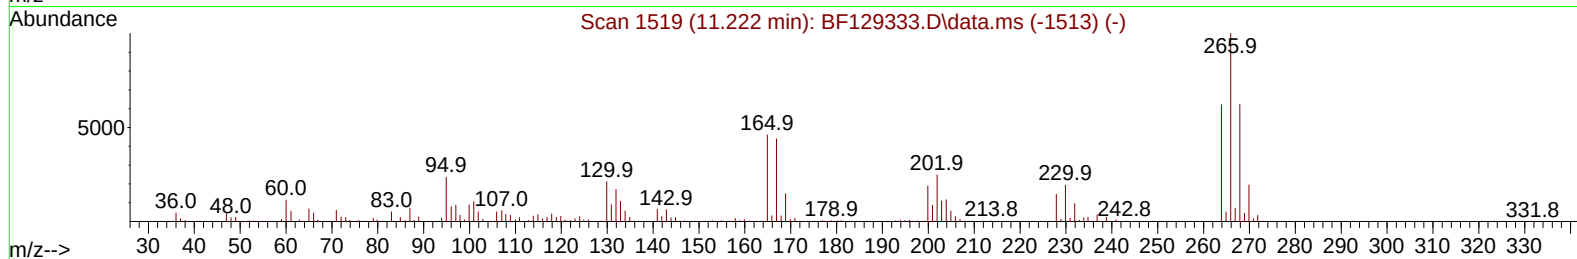
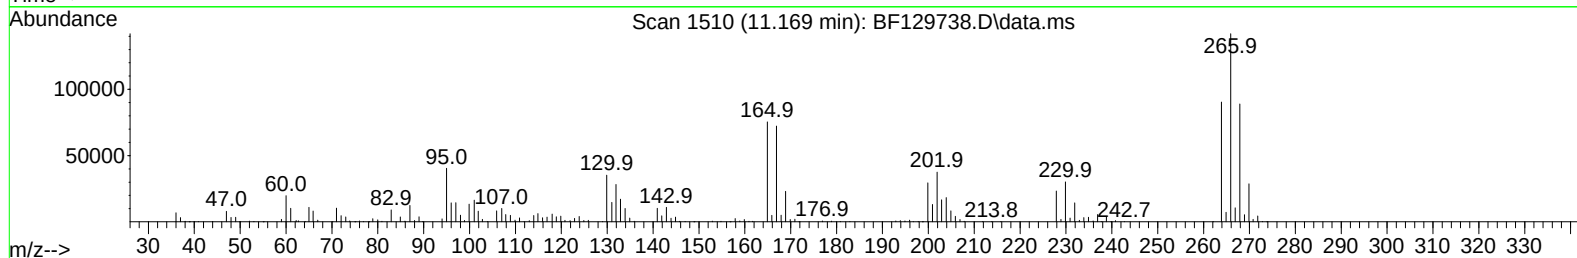


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081222\
Data File : BF129738.D
Acq On : 12 Aug 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 07:44:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 12 15:52:45 2022
Response via : Initial Calibration

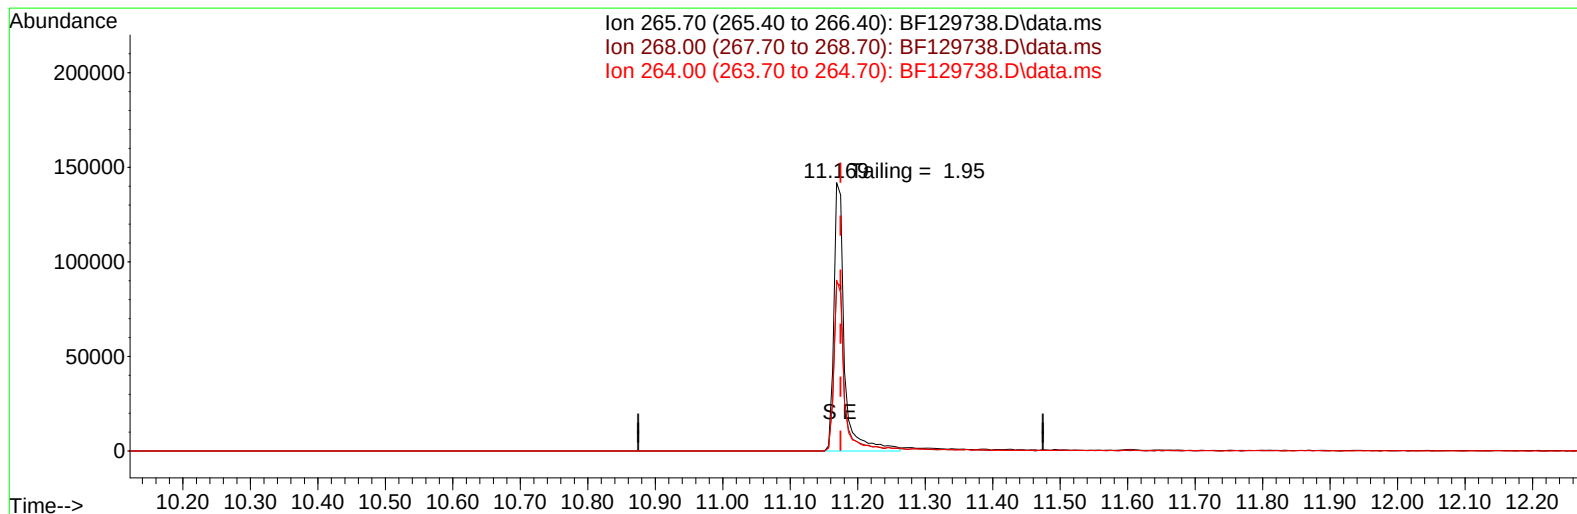

TIC: BF129738.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 138850.93 ng

response 154941

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.65
264.00	61.80	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081222\
Data File : BF129738.D
Acq On : 12 Aug 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 07:41:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 12 15:52:45 2022
Response via : Initial Calibration

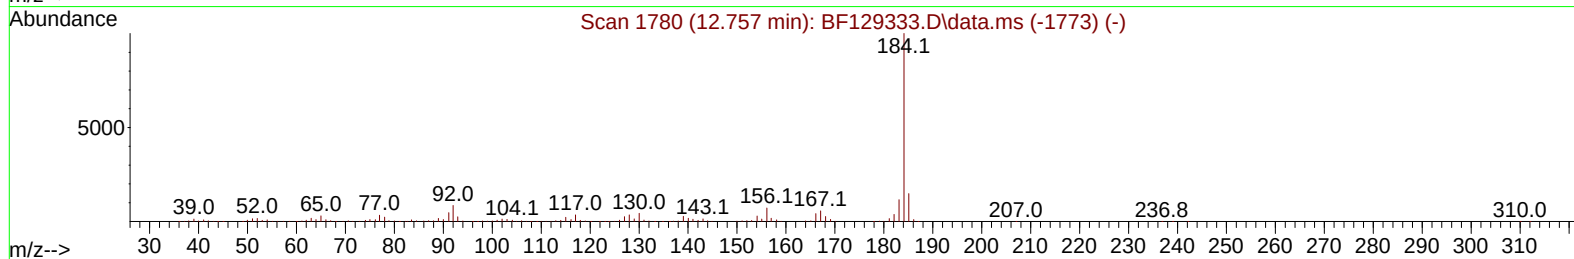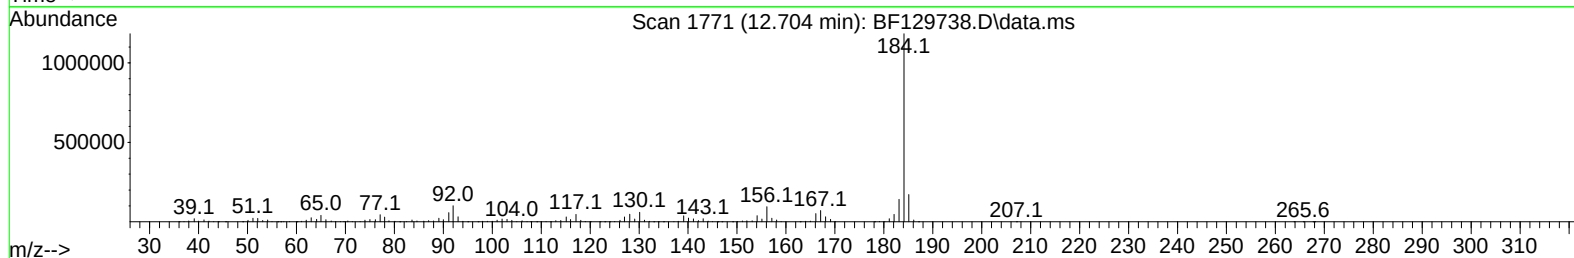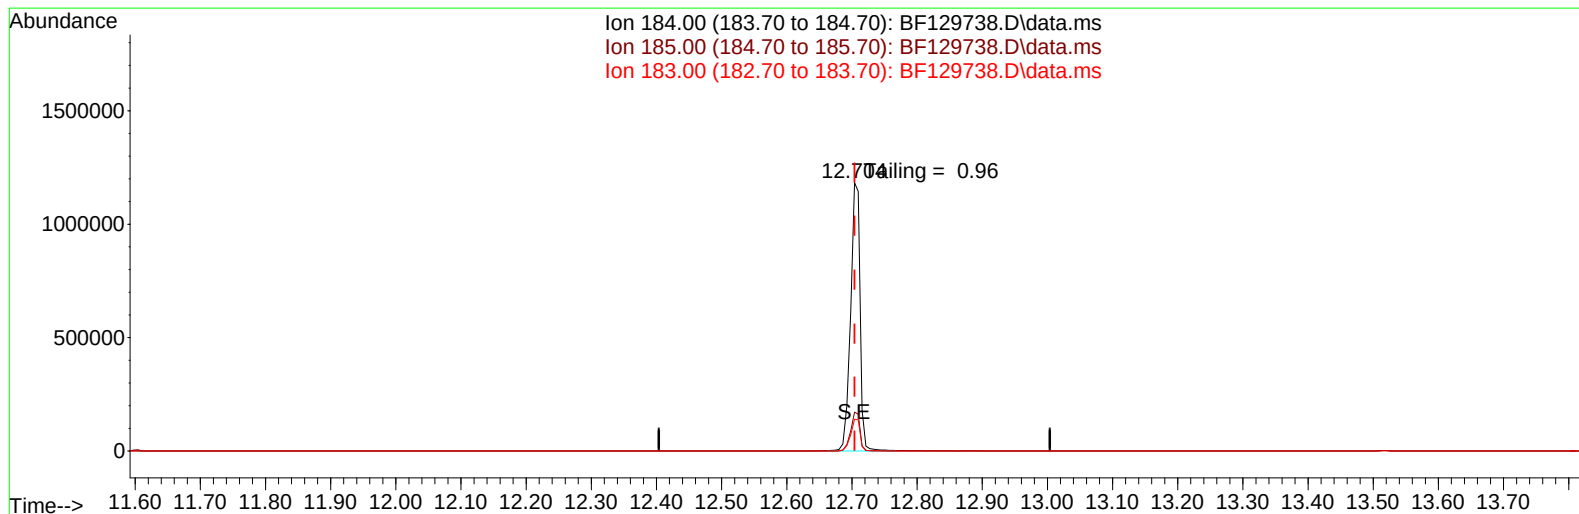

TIC: BF129738.D\data.ms

(77) Benzidine

12.704min (0.000) 45419.96 ng

response 1217872

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.48
183.00	11.60	11.91
0.00	0.00	0.00