


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081222\
 Data File : BF129738.D
 Acq On : 12 Aug 2022 11:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 12 15:52:45 2022

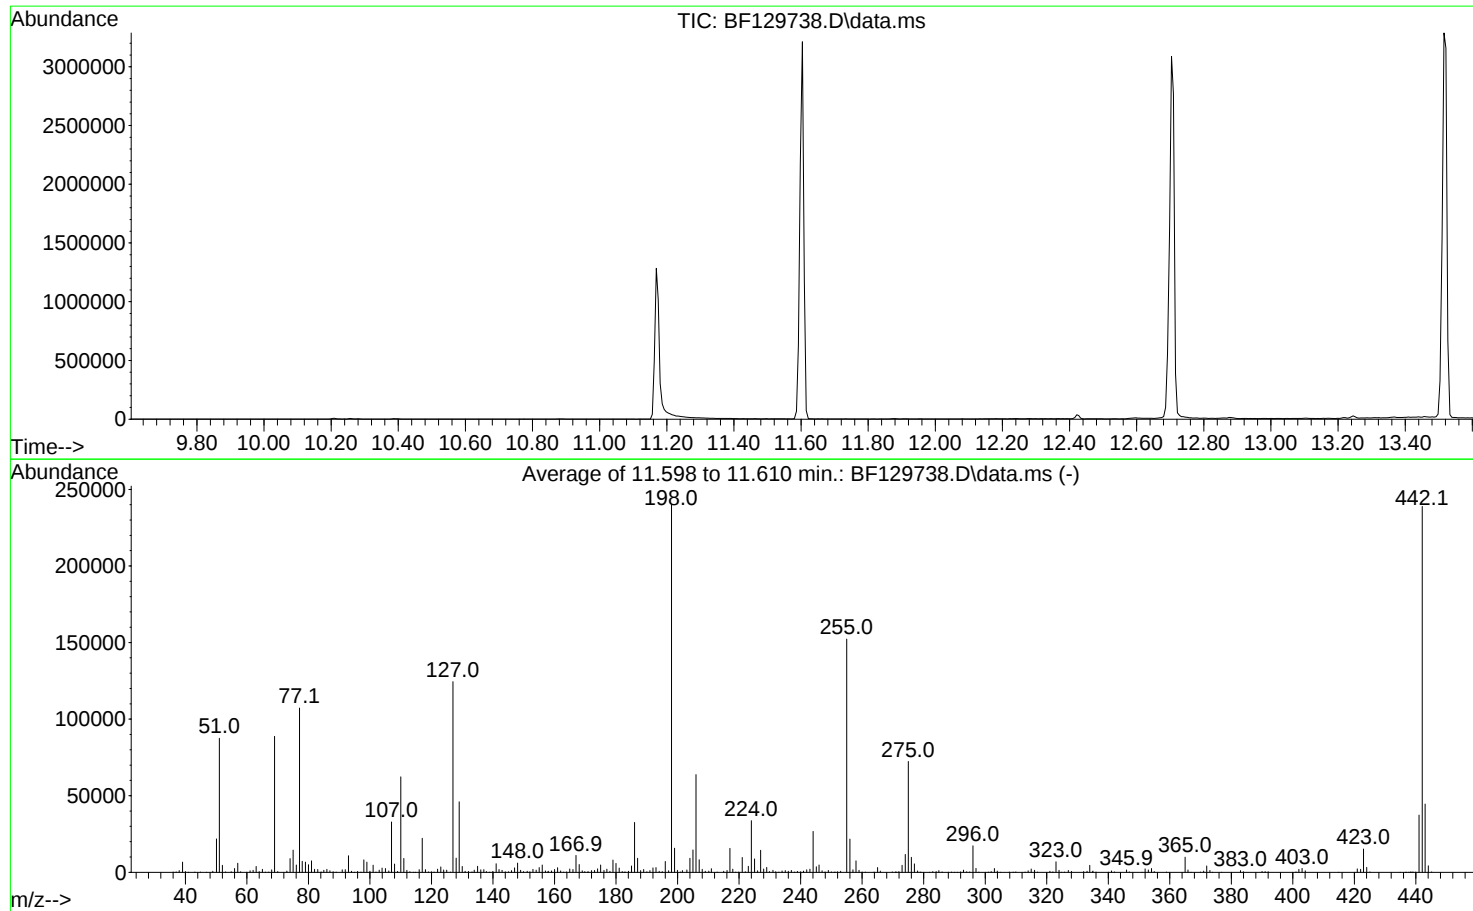




AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	87557	PASS
68	69	0.00	2	1.8	1621	PASS
69	198	0.00	100	37.0	88757	PASS
70	69	0.00	2	0.5	443	PASS
127	198	10	80	51.8	124469	PASS
197	198	0.00	2	0.4	1019	PASS
198	198	100	100	100.0	240192	PASS
199	198	5	9	6.6	15748	PASS
275	198	10	60	30.1	72309	PASS
365	198	1	100	4.1	9870	PASS
441	198	0.01	100	15.5	37339	PASS
442	442	50	100	100.0	238848	PASS
443	442	15	24	18.7	44552	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081222\
Data File : BF129738.D
Acq On : 12 Aug 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 07:44:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 12 15:52:45 2022
Response via : Initial Calibration

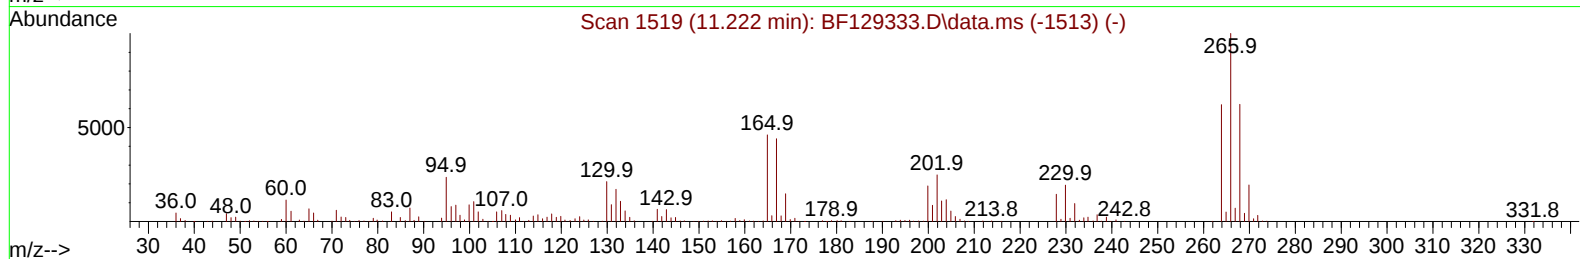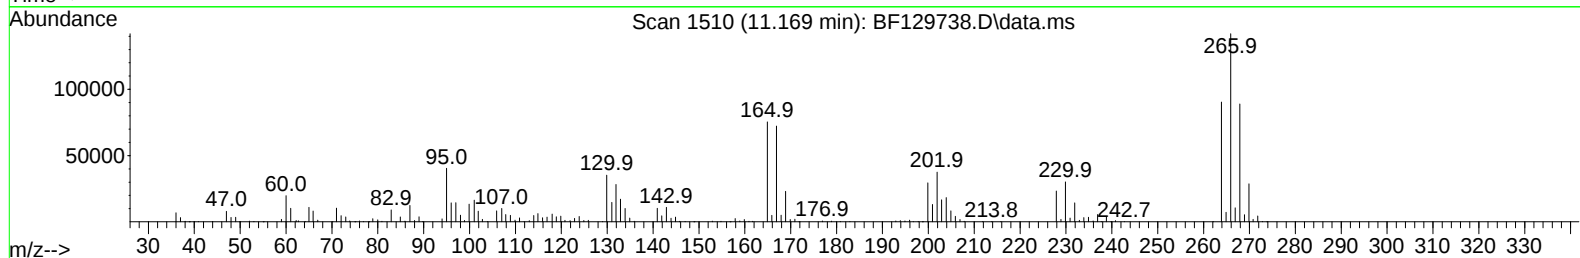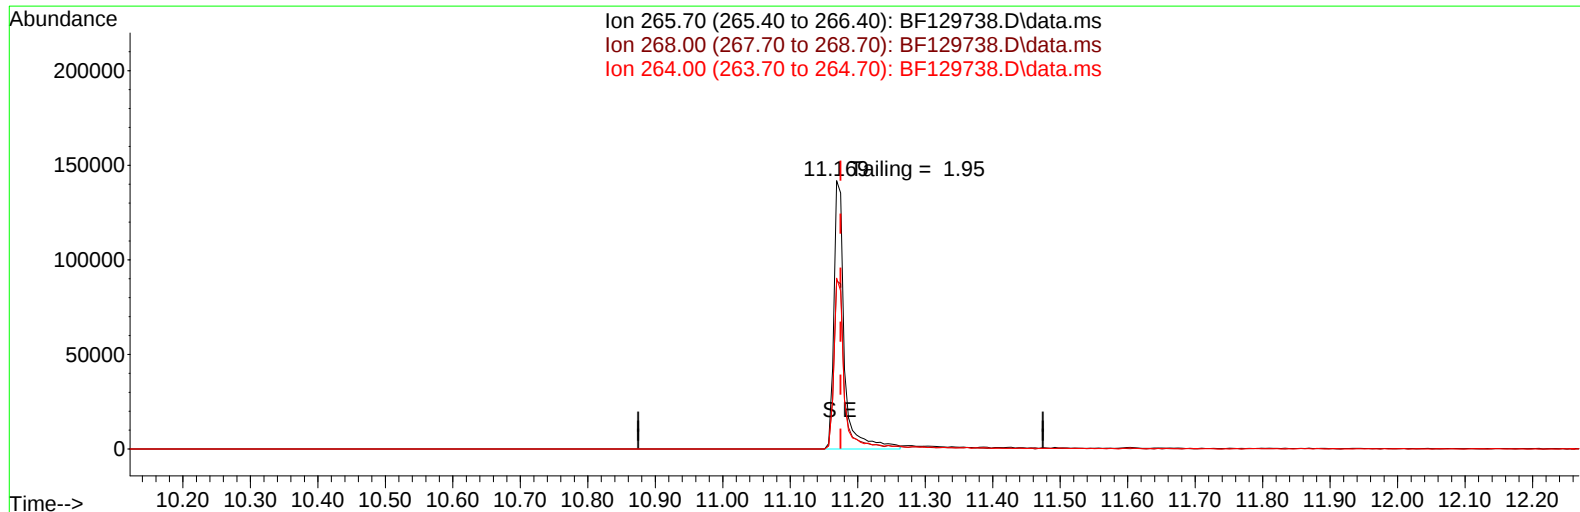

TIC: BF129738.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 138850.93 ng




response 154941

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.65
264.00	61.80	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081222\
Data File : BF129738.D
Acq On : 12 Aug 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 07:41:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 12 15:52:45 2022
Response via : Initial Calibration

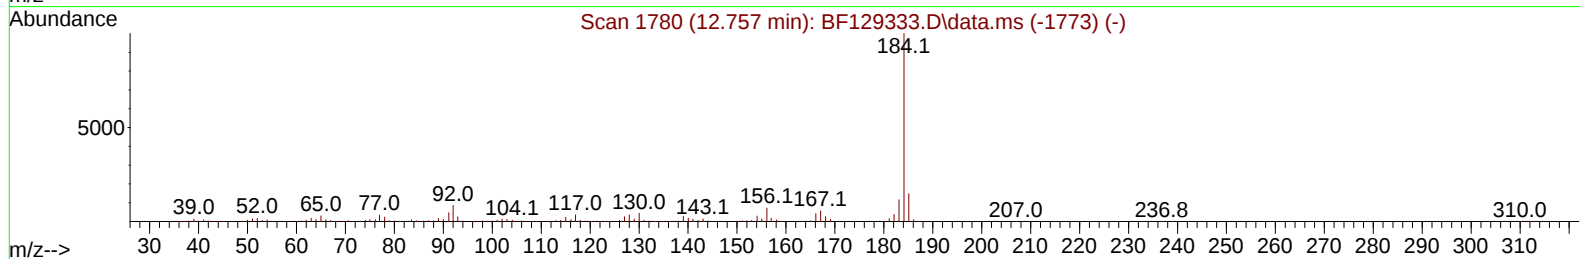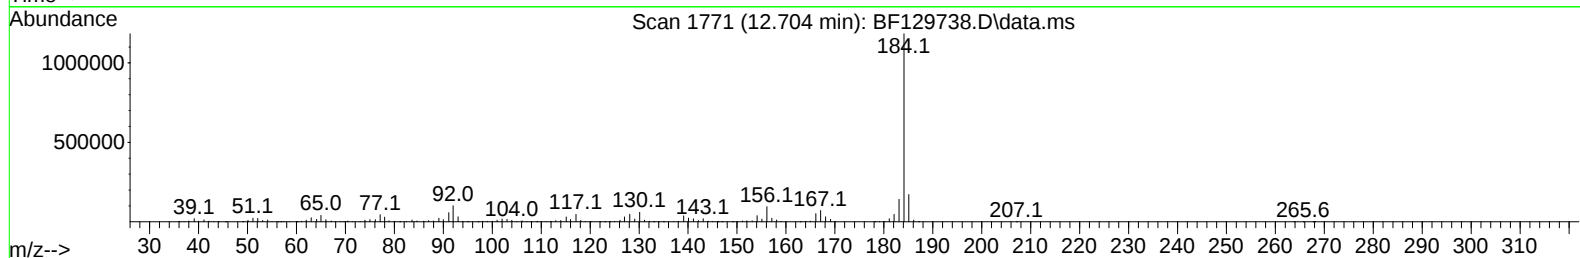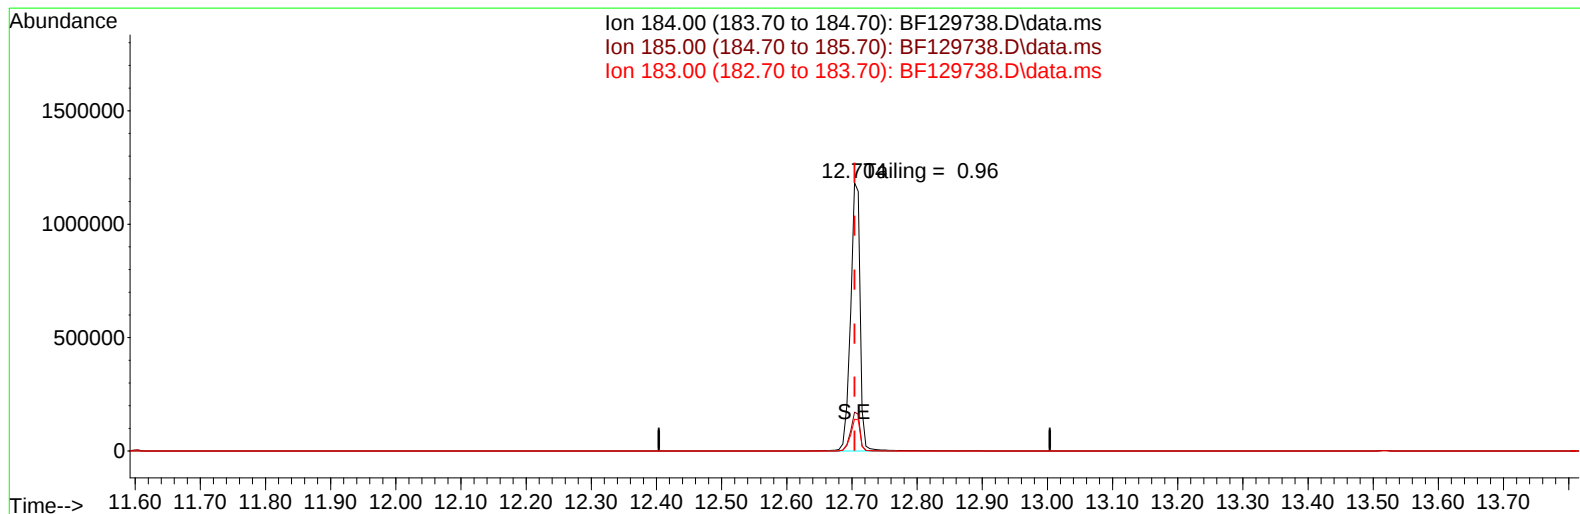

TIC: BF129738.D\data.ms

(77) Benzidine

12.704min (0.000) 45419.96 ng

response 1217872

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.48
183.00	11.60	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/12/2022	BNA_F	<u>BF129738.D</u>
Compound Name	Response	Retention Time
DDT	607761	13.521
DDD	5177	13.245
DDE	1517	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6694	614455	1.09

Instrument :
BNA_F
ClientSampleId :
DFTPP