
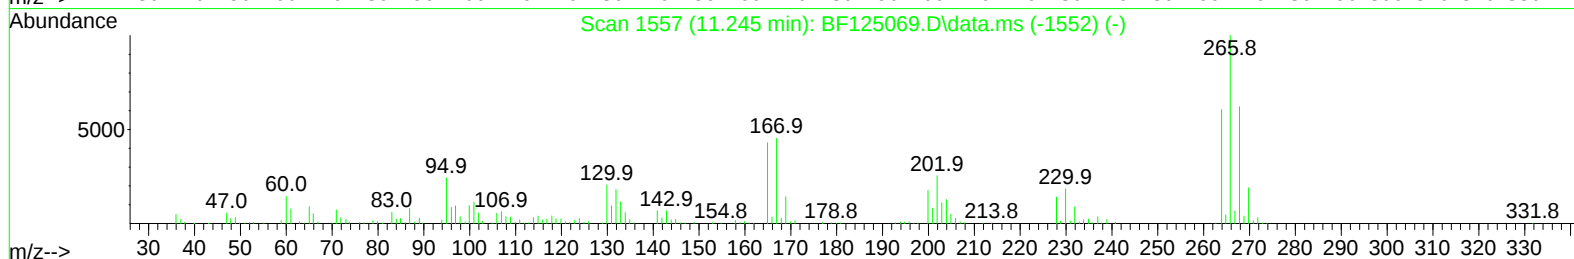
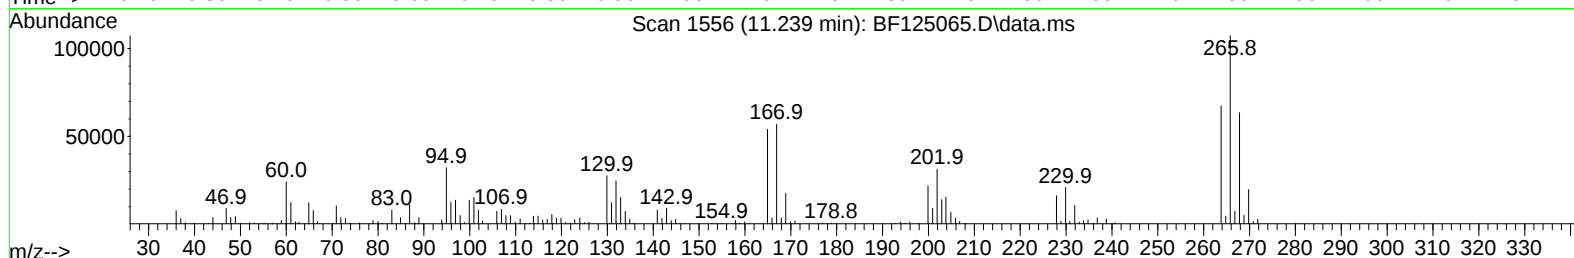


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081721\
Data File : BF125065.D
Acq On : 17 Aug 2021 11:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 17:24:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 17 16:45:36 2021
Response via : Initial Calibration

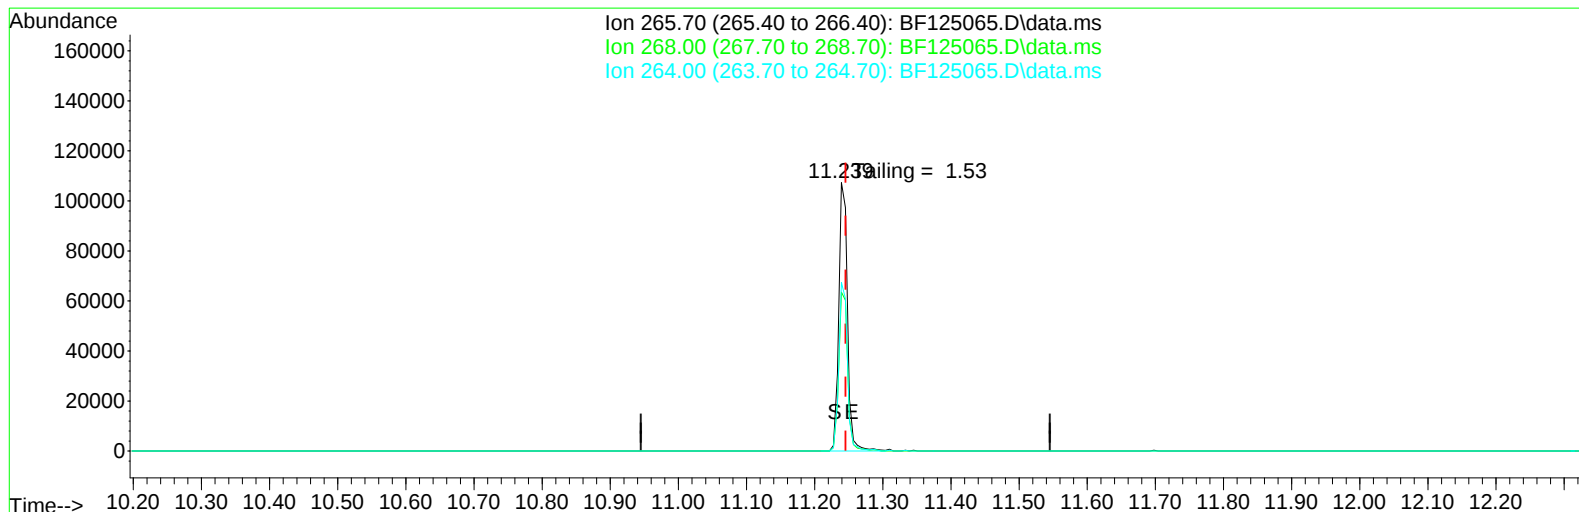

TIC: BF125065.D\data.ms

(70) Pentachlorophenol (C)




11.239min (-0.006) 39036.28 ng

response 95723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	59.22
264.00	69.90	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081721\
Data File : BF125065.D
Acq On : 17 Aug 2021 11:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 17:24:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 17 16:45:36 2021
Response via : Initial Calibration

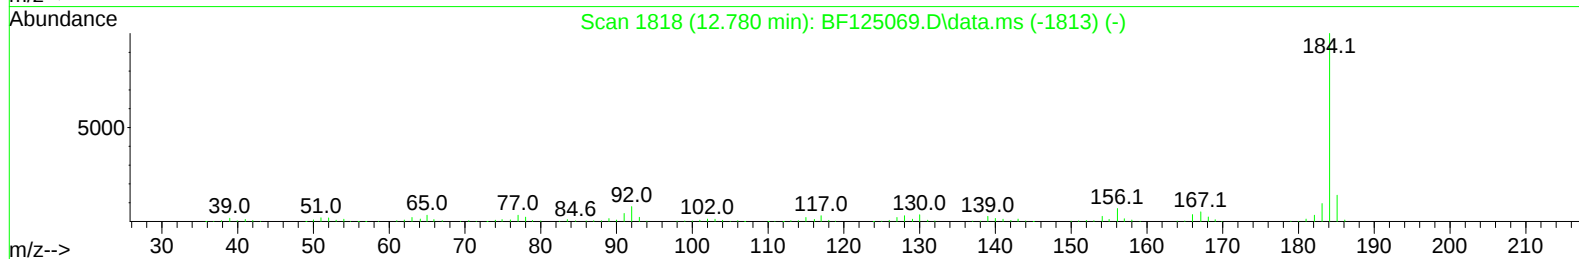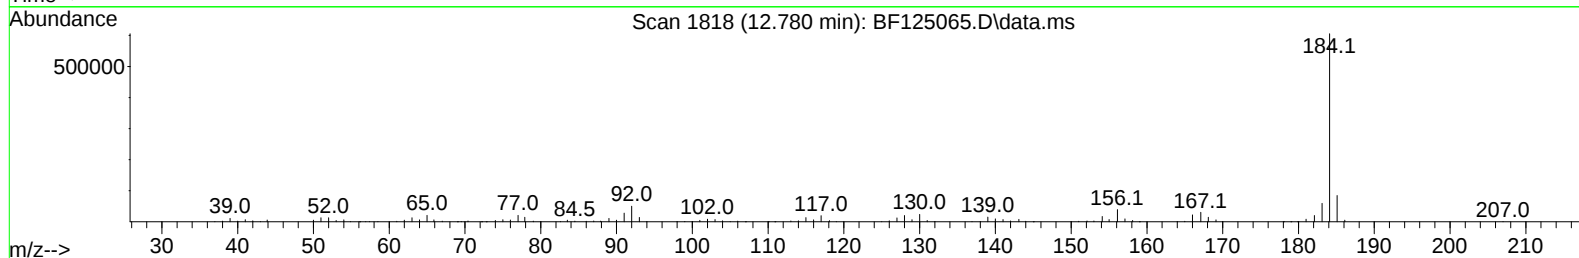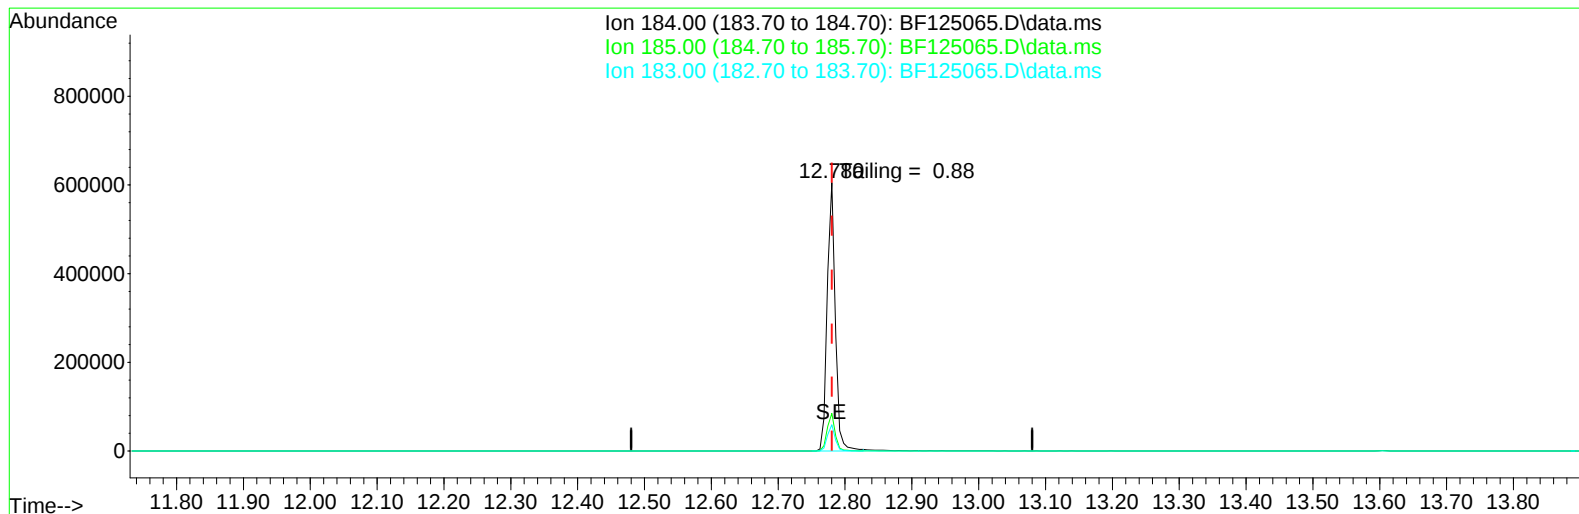

TIC: BF125065.D\data.ms

(77) Benzidine

12.780min (-0.000) 0.00 ng

response 514018

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.00
183.00	10.10	9.82
0.00	0.00	0.00