

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081721\
 Data File : BF125075.D
 Acq On : 17 Aug 2021 18:55
 Operator : JU/CG
 Sample : M3428-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-01-COMP

Quant Time: Aug 18 05:01:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 17 16:45:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.916	152	167183	20.000	ng	0.00
21) Naphthalene-d8	8.204	136	640494	20.000	ng	# 0.00
39) Acenaphthene-d10	9.957	164	303538	20.000	ng	0.00
64) Phenanthrene-d10	11.445	188	566136	20.000	ng	0.00
76) Chrysene-d12	14.080	240	414057	20.000	ng	0.00
86) Perylene-d12	15.574	264	275770	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.534	112	1008587	90.127	ng	0.00
7) Phenol-d6	6.534	99	1221376	88.731	ng	0.00
23) Nitrobenzene-d5	7.481	82	809193	69.901	ng	0.00
42) 2,4,6-Tribromophenol	10.745	330	307724	108.587	ng	0.00
45) 2-Fluorobiphenyl	9.281	172	1263643	55.489	ng	0.00
79) Terphenyl-d14	13.033	244	1425582	49.576	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081721\
Data File : BF125075.D
Acq On : 17 Aug 2021 18:55
Operator : JU/CG
Sample : M3428-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-01-COMP

Quant Time: Aug 18 05:01:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 17 16:45:36 2021
Response via : Initial Calibration




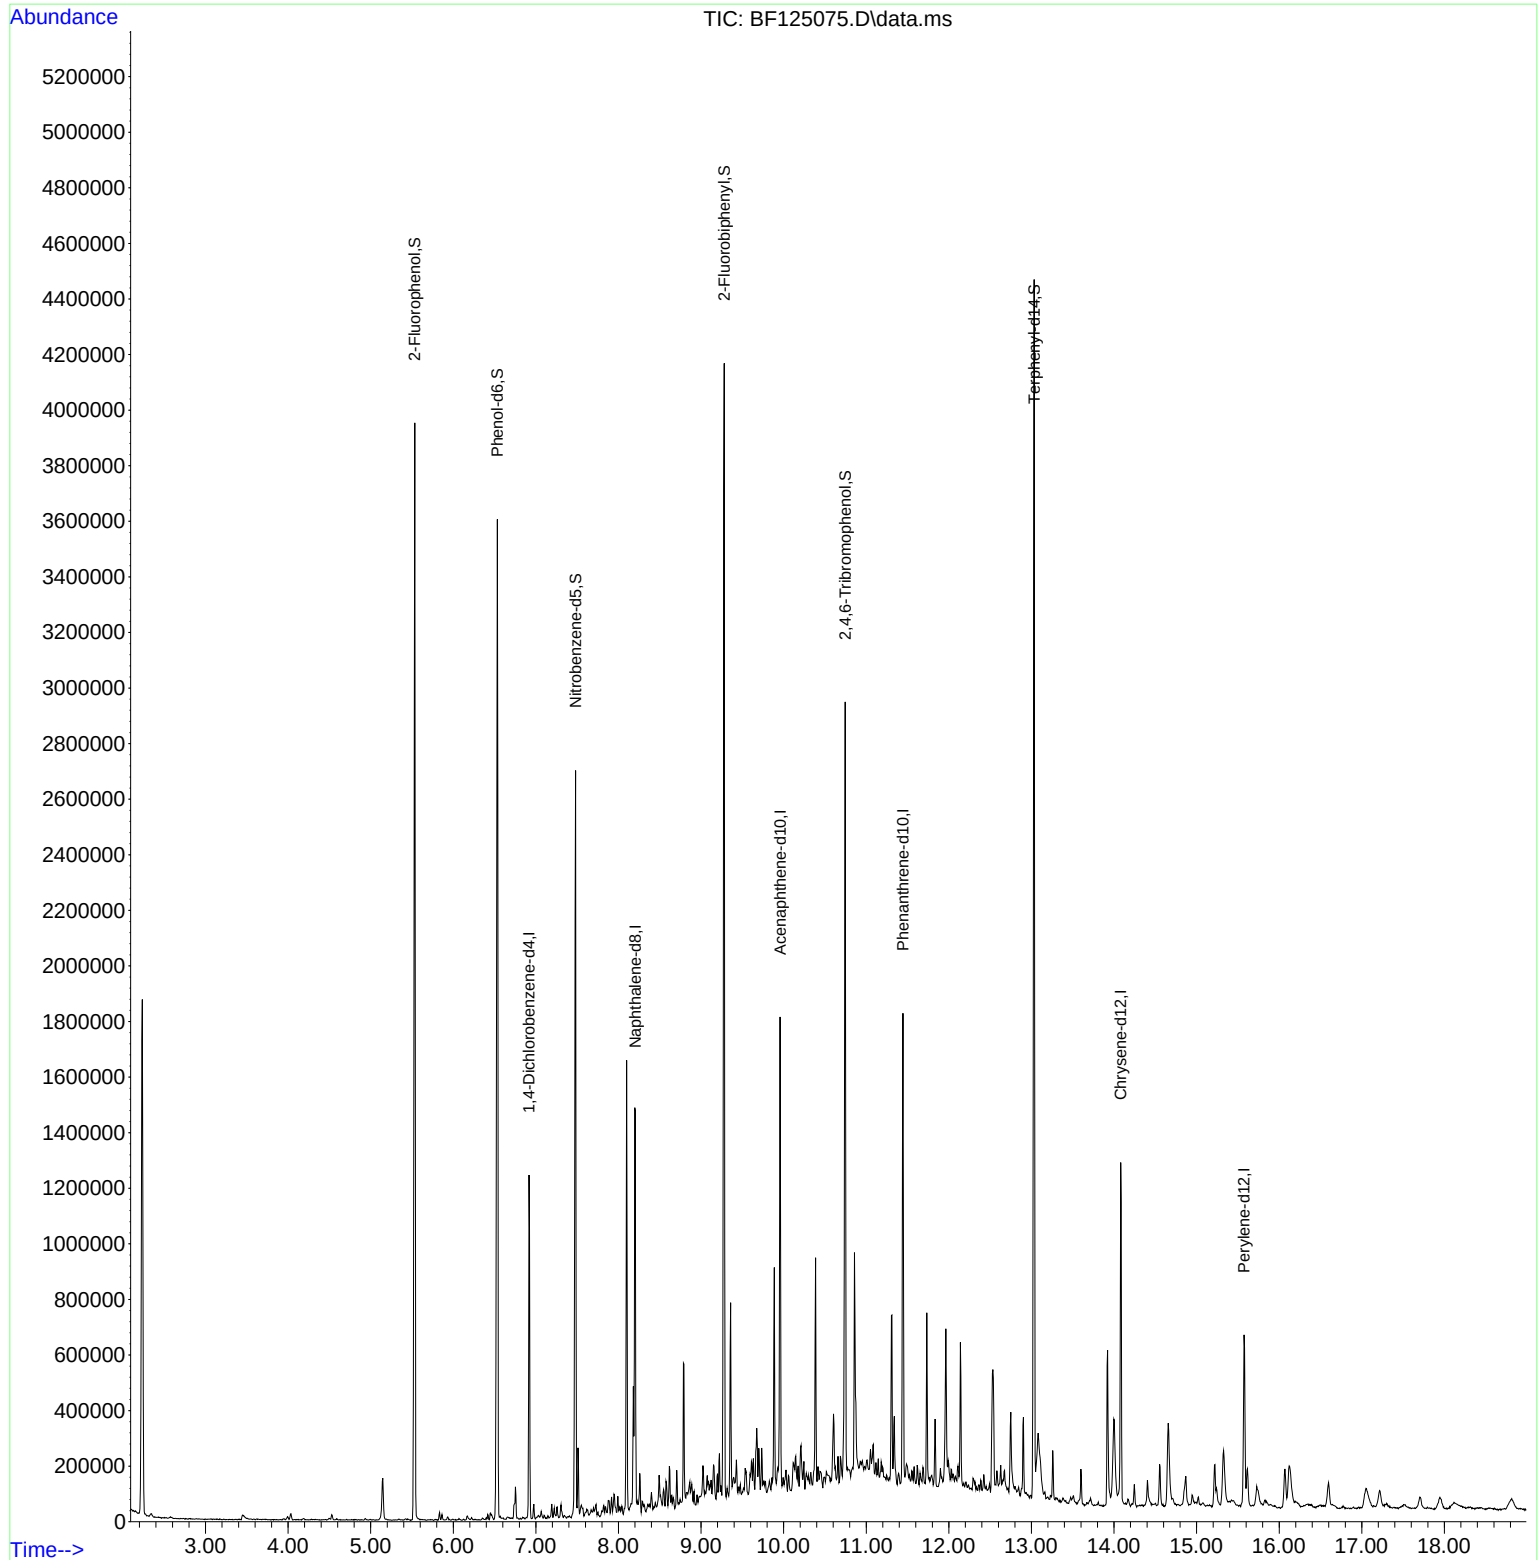




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.916 min Scan# 821
Delta R.T. -0.006 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55




Instrument :
BNA_F
ClientSampleId :
SB-01-COMP


Tgt Ion:152 Resp: 167183
Ion Ratio Lower Upper
152 100
150 157.8 117.6 176.4
115 63.4 47.1 70.7

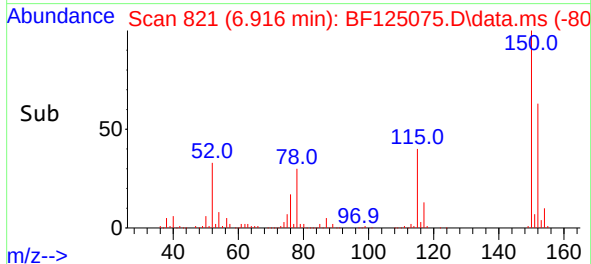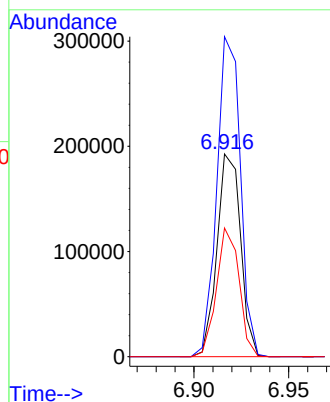

#5
2-Fluorophenol
Concen: 90.127 ng
RT: 5.534 min Scan# 586
Delta R.T. 0.000 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55

Tgt Ion:112 Resp: 1008587
Ion Ratio Lower Upper
112 100
64 70.0 44.2 66.2#
63 37.5 26.2 39.2


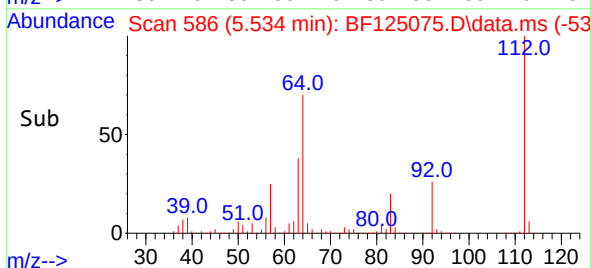
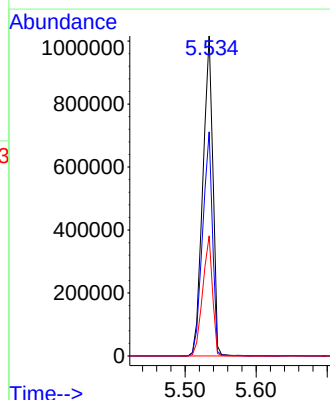
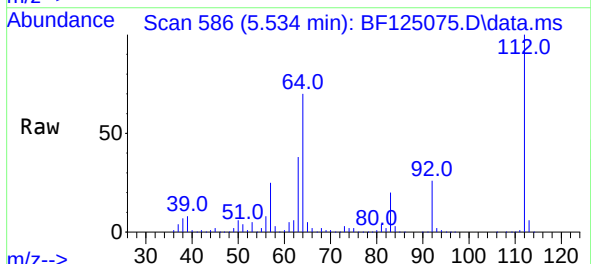




#7
Phenol-d6
Concen: 88.731 ng
RT: 6.534 min Scan# 756
Delta R.T. -0.006 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55




Instrument :
BNA_F
ClientSampleId :
SB-01-COMP


Tgt Ion: 99 Resp: 1221376
Ion Ratio Lower Upper
99 100
42 26.2 23.5 35.3
71 39.2 25.6 38.4#

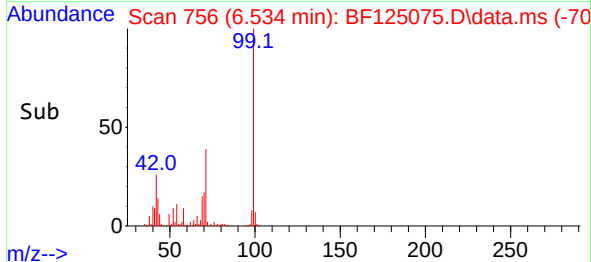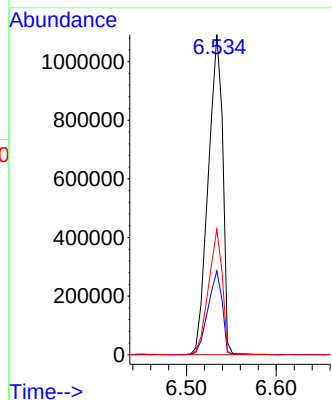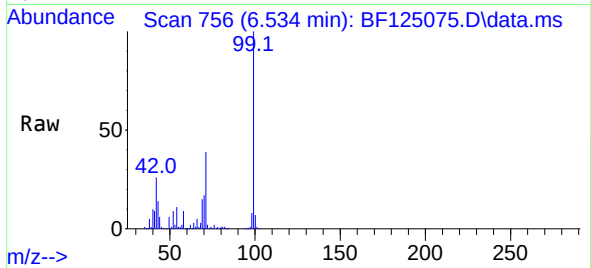

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.204 min Scan# 1040
Delta R.T. 0.000 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55

Tgt Ion: 136 Resp: 640494
Ion Ratio Lower Upper
136 100
137 10.6 9.8 14.6
54 9.9 6.4 9.6#
68 6.1 3.3 4.9#


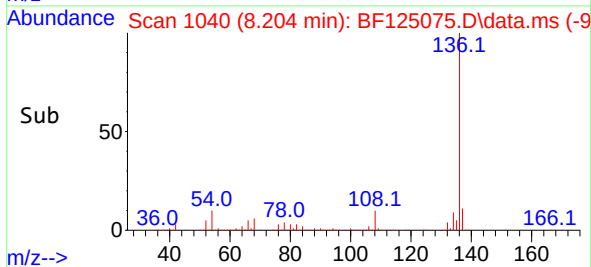
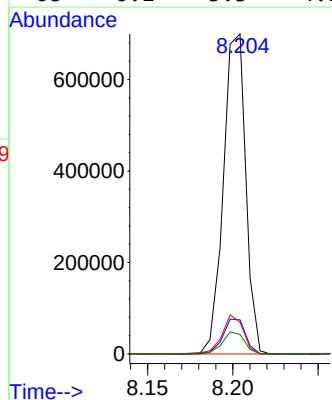
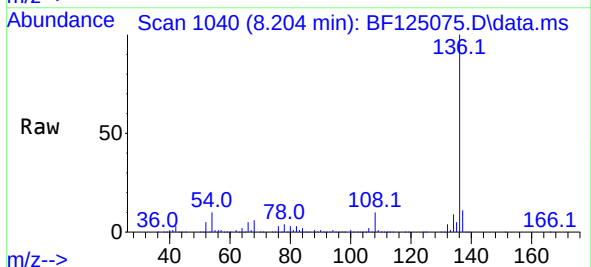




#23
Nitrobenzene-d5
Concen: 69.901 ng
RT: 7.481 min Scan# 917
Delta R.T. -0.006 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55




Instrument :
BNA_F
ClientSampleId :
SB-01-COMP


Tgt Ion: 82 Resp: 809193
Ion Ratio Lower Upper
82 100
128 40.7 40.6 60.8
54 66.6 49.6 74.4

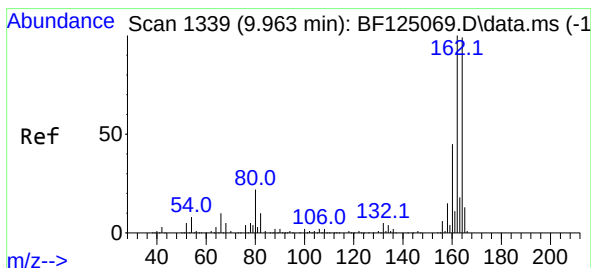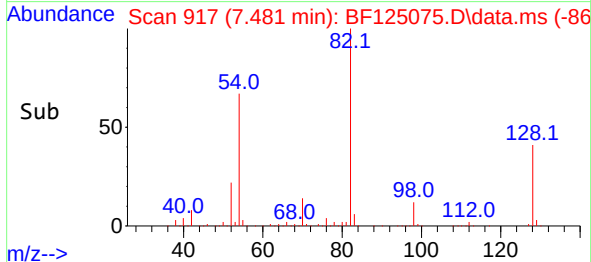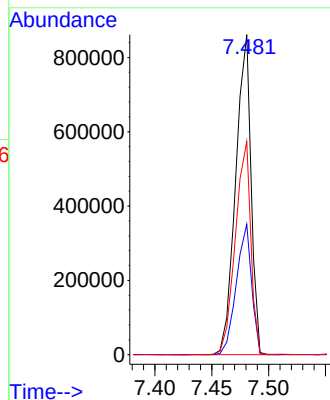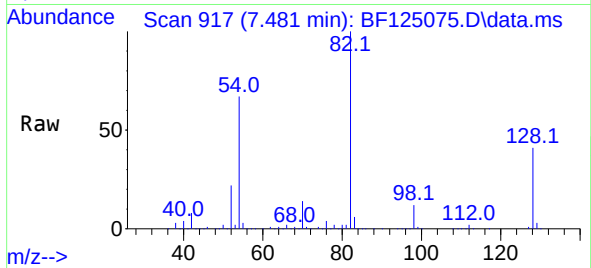

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.957 min Scan# 1338
Delta R.T. -0.006 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55

Tgt Ion:164 Resp: 303538
Ion Ratio Lower Upper
164 100
162 102.9 81.3 121.9
160 47.0 38.0 57.0


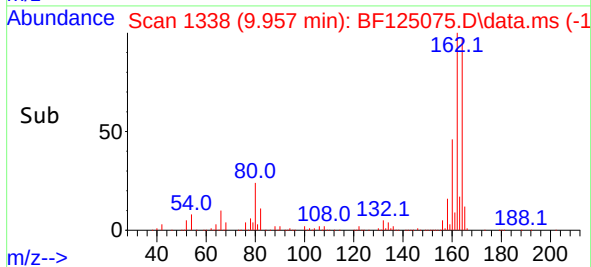
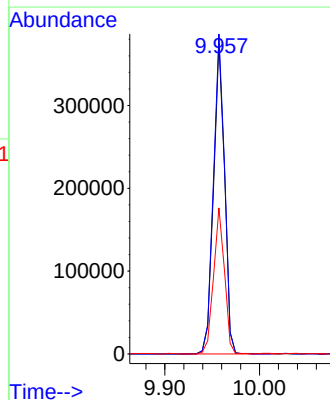
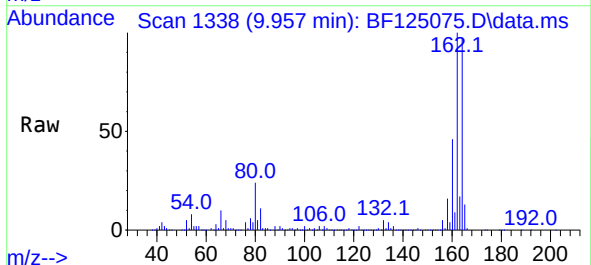




#42
2,4,6-Tribromophenol
Concen: 108.587 ng
RT: 10.745 min Scan# 1472
Delta R.T. -0.006 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55




Instrument :
BNA_F
ClientSampleId :
SB-01-COMP


Tgt Ion: 330 Resp: 307724
Ion Ratio Lower Upper
330 100
332 95.3 76.2 114.4
141 34.8 44.6 66.8#

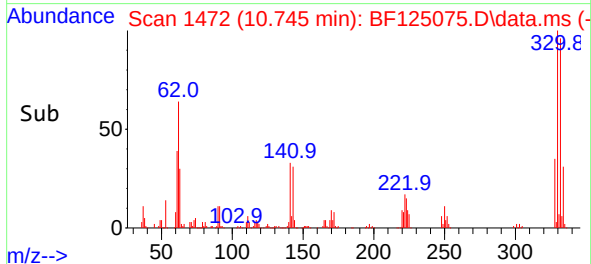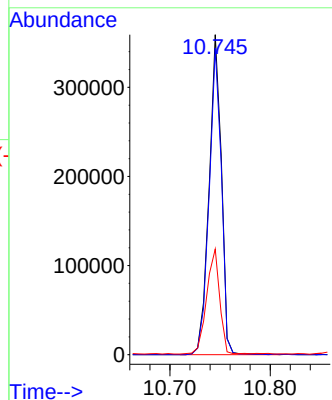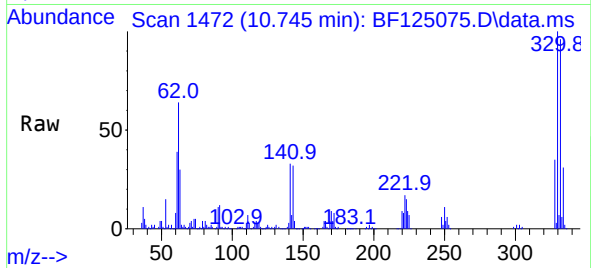

#45
2-Fluorobiphenyl
Concen: 55.489 ng
RT: 9.281 min Scan# 1223
Delta R.T. 0.000 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55

Tgt Ion: 172 Resp: 1263643
Ion Ratio Lower Upper
172 100
171 35.6 26.5 39.7
170 24.4 18.8 28.2


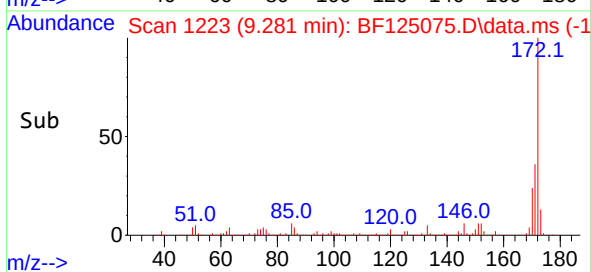
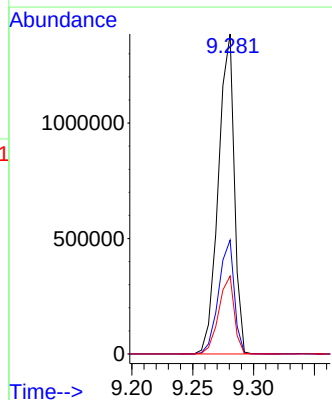





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.445 min Scan# 1591
Delta R.T. 0.000 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55




Instrument :
BNA_F
ClientSampleId :
SB-01-COMP


Tgt Ion:188 Resp: 566136
Ion Ratio Lower Upper
188 100
94 9.8 6.7 10.1
80 10.9 7.5 11.3

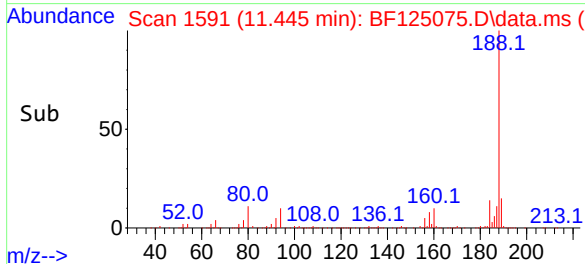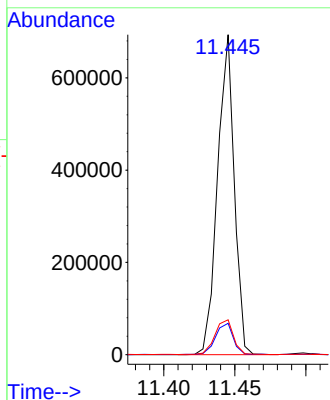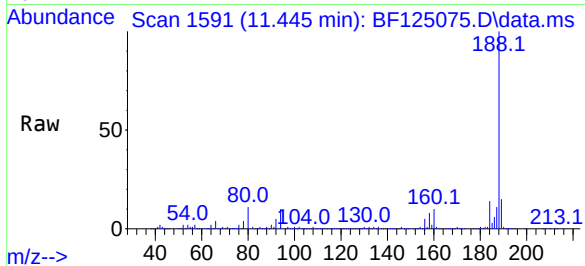

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.080 min Scan# 2039
Delta R.T. -0.006 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55

Tgt Ion:240 Resp: 414057
Ion Ratio Lower Upper
240 100
120 13.6 10.8 16.2
236 24.4 21.6 32.4


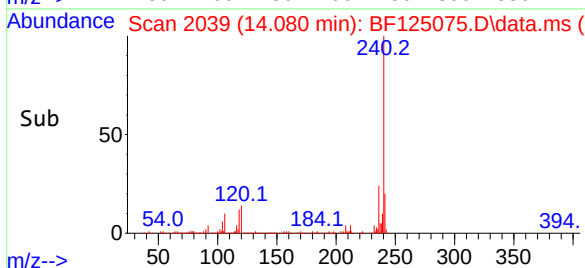
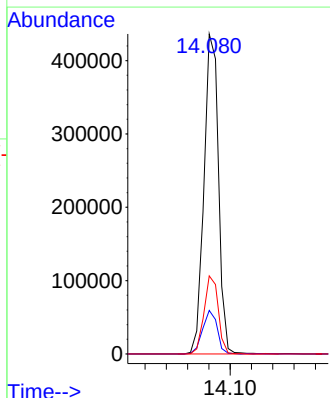
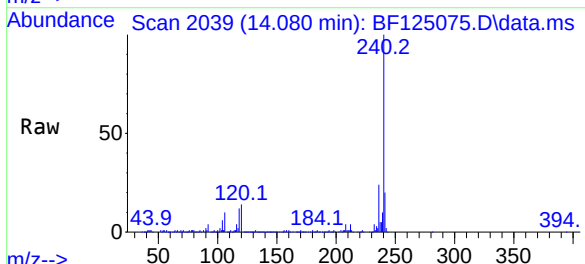




#79
Terphenyl-d14
Concen: 49.576 ng
RT: 13.033 min Scan# 1861
Delta R.T. 0.000 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55

Instrument :
BNA_F
ClientSampleId :
SB-01-COMP

Tgt Ion:244 Resp: 1425582
Ion Ratio Lower Upper
244 100
212 6.8 5.9 8.9
122 10.3 9.0 13.4

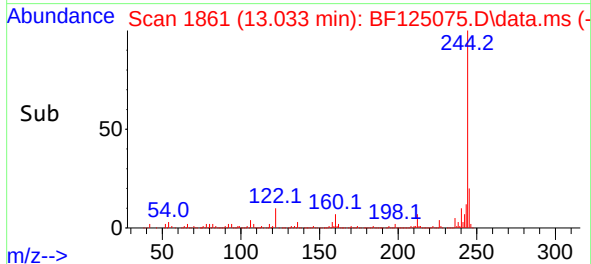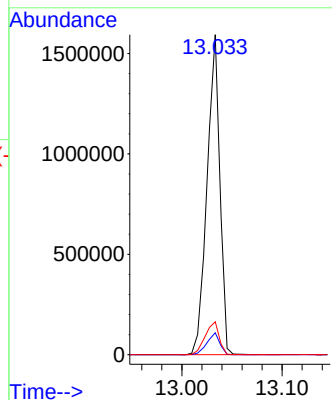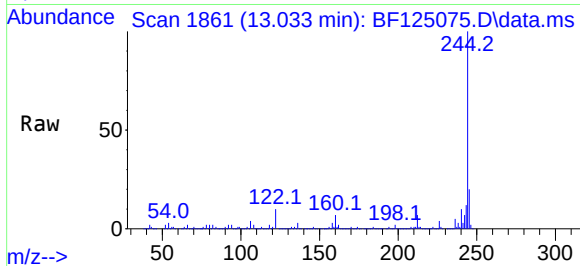

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.574 min Scan# 2293
Delta R.T. -0.006 min
Lab File: BF125075.D
Acq: 17 Aug 2021 18:55

Tgt Ion:264 Resp: 275770
Ion Ratio Lower Upper
264 100
260 25.1 19.6 29.4
265 21.9 17.2 25.8

