
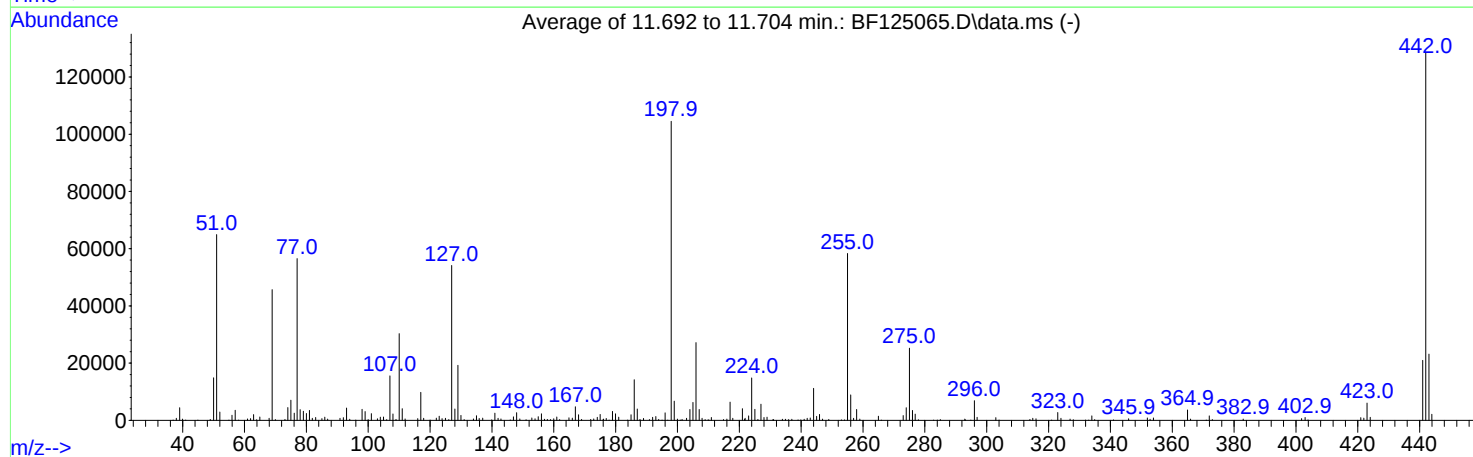


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081721\
 Data File : BF125065.D
 Acq On : 17 Aug 2021 11:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 17 16:45:36 2021

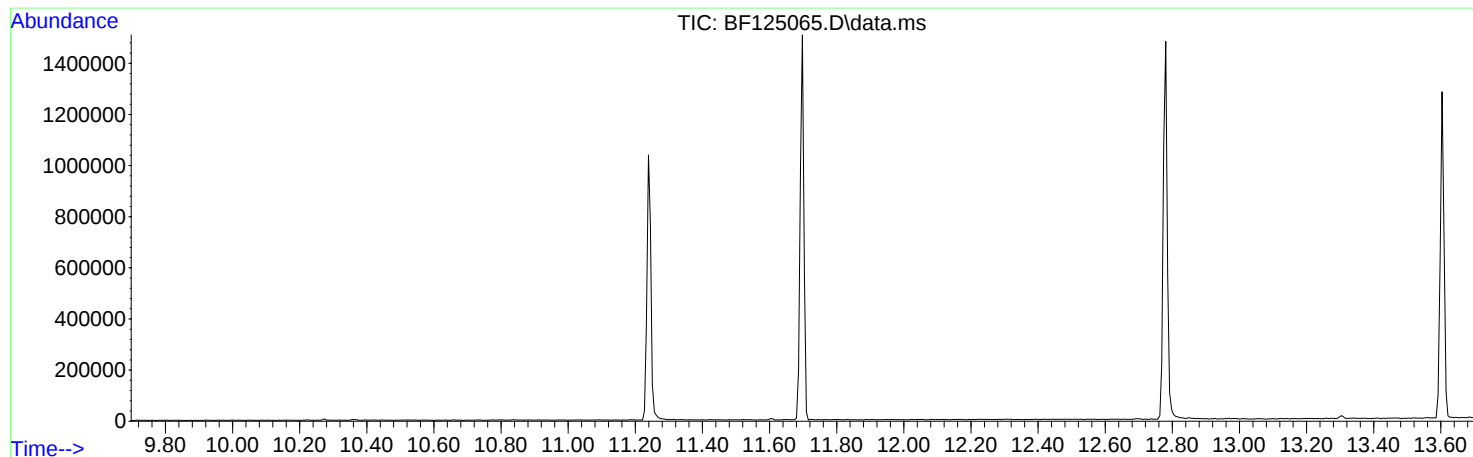




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.1	64931	PASS
68	69	0.00	2	1.7	758	PASS
69	198	0.00	100	43.7	45699	PASS
70	69	0.00	2	0.6	278	PASS
127	198	10	80	51.8	54104	PASS
197	198	0.00	2	0.1	112	PASS
198	198	100	100	100.0	104509	PASS
199	198	5	9	6.4	6733	PASS
275	198	10	60	24.1	25197	PASS
365	198	1	100	3.5	3632	PASS
441	198	0.01	100	20.1	20973	PASS
442	442	50	100	100.0	128555	PASS
443	442	15	24	18.0	23158	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081721\
Data File : BF125065.D
Acq On : 17 Aug 2021 11:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 17:24:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 17 16:45:36 2021
Response via : Initial Calibration

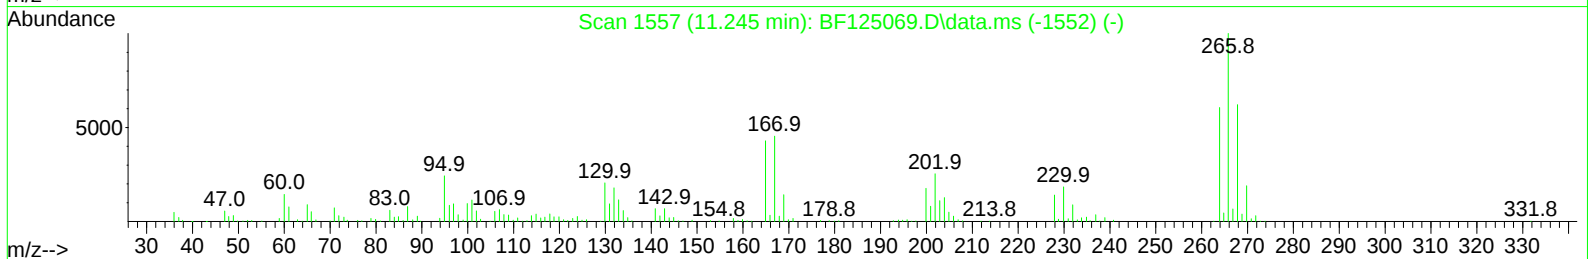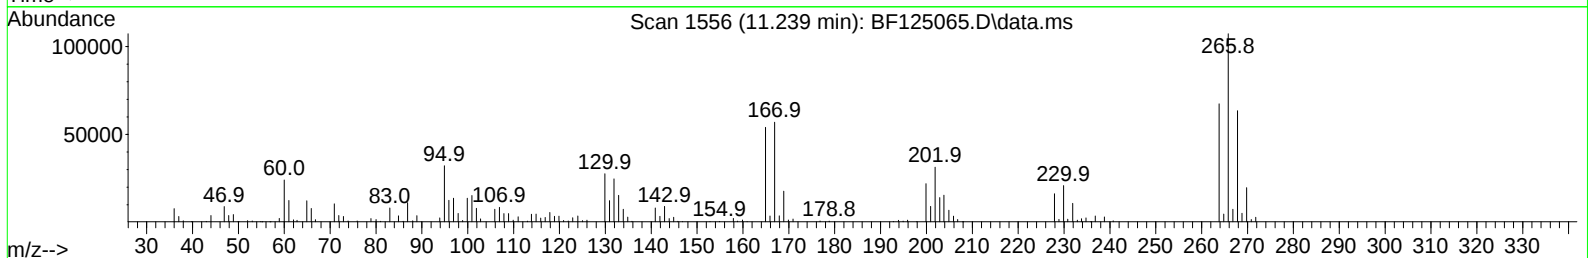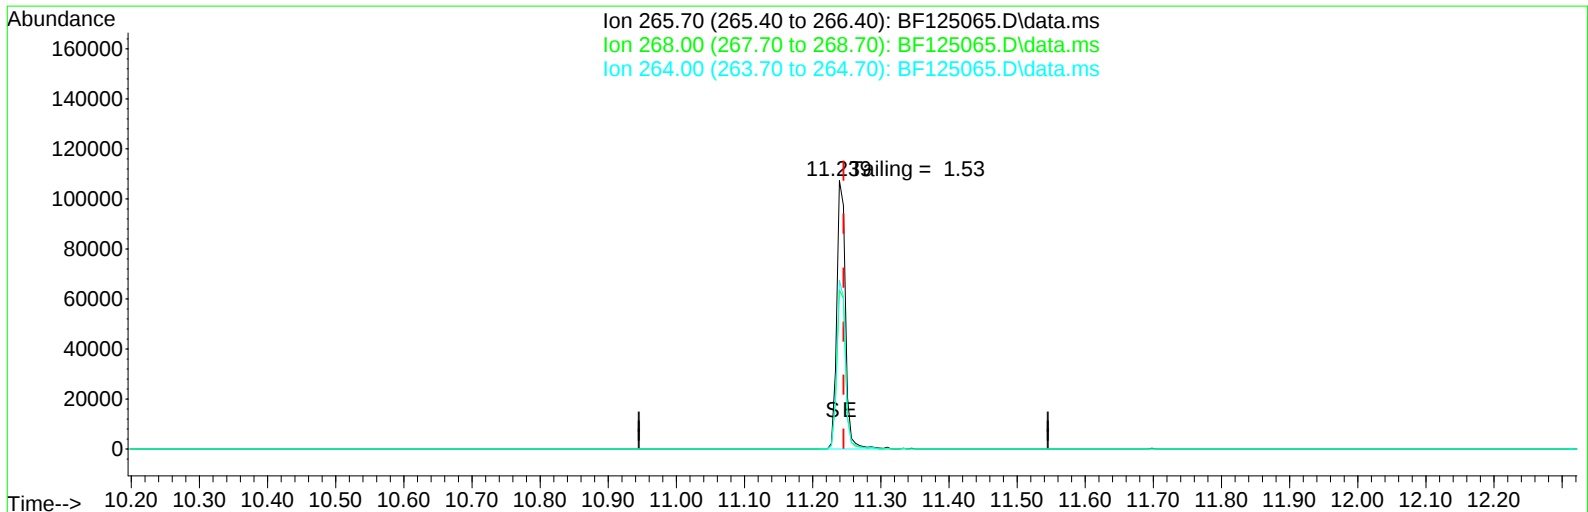

TIC: BF125065.D\data.ms

(70) Pentachlorophenol (C)

11.239min (-0.006) 39036.28 ng




response 95723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	59.22
264.00	69.90	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081721\
Data File : BF125065.D
Acq On : 17 Aug 2021 11:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 17:24:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 17 16:45:36 2021
Response via : Initial Calibration

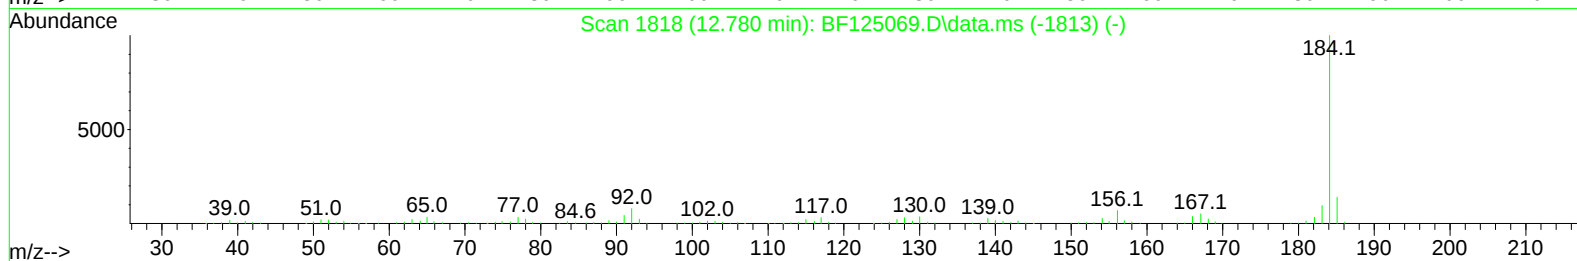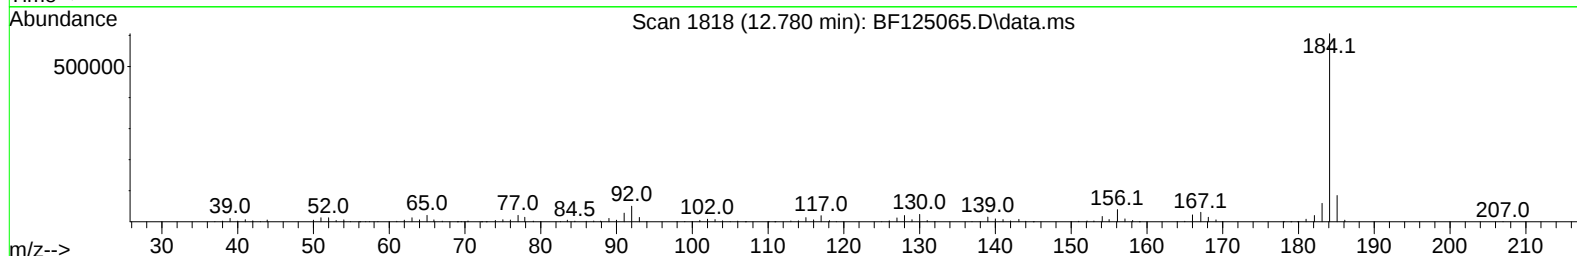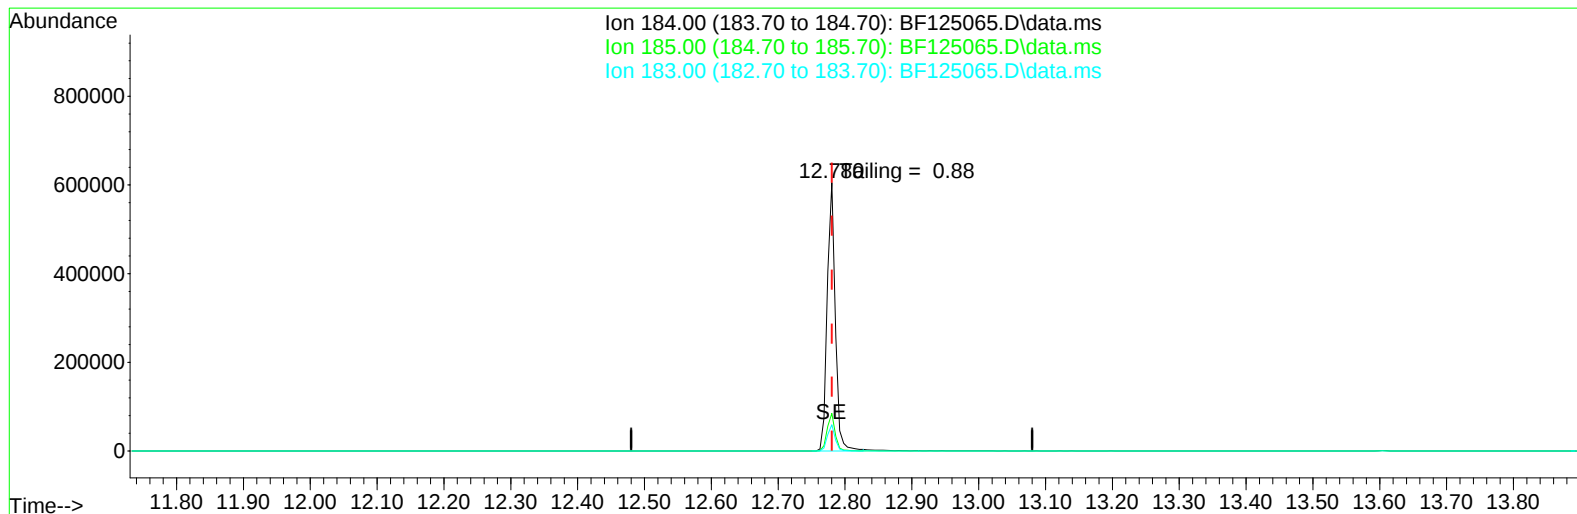

TIC: BF125065.D\data.ms

(77) Benzidine

12.780min (-0.000) 0.00 ng

response 514018

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.00
183.00	10.10	9.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2021	BNA_F	<u>BF125065.D</u>
Compound Name	Response	Retention Time
DDT	164465	13.6
DDD	2472	13.3
DDE	422	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2894	167359	1.73