
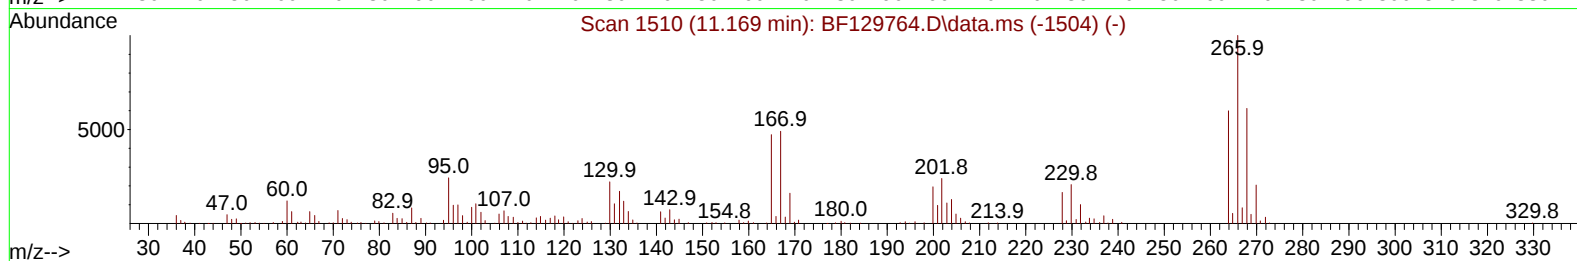
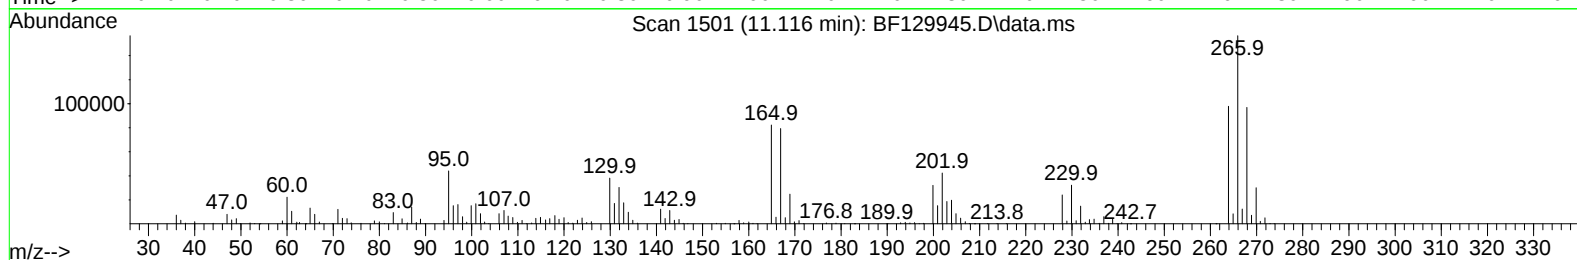


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
Data File : BF129945.D
Acq On : 23 Aug 2022 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 03:32:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 04:41:40 2022
Response via : Initial Calibration

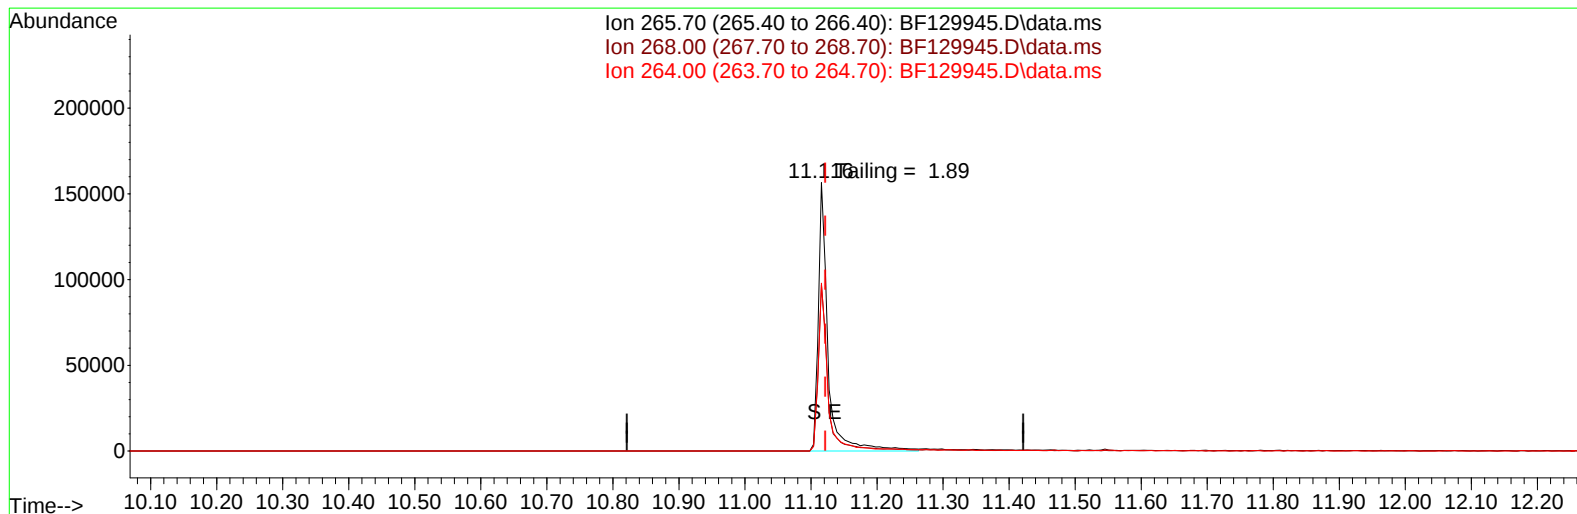

TIC: BF129945.D\data.ms




(70) Pentachlorophenol (C)

11.116min (-0.006) 659787.73 ng

response 160980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.89
264.00	59.90	62.54
0.00	0.00	0.00

Quant Time: Aug 24 03:32:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 04:41:40 2022
Response via : Initial Calibration

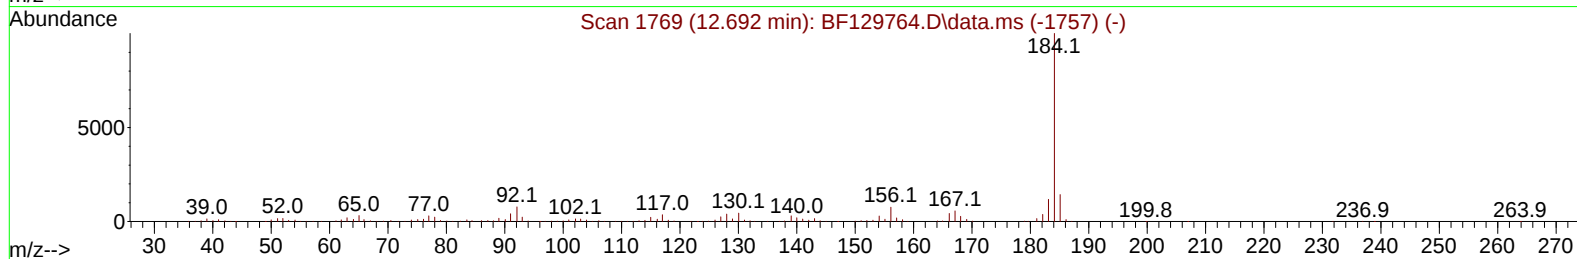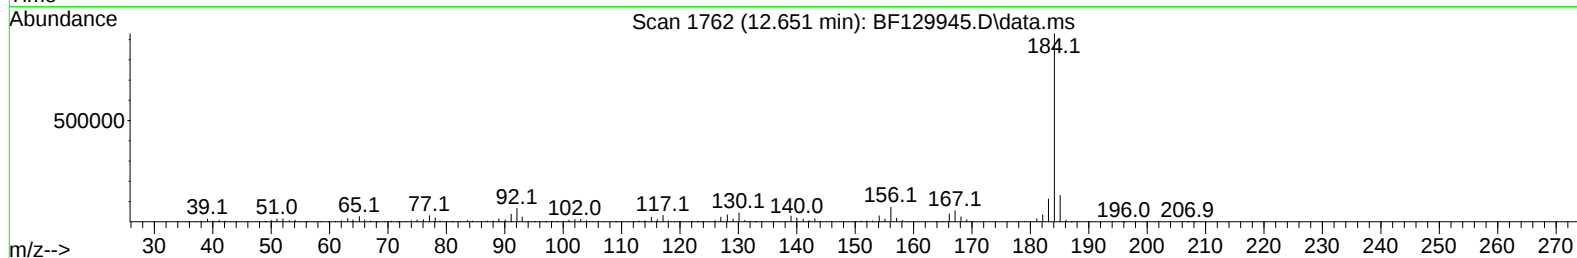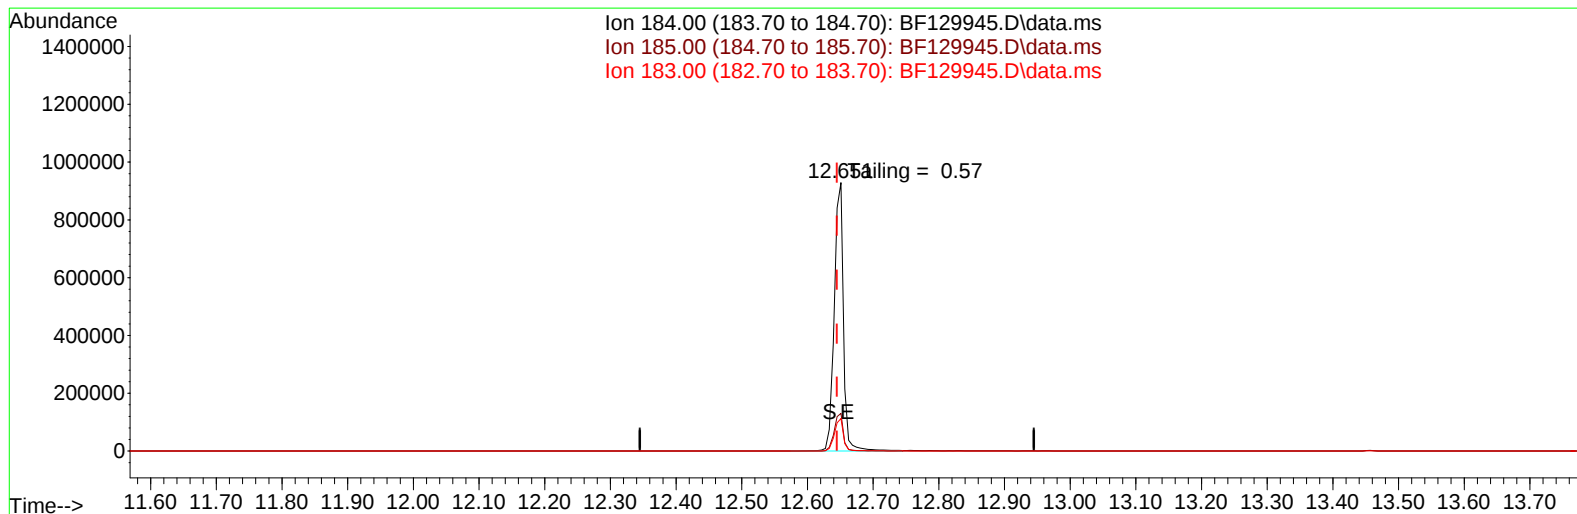

TIC: BF129945.D\data.ms

(77) Benzidine

12.651min (+ 0.006) 174486.16 ng

response 911342

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.06
183.00	11.80	12.09
0.00	0.00	0.00