

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
 Data File : BF129947.D
 Acq On : 23 Aug 2022 10:45
 Operator : CG\JU
 Sample : PB147059BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147059BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	529	532	550	rBV	2758691	2916205	47.06%	9.640%
2	6.434	701	705	725	rBV	2960432	2941375	47.46%	9.724%
3	6.775	759	763	774	rVB	918284	778480	12.56%	2.573%
4	7.345	855	860	863	rBV	2719772	2804486	45.26%	9.271%
5	8.057	976	981	994	rBV	1244152	1133937	18.30%	3.749%
6	9.133	1158	1164	1167	rBV	5862340	5422709	87.51%	17.926%
7	9.810	1274	1279	1283	rBV	1684249	1357108	21.90%	4.486%
8	10.604	1410	1414	1431	rBV	2551757	2407770	38.85%	7.960%
9	11.298	1529	1532	1536	rBV	1602083	1420613	22.92%	4.696%
10	12.892	1797	1803	1806	rBV	6295026	6196954	100.00%	20.486%
11	13.945	1979	1982	1991	rBV	1327421	1251627	20.20%	4.138%
12	14.033	1991	1997	2002	rBV	116456	135365	2.18%	0.447%
13	15.404	2225	2230	2245	rVB	793210	1059176	17.09%	3.501%
14	15.792	2291	2296	2301	rBV	59255	88527	1.43%	0.293%
15	16.274	2372	2378	2386	rVB	55529	97803	1.58%	0.323%
16	16.668	2433	2445	2458	rBV6	18975	96468	1.56%	0.319%
17	16.833	2468	2473	2483	rVB	39917	78724	1.27%	0.260%
18	17.498	2581	2586	2594	rVB3	29045	62580	1.01%	0.207%




Sum of corrected areas: 30249907

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
Data File : BF129947.D
Acq On : 23 Aug 2022 10:45
Operator : CG\JU
Sample : PB147059BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147059BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

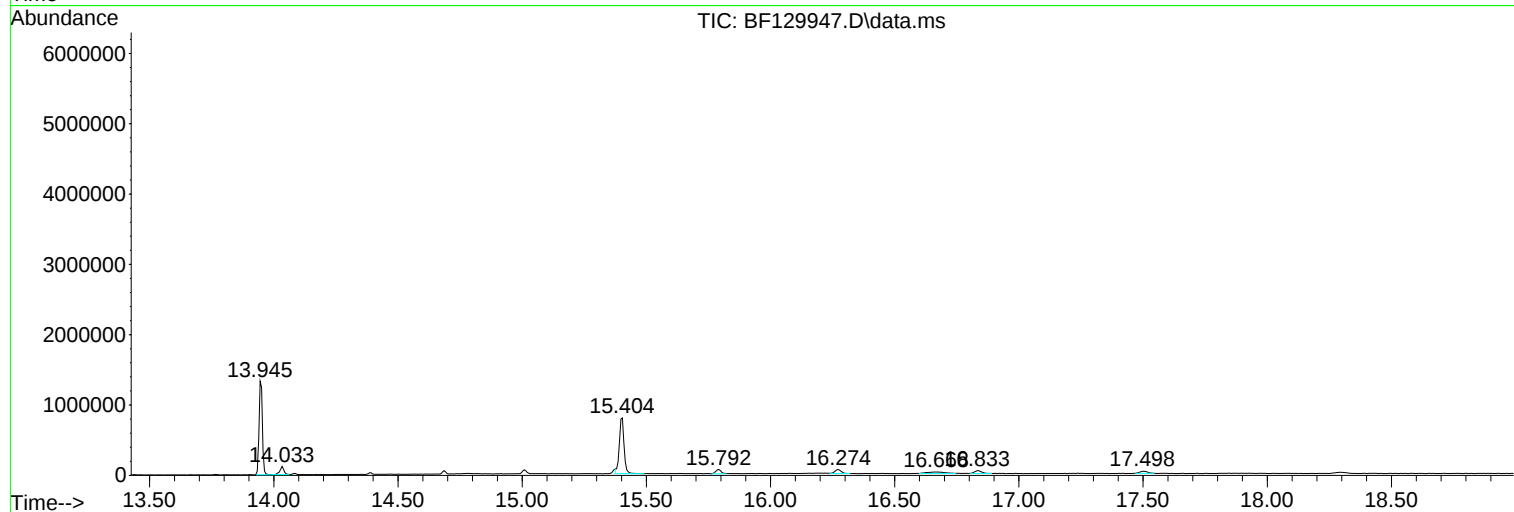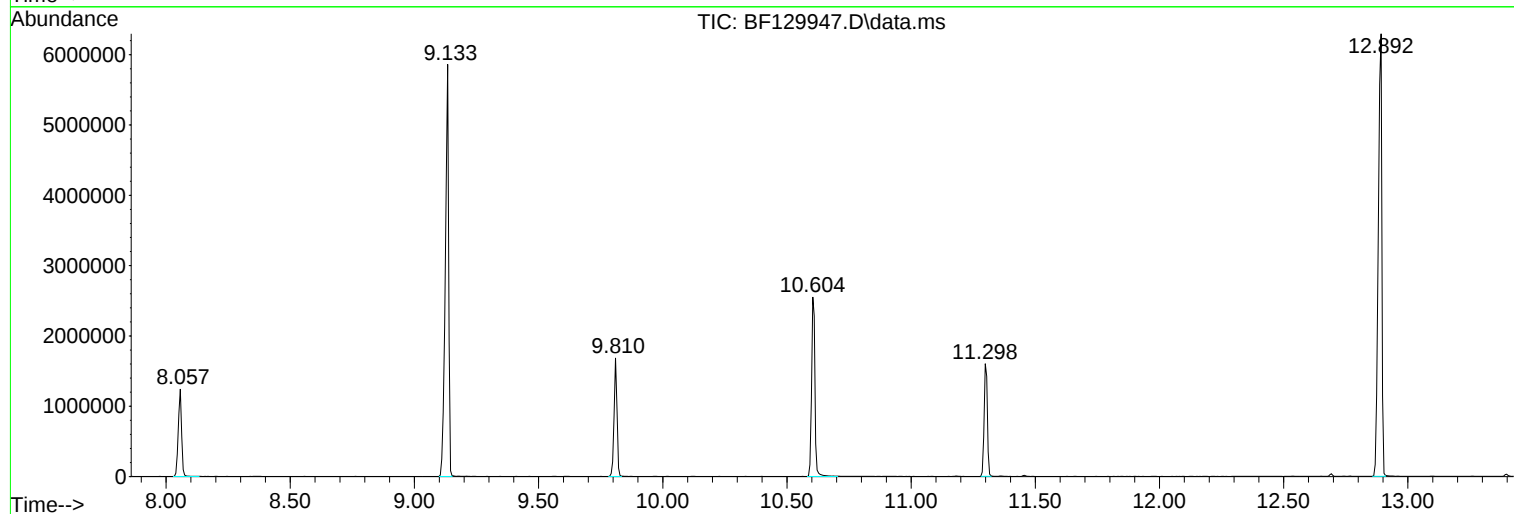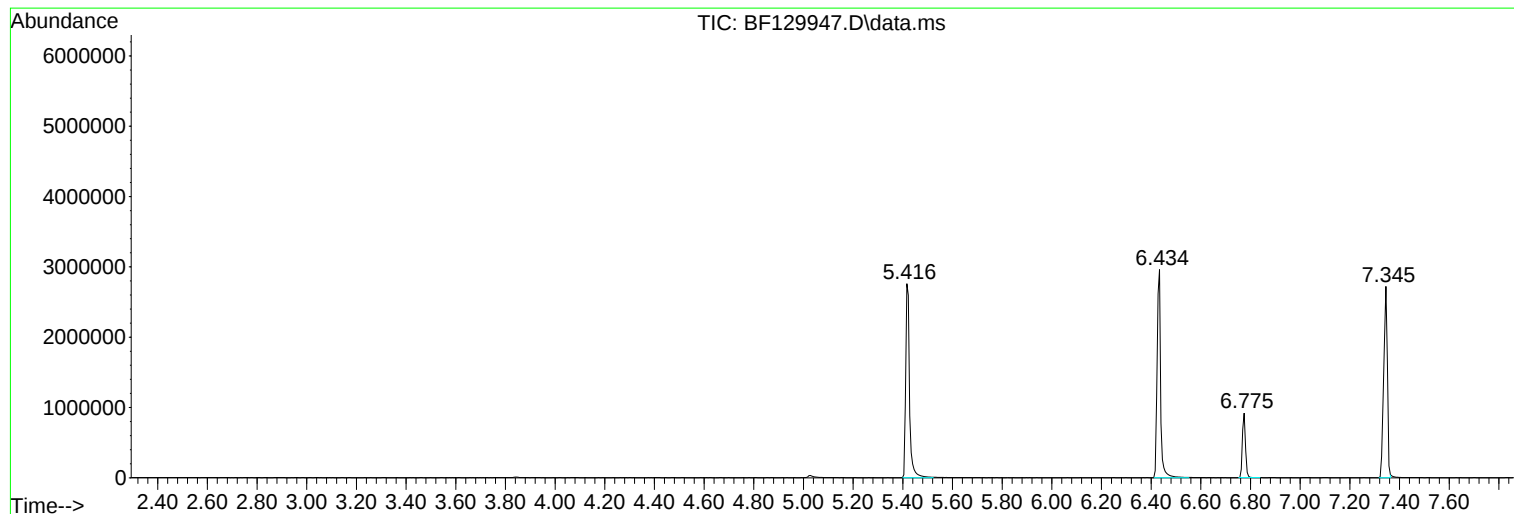

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
Data File : BF129947.D
Acq On : 23 Aug 2022 10:45
Operator : CG\JU
Sample : PB147059BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147059BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
Data File : BF129947.D
Acq On : 23 Aug 2022 10:45
Operator : CG\JU
Sample : PB147059BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147059BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------