
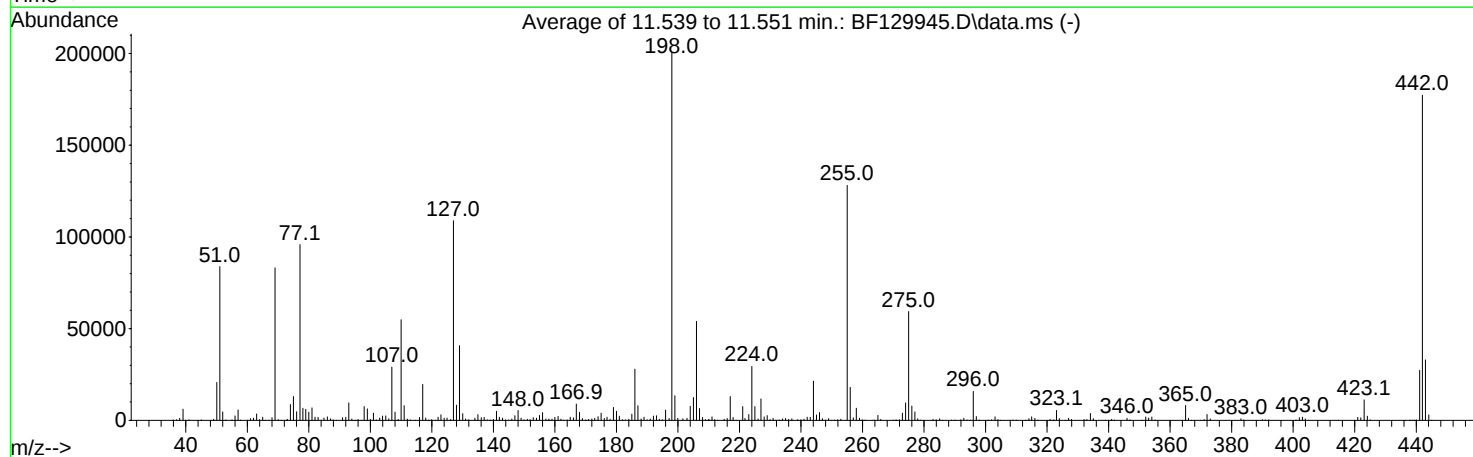


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
 Data File : BF129945.D
 Acq On : 23 Aug 2022 09:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 23 04:41:40 2022

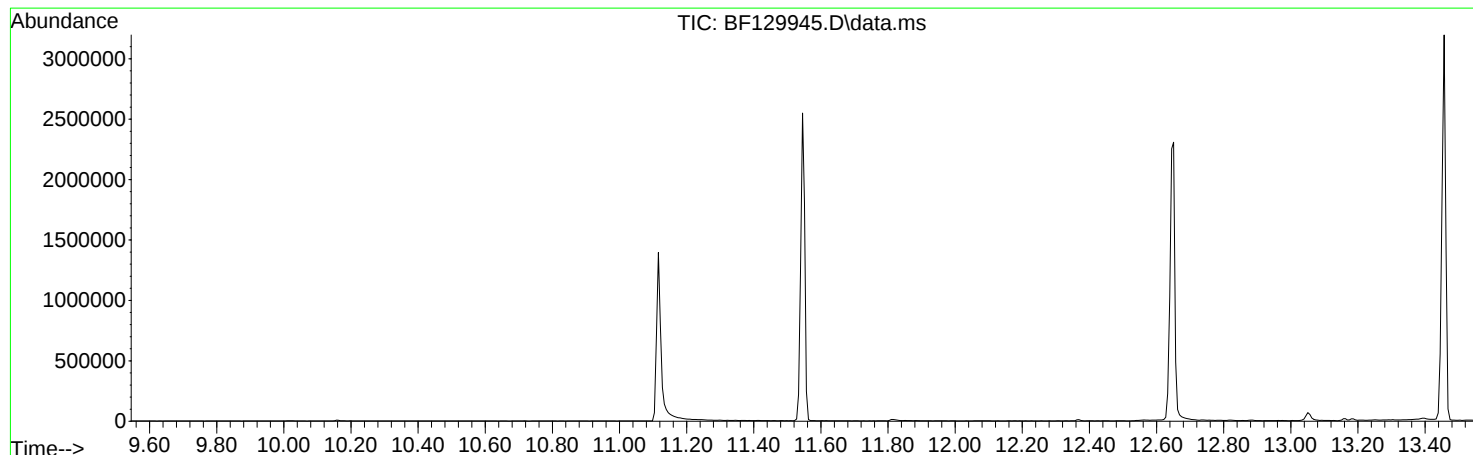

AutoFind: Scans 1573, 1574, 1575; Background Corrected with Scan 1568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	83808	PASS
68	69	0.00	2	1.8	1474	PASS
69	198	0.00	100	41.5	83168	PASS
70	69	0.00	2	0.5	444	PASS
127	198	10	80	54.3	108875	PASS
197	198	0.00	2	0.5	1013	PASS
198	198	100	100	100.0	200555	PASS
199	198	5	9	6.7	13400	PASS
275	198	10	60	29.6	59304	PASS
365	198	1	100	4.1	8150	PASS
441	198	0.01	100	13.6	27266	PASS
442	442	50	100	100.0	177219	PASS
443	442	15	24	18.6	32977	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/23/2022	BNA_F	<u>BF129945.D</u>
Compound Name	Response	Retention Time
DDT	481754	13.457
DDD	5657	13.163
DDE	842	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6499	488253	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
 Data File : BF129945.D
 Acq On : 23 Aug 2022 09:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 24 03:32:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 23 04:41:40 2022
 Response via : Initial Calibration

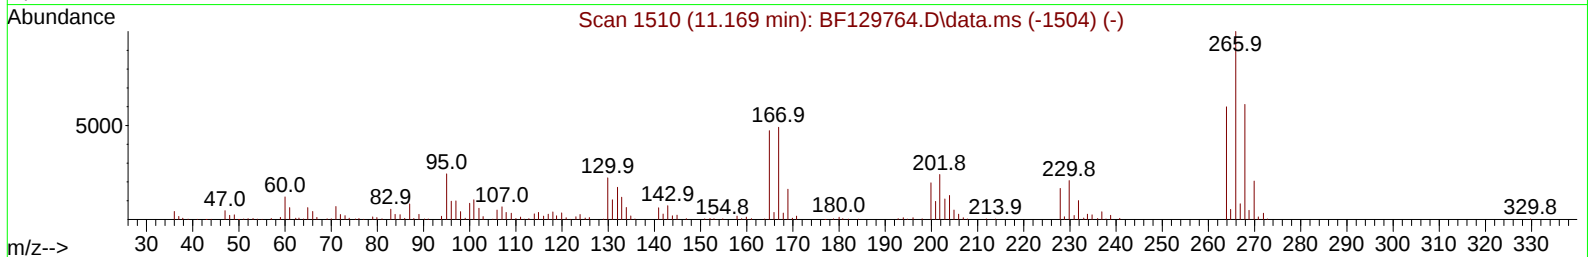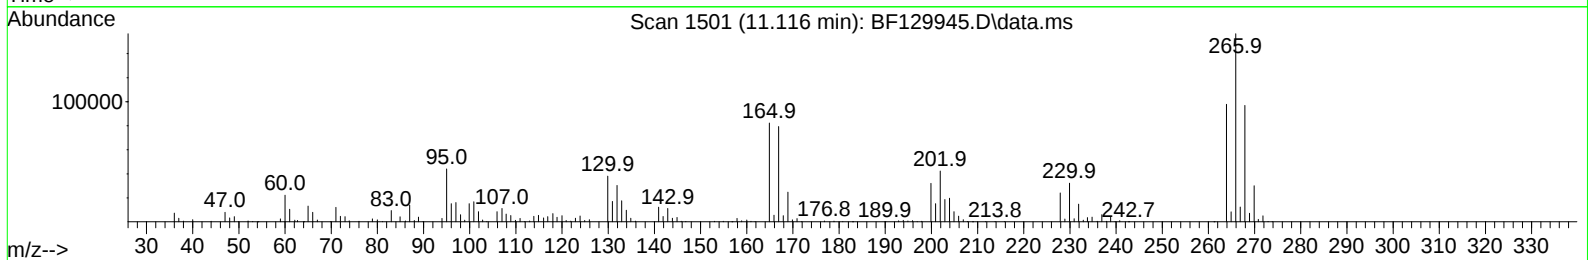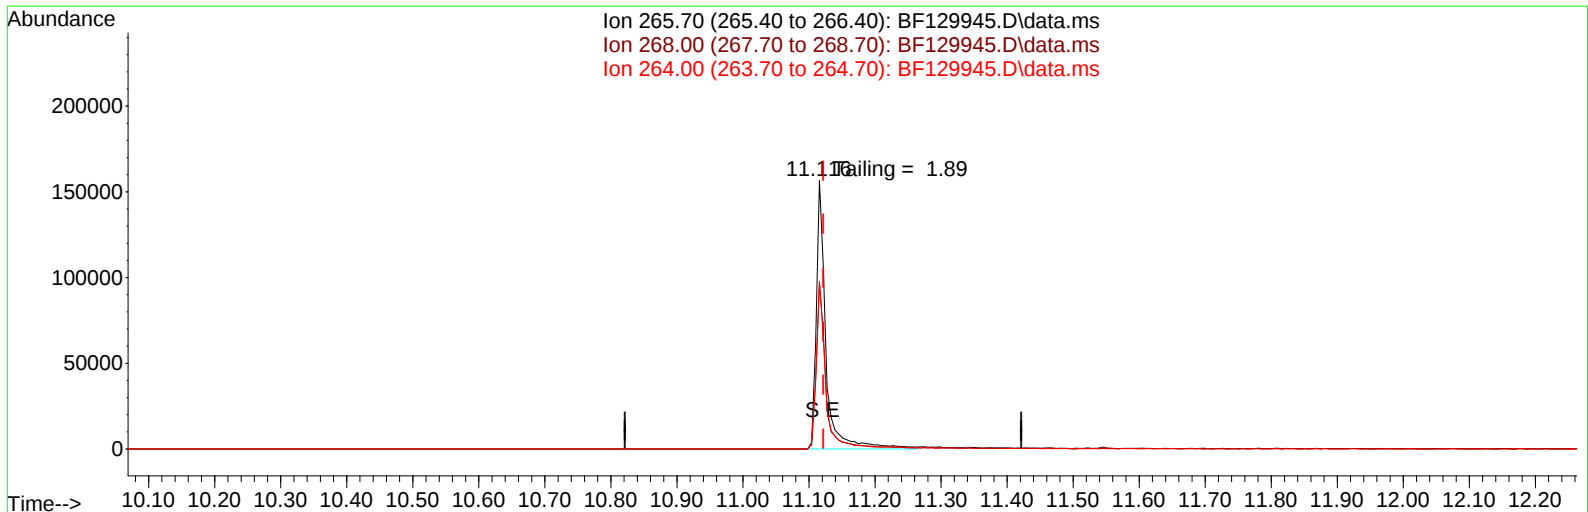

TIC: BF129945.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 659787.73 ng




response 160980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.89
264.00	59.90	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082322\
Data File : BF129945.D
Acq On : 23 Aug 2022 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 24 03:32:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 04:41:40 2022
Response via : Initial Calibration

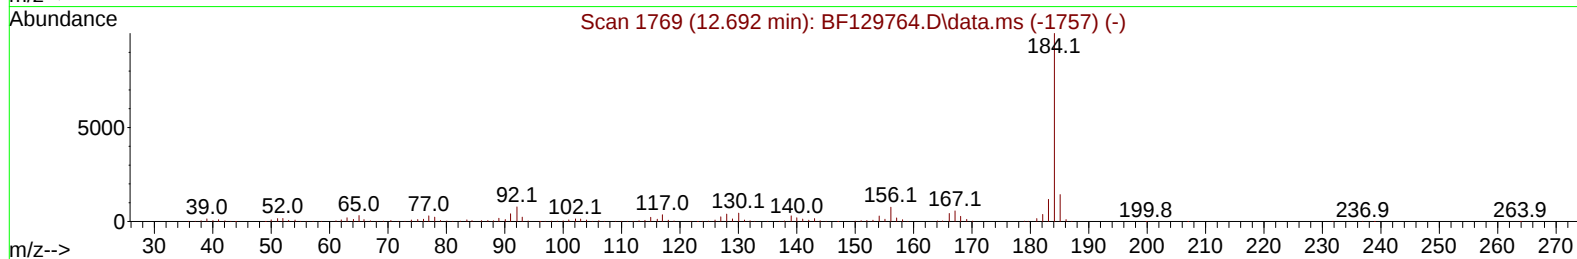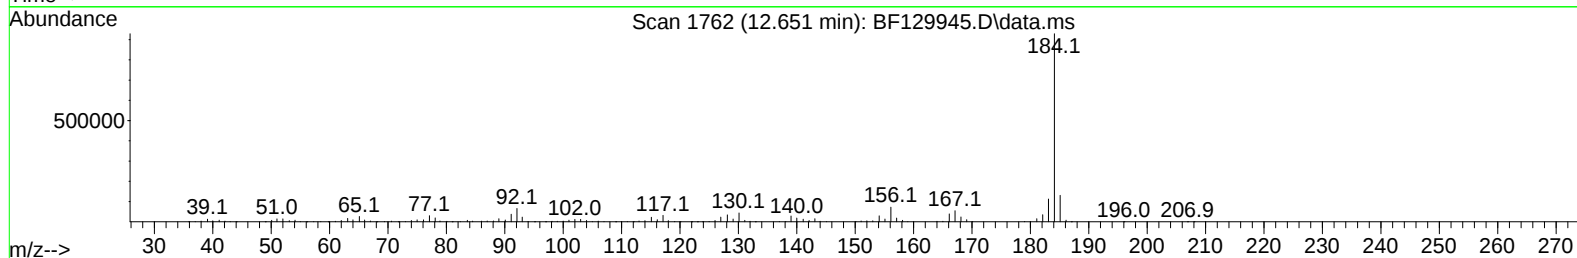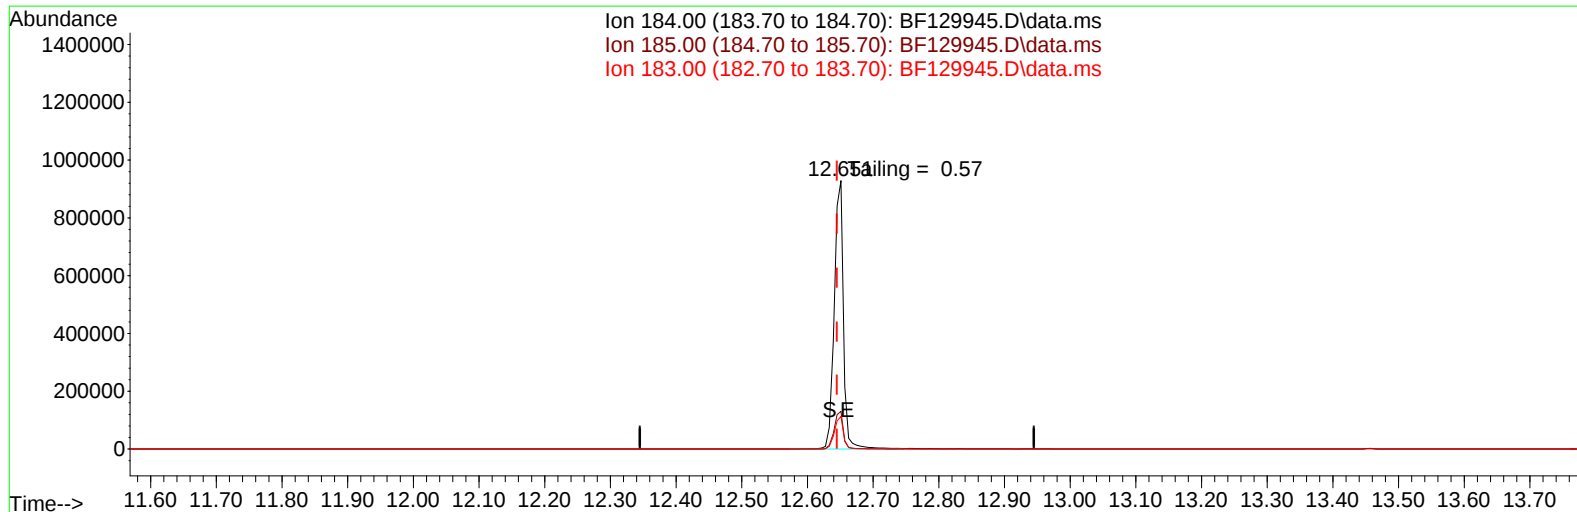

TIC: BF129945.D\data.ms

(77) Benzidine

12.651min (+ 0.006) 174486.16 ng

response 911342

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.06
183.00	11.80	12.09
0.00	0.00	0.00