
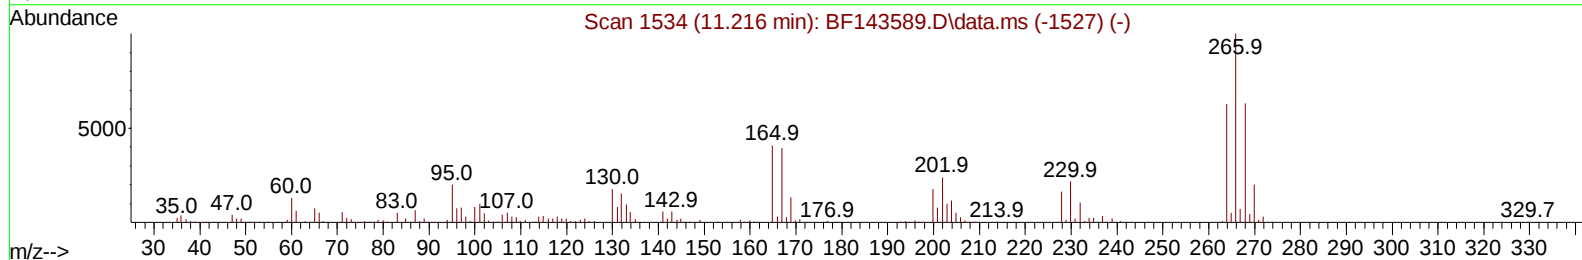
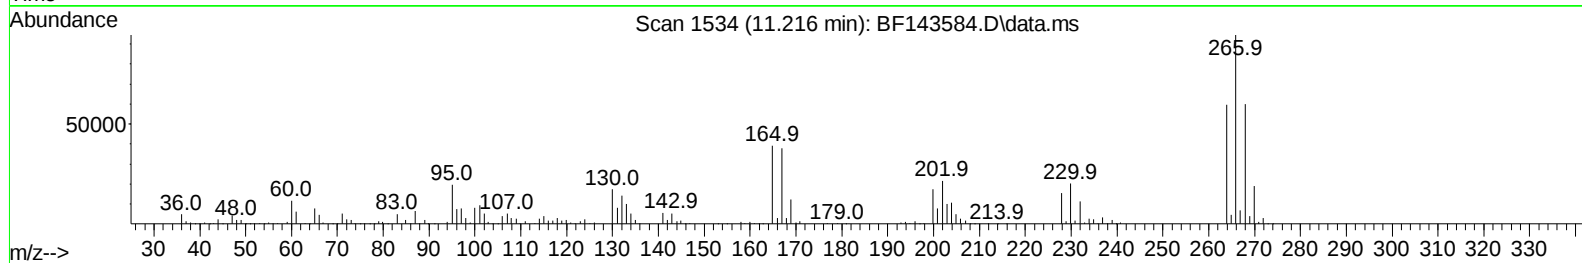


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082625\
Data File : BF143584.D
Acq On : 26 Aug 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 16:49:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

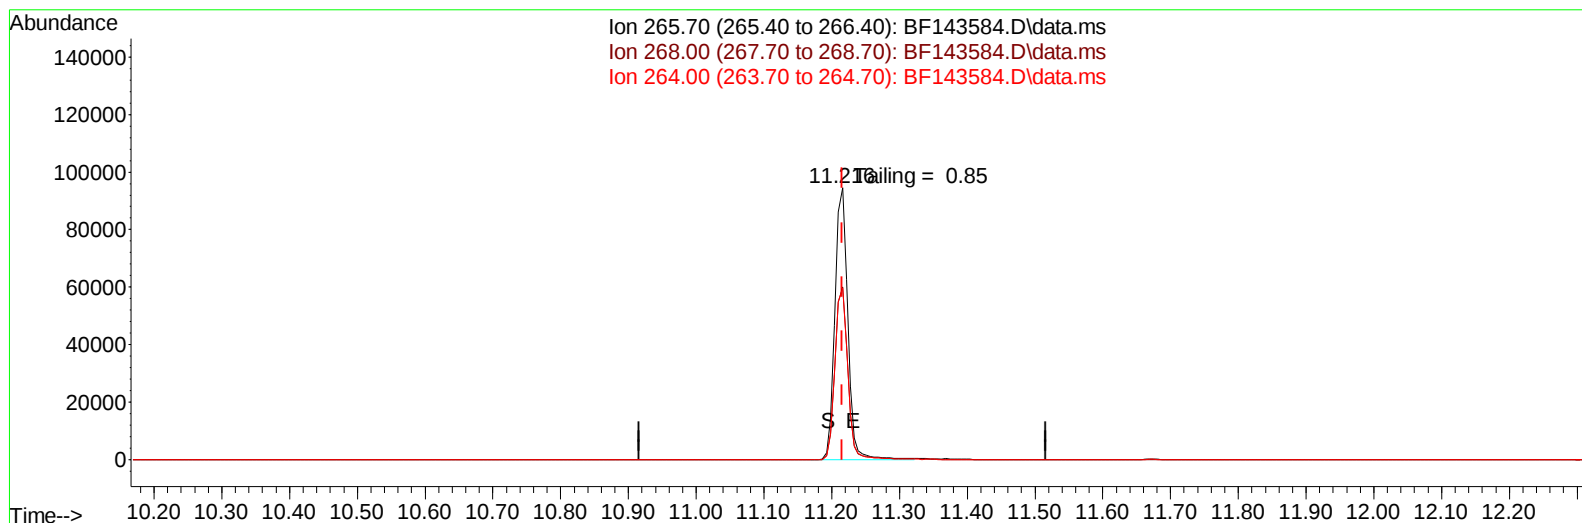

TIC: BF143584.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 43843.49 ng

response 124332

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.55
264.00	62.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082625\
Data File : BF143584.D
Acq On : 26 Aug 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 16:49:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

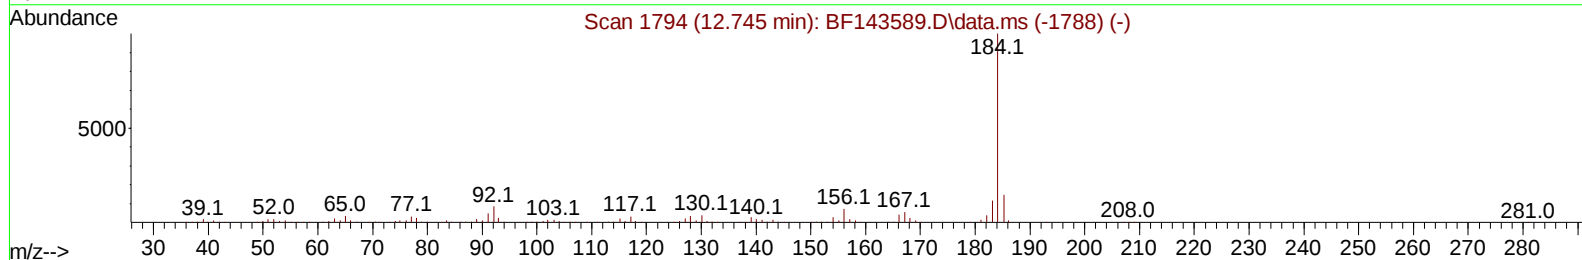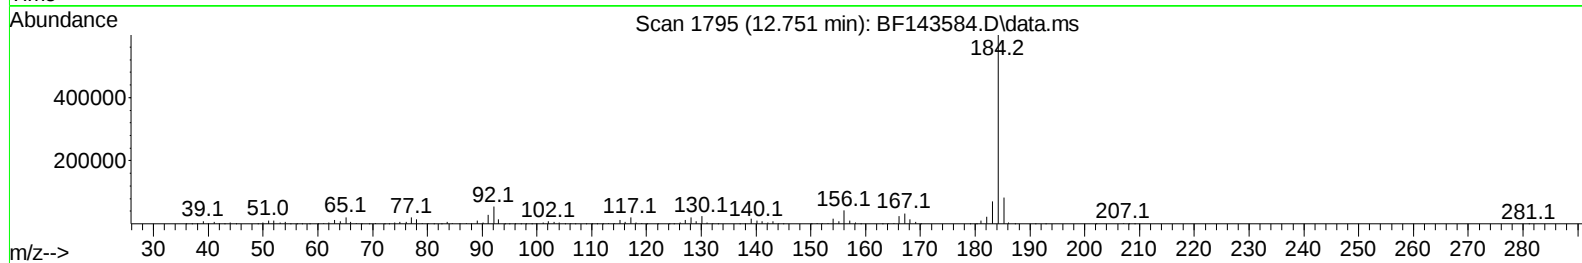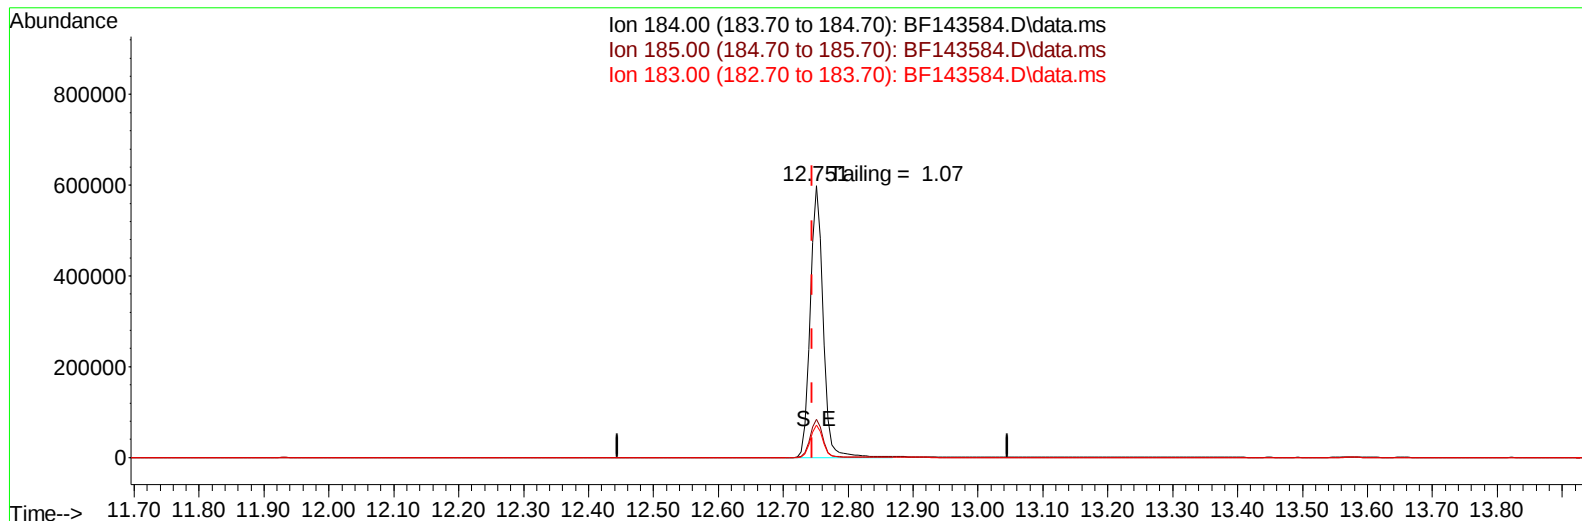

TIC: BF143584.D\data.ms

(77) Benzidine**12.751min (+ 0.006) 32424.16 ng****response 824131**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.06
183.00	11.40	11.84
0.00	0.00	0.00