

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082918\
 Data File : BF108618.D
 Acq On : 29 Aug 2018 21:29
 Operator : JU/SJ
 Sample : J4683-11
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082718-DBRI-F-D-S

Quant Time: Aug 30 01:10:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	111070	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	398737	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	160719	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	258630	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	260857	20.00	ng	0.00
86) Perylene-d12	15.75	264	256661	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	205214	33.45	ng	0.00
7) Phenol-d6	6.63	99	200325	24.57	ng	0.00
23) Nitrobenzene-d5	7.57	82	769209	107.65	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	144932	90.41	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	1294374	129.30	ng	-0.01
78) Terphenyl-d14	13.12	244	944639	92.07	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.57	70	99439	18.037	ng	# 80
25) Isophorone	7.57	82	770749	56.590	ng	# 64
49) Dimethylphthalate	9.74	163	75209	6.718	ng	# 99
50) 2,6-Dinitrotoluene	10.04	165	19546	8.345	ng	# 26
56) 2,4-Dinitrotoluene	10.04	165	19675	6.526	ng	# 24
64) 4,6-Dinitro-2-methylphenol	10.84	198	116	5.465	ng	# 1
66) 4-Bromophenyl-phenylether	10.84	248	8977	3.194	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082918\
Data File : BF108618.D
Acq On : 29 Aug 2018 21:29
Operator : JU/SJ
Sample : J4683-11
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082718-DBRI-F-D-S

Quant Time: Aug 30 01:10:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

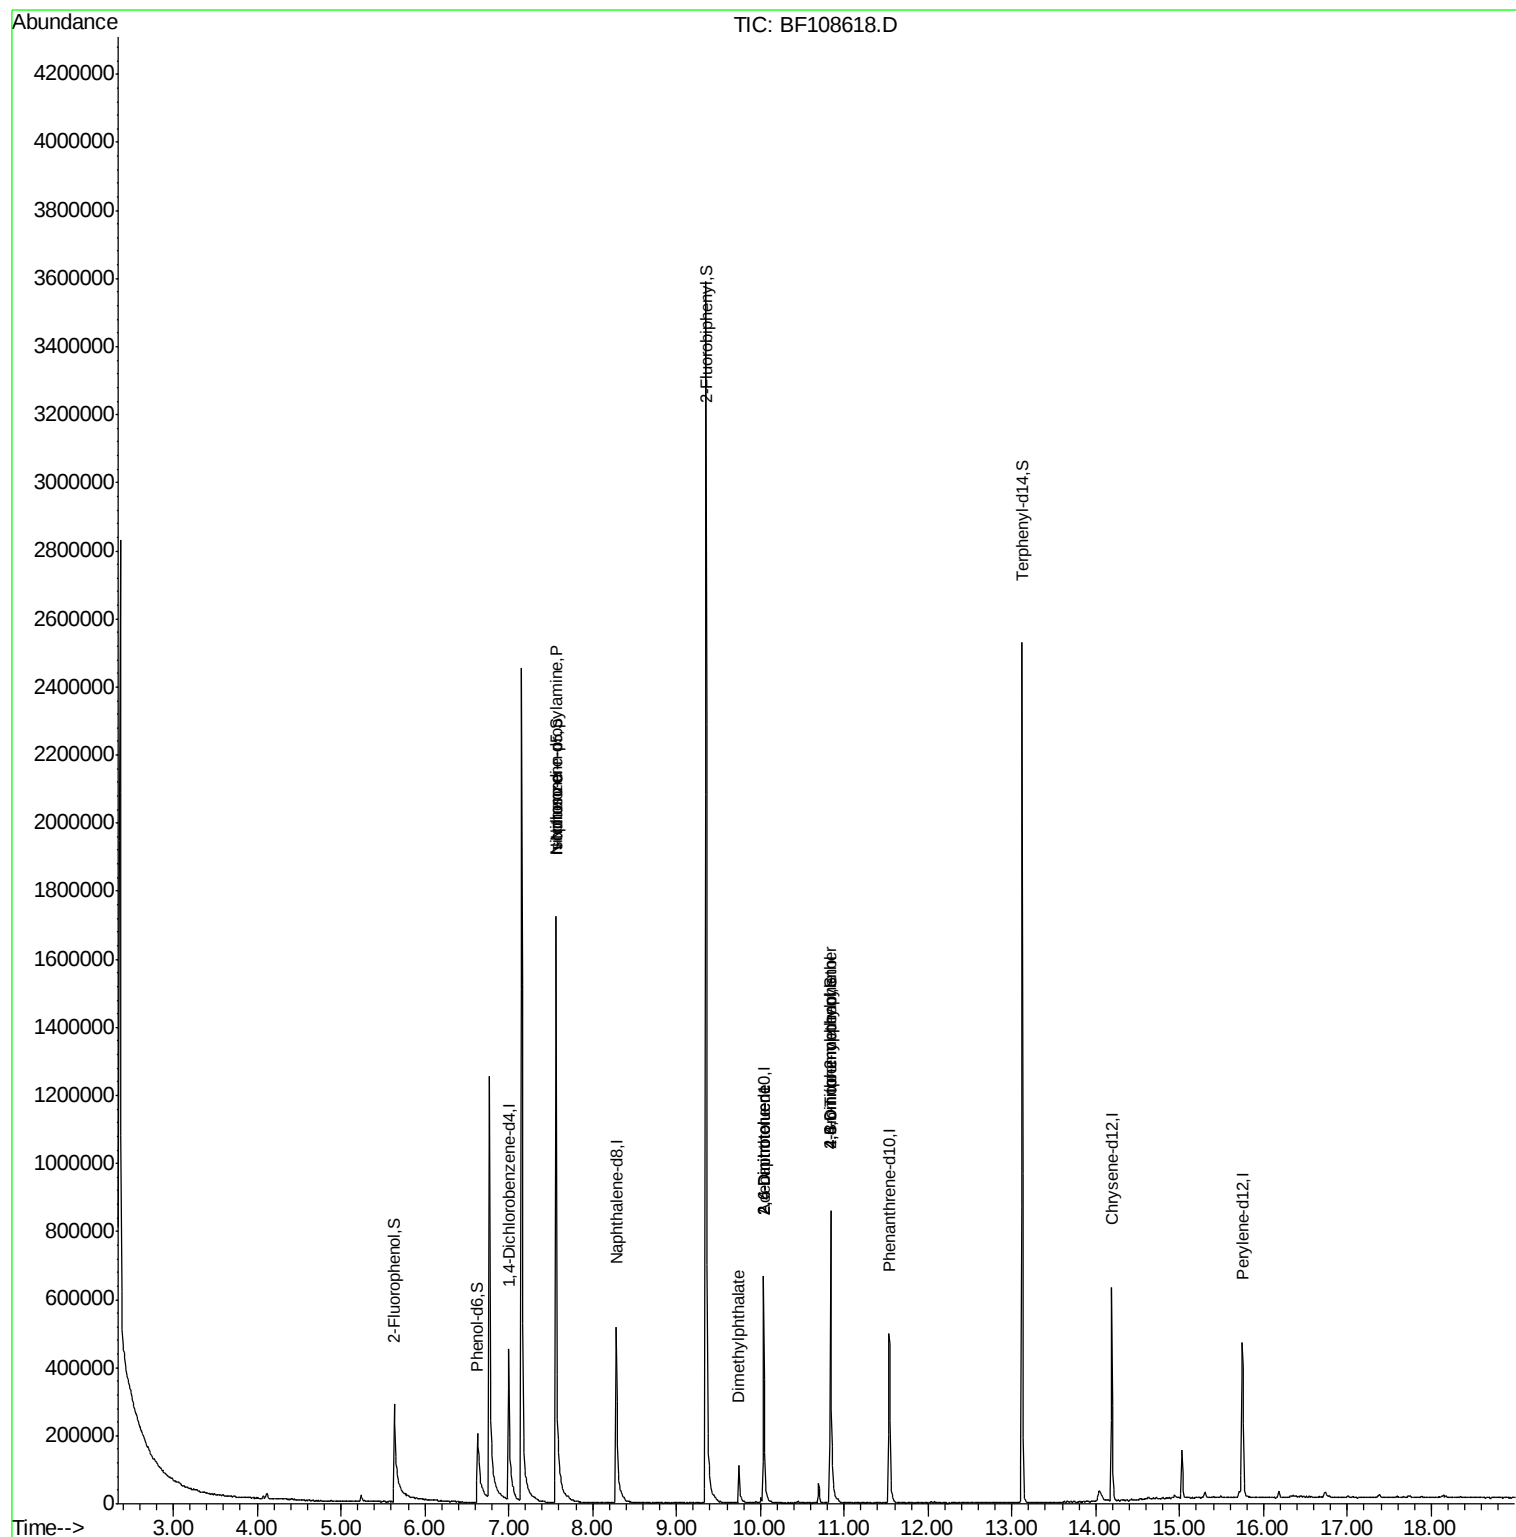

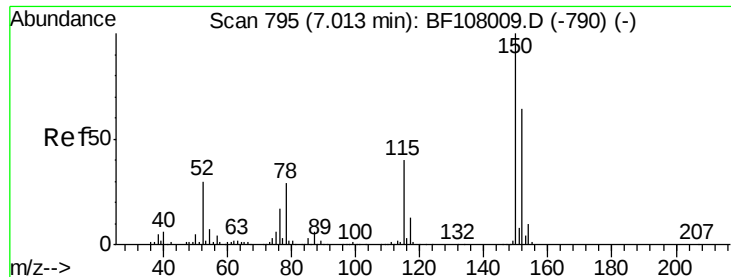


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Instrument :
BNA_F
ClientSampleId :
082718-DBRI-F-D-S

Tgt Ion:152 Resp: 111070
Ion Ratio Lower Upper
152 100
150 156.7 124.6 186.8
115 57.4 50.1 75.1

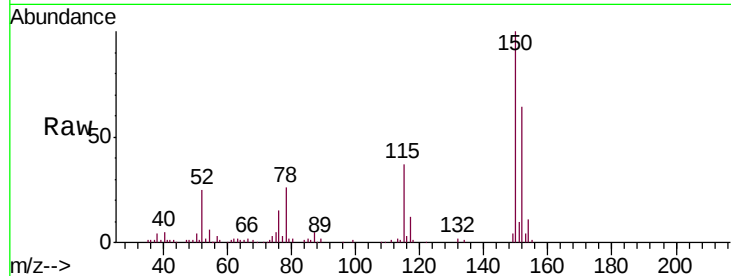


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

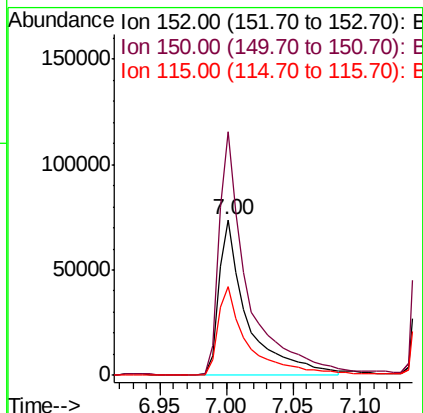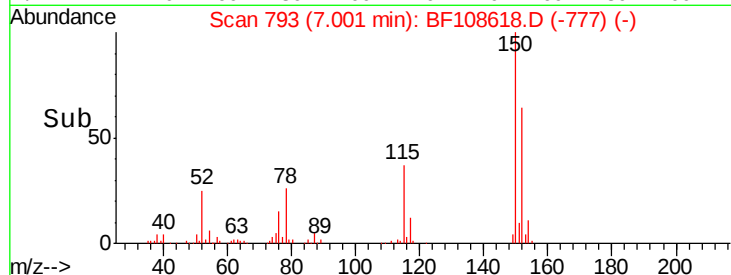



#5

2-Fluorophenol
Concen: 33.450 ng
RT: 5.64 min Scan# 561
Delta R.T. 0.01 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Tgt Ion:112 Resp: 205214
Ion Ratio Lower Upper
112 100
64 67.2 47.9 71.9
63 35.6 23.7 35.5#

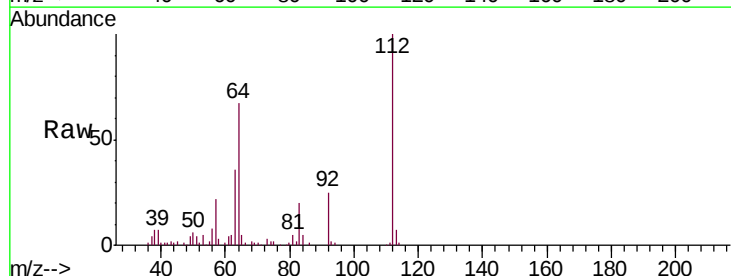

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

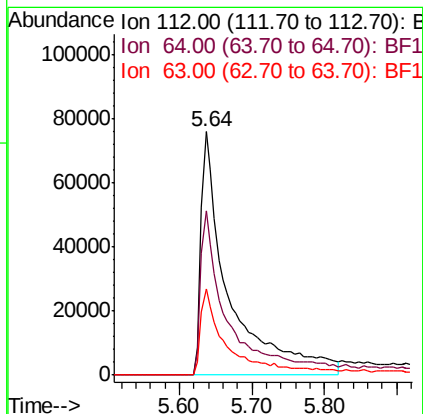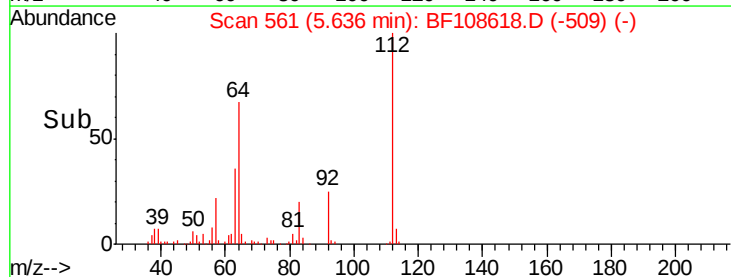



#7

Phenol-d6

Concen: 24.572 ng

RT: 6.63 min Scan# 730

Delta R.T. -0.00 min

Lab File: BF108618.D

Acq: 29 Aug 2018 21:29

Instrument :

BNA_F

ClientSampleId :

082718-DBRI-F-D-S


Tgt Ion: 99 Resp: 200325

Ion Ratio Lower Upper




99 100

42 21.9 14.5 21.7#

71 35.2 25.4 38.0

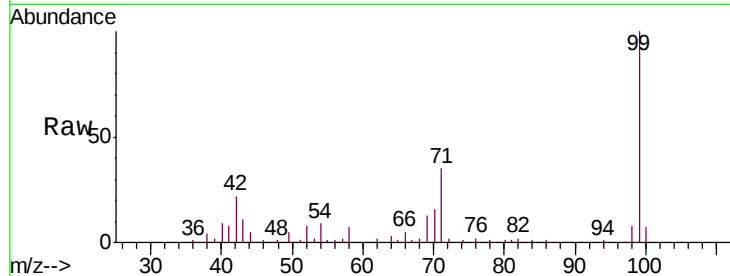

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

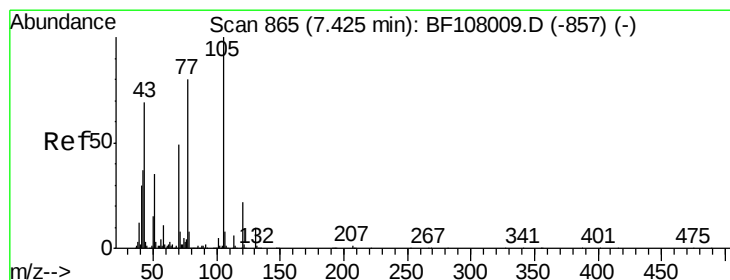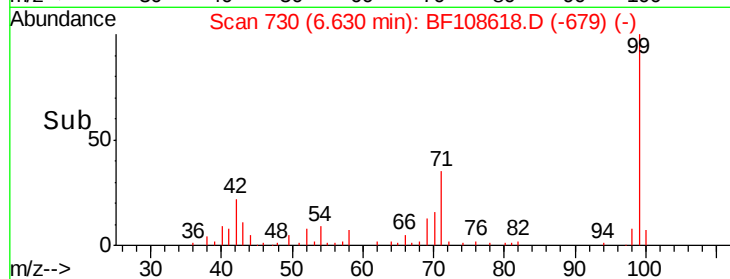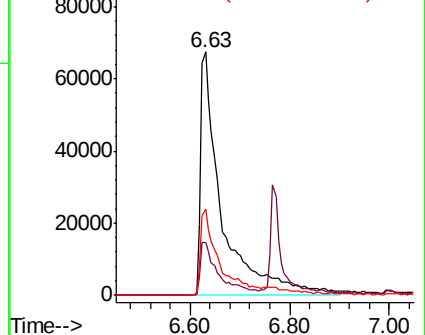

#19

n-Nitroso-di-n-propylamine

Concen: 18.037 ng

RT: 7.57 min Scan# 889

Delta R.T. 0.15 min

Lab File: BF108618.D

Acq: 29 Aug 2018 21:29

Tgt Ion: 70 Resp: 99439


Ion Ratio Lower Upper

70 100



42 50.8 47.5 71.3


101 0.0 7.4 11.2#

130 1.8 16.6 25.0#

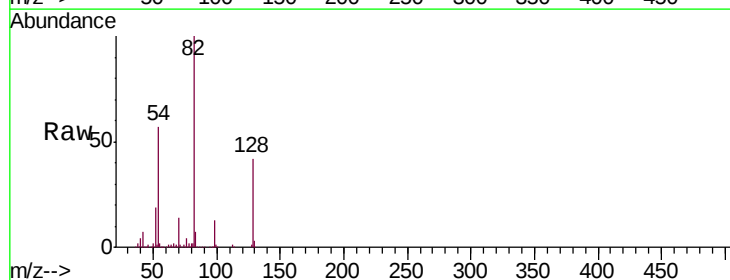

Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1

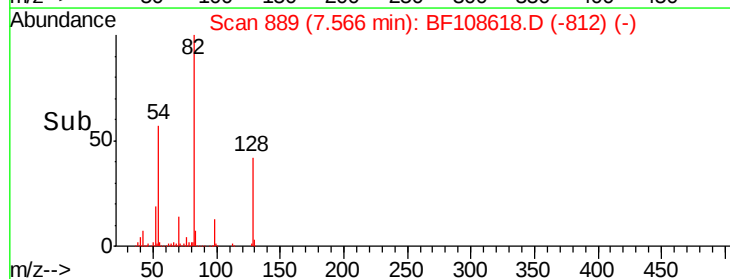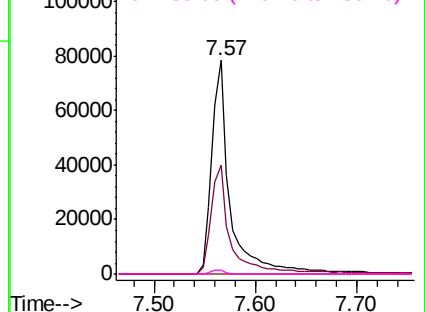


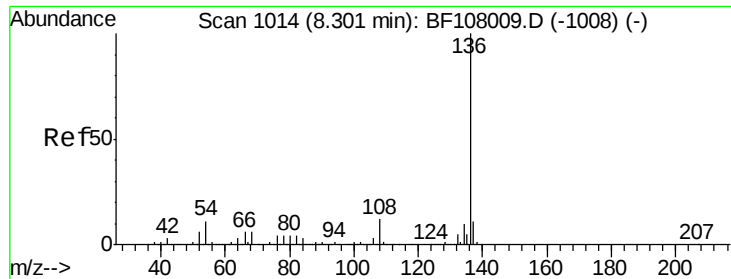



#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.28 min Scan# 1011
Delta R.T. -0.01 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Instrument :
BNA_F
ClientSampleId :
082718-DBRI-F-D-S

Tgt Ion:	136	Resp:	398737
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	8.6	6.6	9.8
68	5.2	5.0	7.4

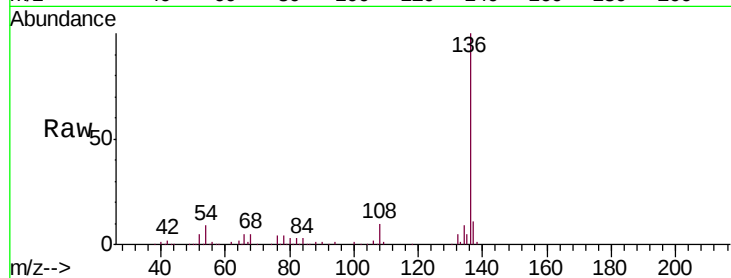


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

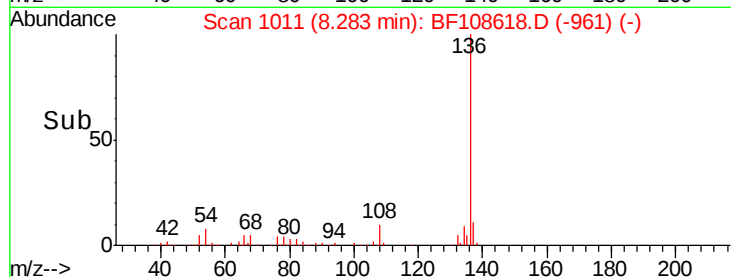
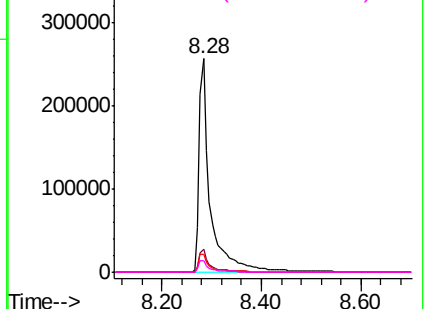


#23
Nitrobenzene-d5
Concen: 107.647 ng
RT: 7.57 min Scan# 889
Delta R.T. -0.01 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Tgt Ion:	82	Resp:	769209
Ion	Ratio	Lower	Upper
82	100		
128	42.5	36.1	54.1
54	57.3	41.4	62.2

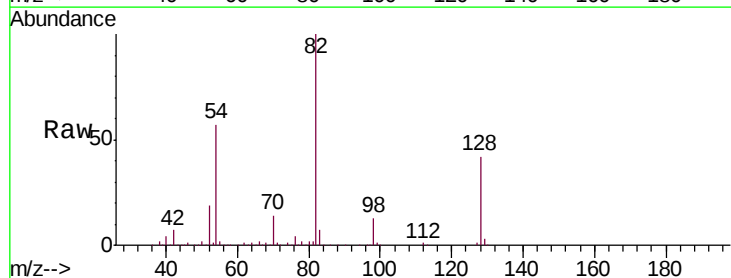

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1



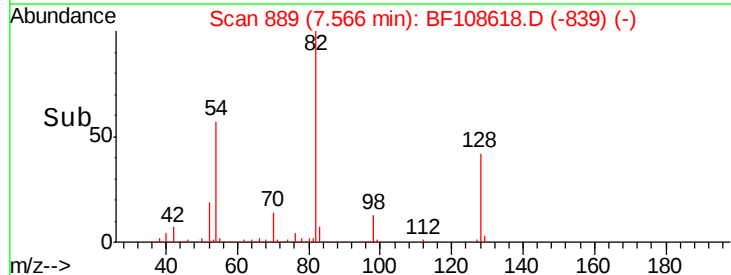
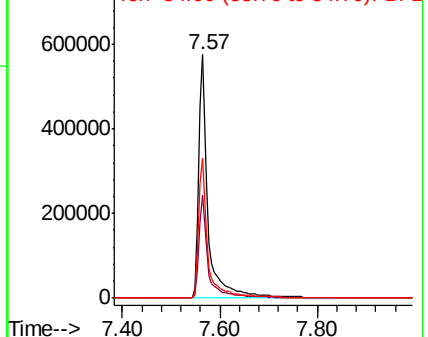




#25
Isophorone
Concen: 56.590 ng
RT: 7.57 min Scan# 889
Delta R.T. -0.26 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29




Instrument :
BNA_F
ClientSampleId :
082718-DBRI-F-D-S

Tgt Ion: 82 Resp: 770749
Ion Ratio Lower Upper
82 100
95 0.0 5.2 7.8#
138 0.0 14.9 22.3#

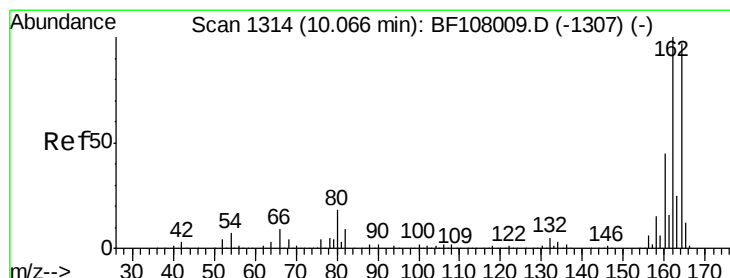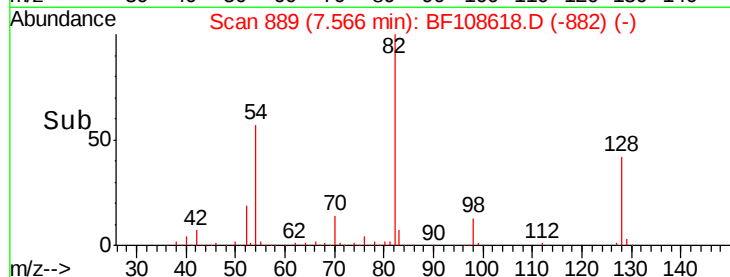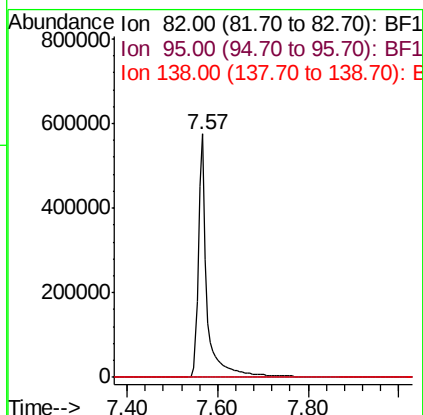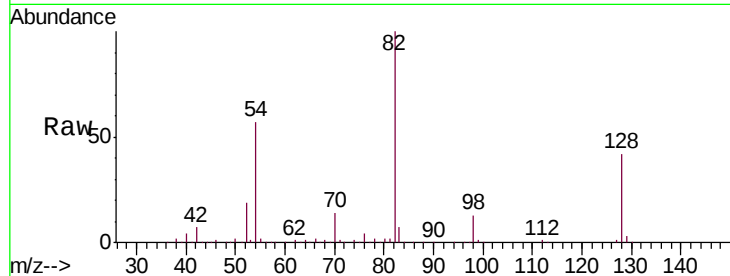

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.04 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Tgt Ion: 164 Resp: 160719
Ion Ratio Lower Upper
164 100
162 104.5 86.1 129.1
160 48.1 38.3 57.5

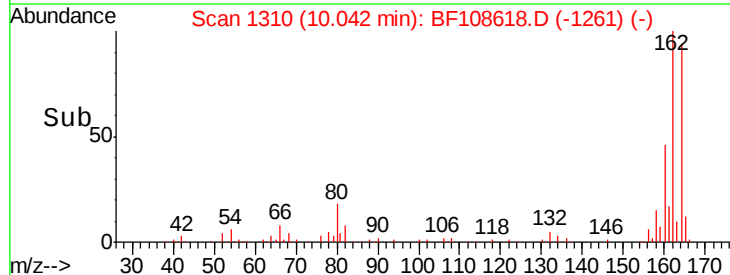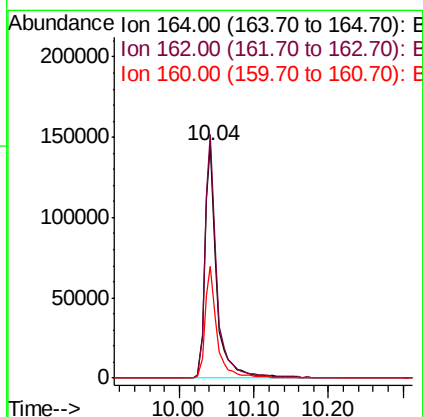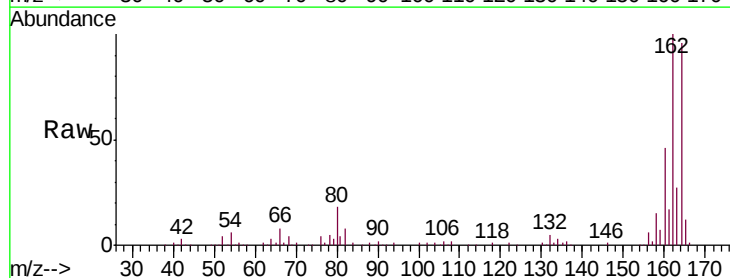






#41
 2,4,6-Tribromophenol
 Concen: 90.406 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108618.D
 Acq: 29 Aug 2018 21:29

Instrument :
 BNA_F
 ClientSampleId :
 082718-DBRI-F-D-S

Tgt Ion	Ratio	Lower	Upper
330	100		
332	94.3	77.0	115.6
141	33.0	29.9	44.9

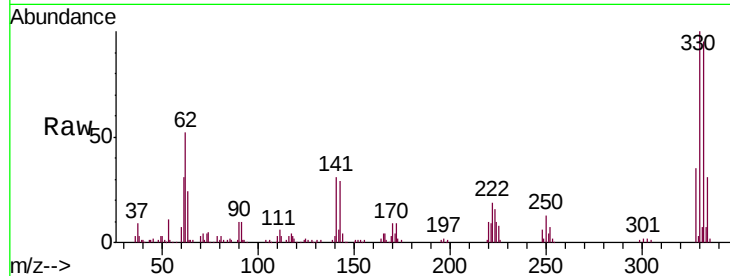


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

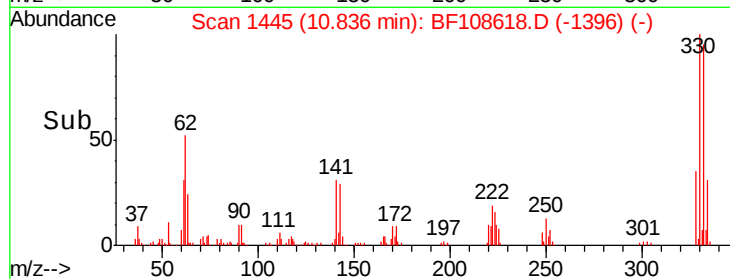
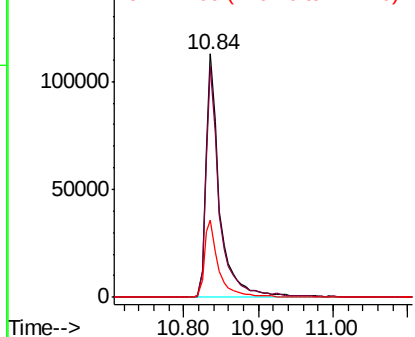



#44
 2-Fluorobiphenyl
 Concen: 129.299 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108618.D
 Acq: 29 Aug 2018 21:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.7	44.5
170	24.5	19.6	29.4

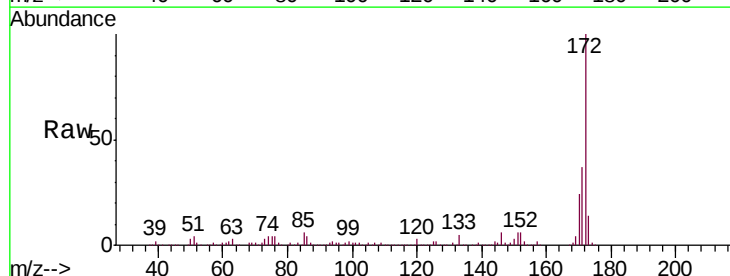

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

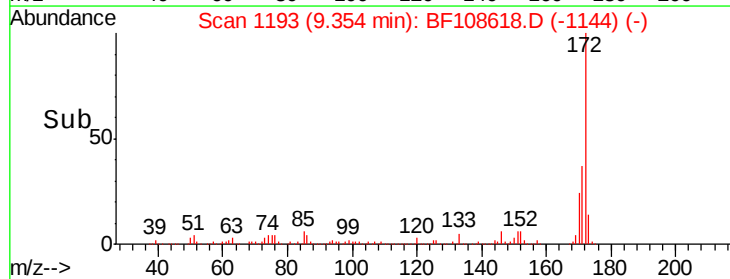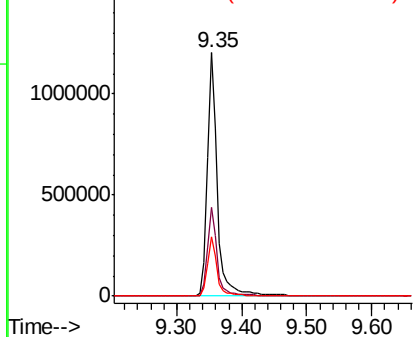


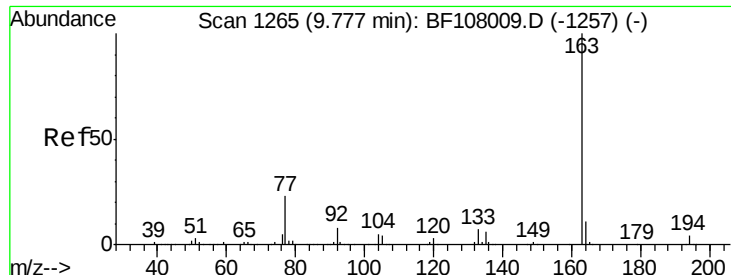




#49
Dimethylphthalate
Concen: 6.718 ng
RT: 9.74 min Scan# 1259
Delta R.T. -0.02 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Instrument :
BNA_F
ClientSampleId :
082718-DBRI-F-D-S

Tgt Ion:163 Resp: 75209
Ion Ratio Lower Upper
163 100
194 2.9 2.7 4.1
164 10.0 8.2 12.2

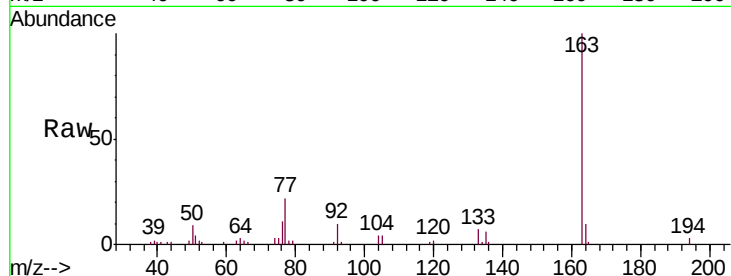


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

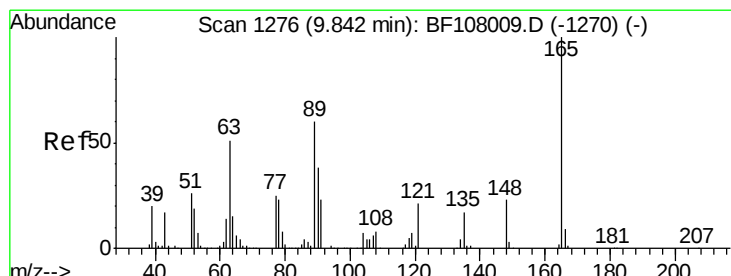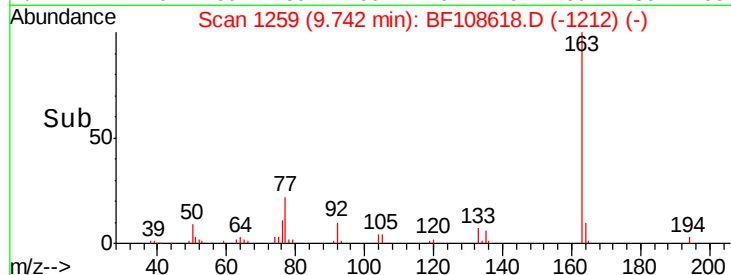
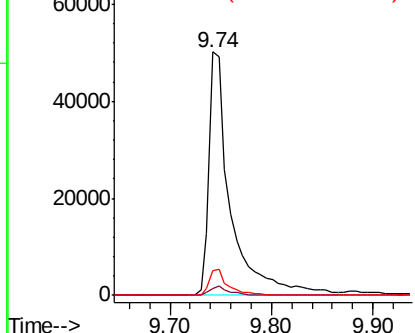


#50
2,6-Dinitrotoluene
Concen: 8.345 ng
RT: 10.04 min Scan# 1310
Delta R.T. 0.21 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Tgt Ion:165 Resp: 19546
Ion Ratio Lower Upper
165 100
63 2.1 44.7 67.1#
89 1.9 44.0 66.0#

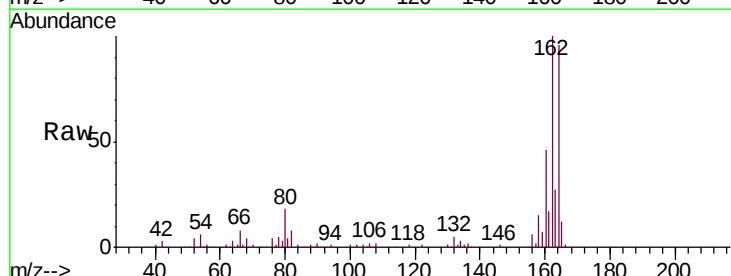

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

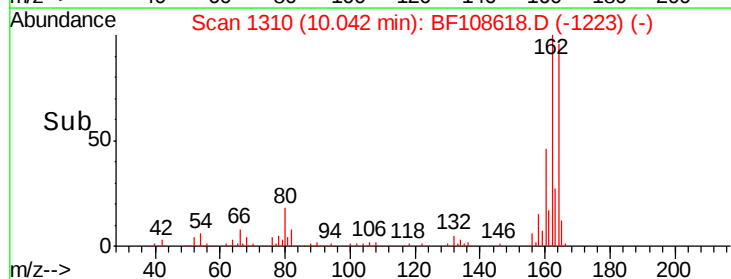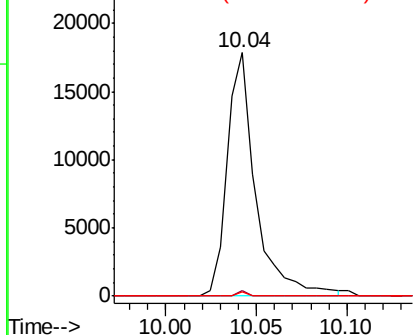




#56
 2,4-Dinitrotoluene
 Concen: 6.526 ng
 RT: 10.04 min Scan# 1310
 Delta R.T. -0.19 min
 Lab File: BF108618.D
 Acq: 29 Aug 2018 21:29

Instrument :
 BNA_F
 ClientSampleId :
 082718-DBRI-F-D-S

Tgt Ion:	165	Resp:	19675
Ion	Ratio	Lower	Upper
165	100		
63	2.1	36.4	54.6#
89	1.9	57.8	86.6#
182	0.0	1.6	2.4#


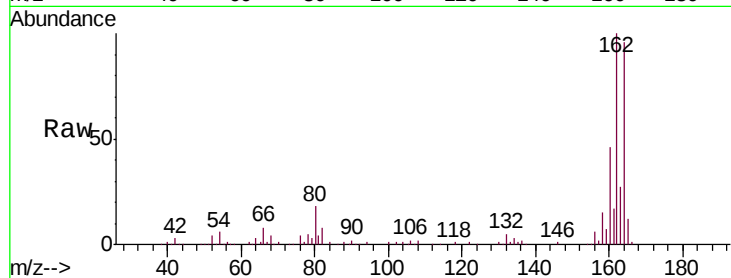


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

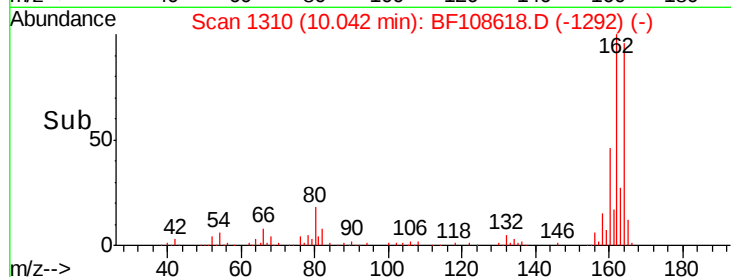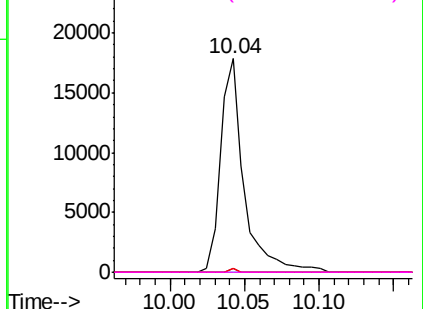

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.54 min Scan# 1564
 Delta R.T. -0.01 min
 Lab File: BF108618.D
 Acq: 29 Aug 2018 21:29



Tgt Ion:	188	Resp:	258630
Ion	Ratio	Lower	Upper
188	100		
94	8.9	8.5	12.7
80	9.6	9.2	13.8

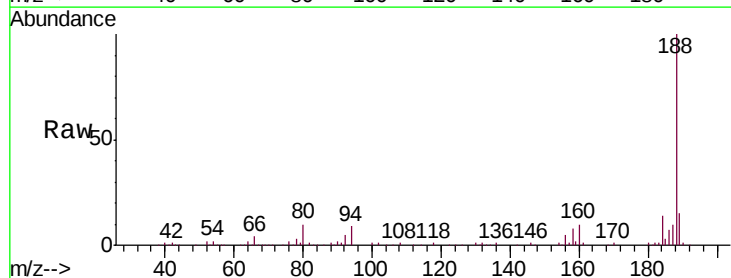

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

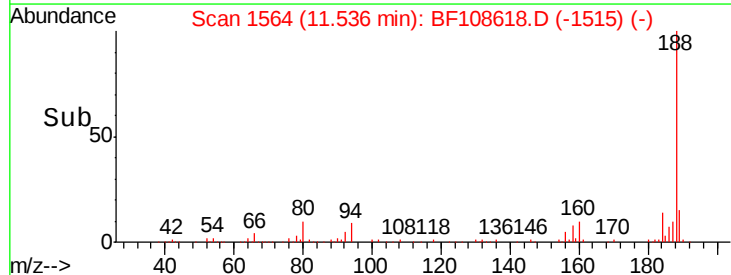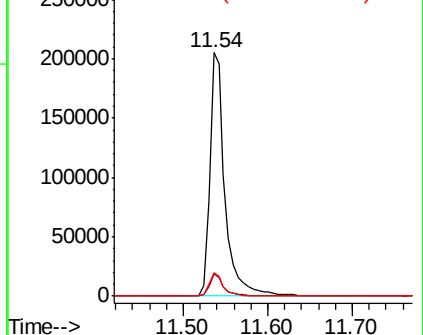







#64
 4,6-Dinitro-2-methylphenol
 Concen: 5.465 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. 0.19 min
 Lab File: BF108618.D
 Acq: 29 Aug 2018 21:29

Instrument :
 BNA_F
 ClientSampleId :
 082718-DBRI-F-D-S

Tgt Ion:198 Resp: 116
 Ion Ratio Lower Upper
 198 100
 51 249.4 37.7 77.7#
 105 167.7 36.3 76.3#

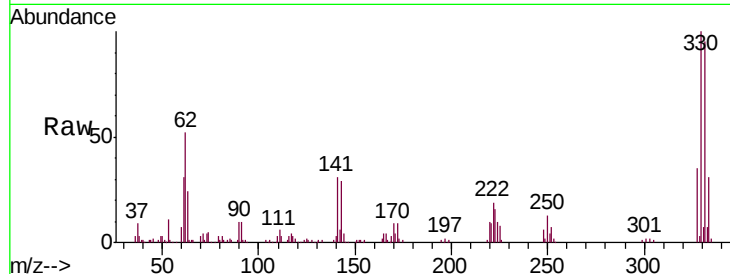


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

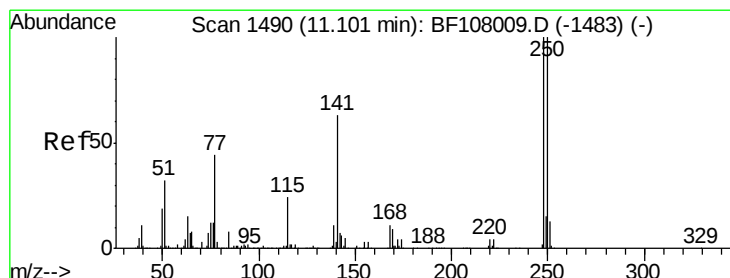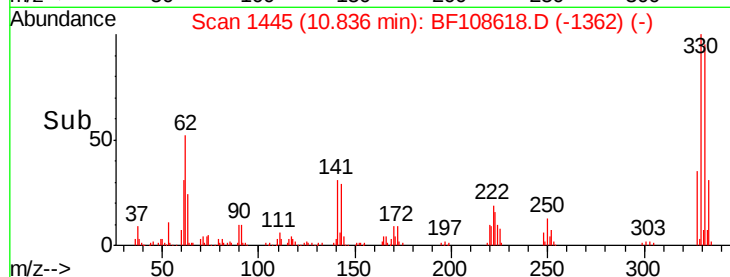
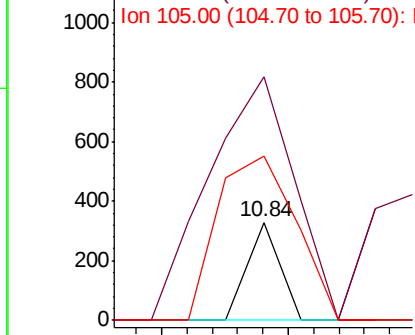



#66
 4-Bromophenyl-phenylether
 Concen: 3.194 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.25 min
 Lab File: BF108618.D
 Acq: 29 Aug 2018 21:29

Tgt Ion:248 Resp: 8977
 Ion Ratio Lower Upper
 248 100
 250 208.6 76.9 115.3#
 141 496.5 74.4 111.6#

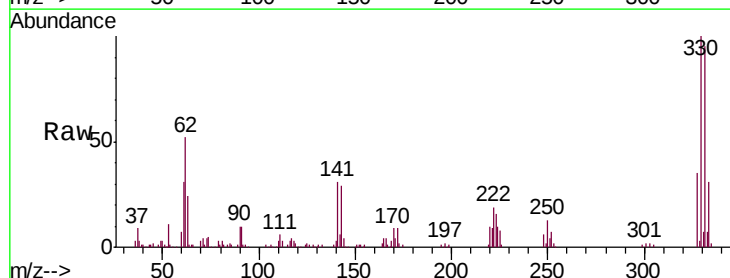

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

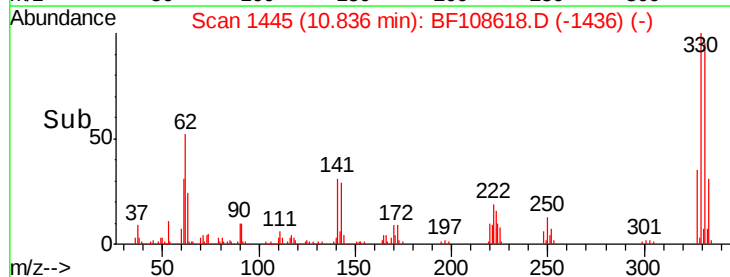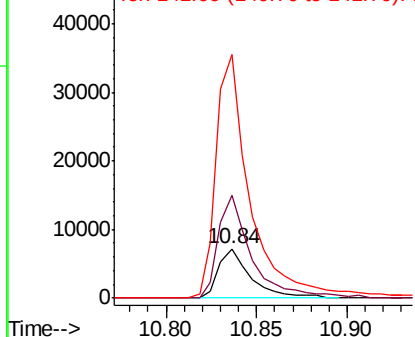

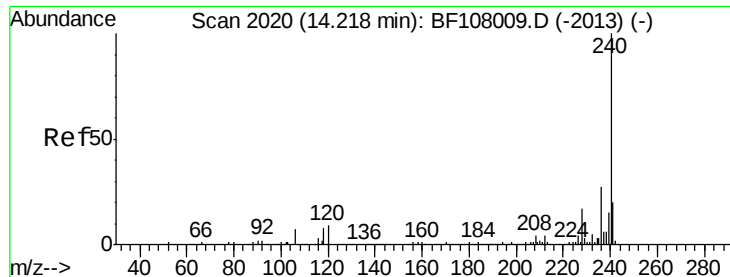

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2016

Delta R.T. -0.01 min

Lab File: BF108618.D

Acq: 29 Aug 2018 21:29

Instrument :

BNA_F

ClientSampleId :

082718-DBRI-F-D-S


Tgt Ion:240 Resp: 260857

Ion Ratio Lower Upper

240 100

120 8.5 9.5 14.3#




236 25.7 20.7 31.1

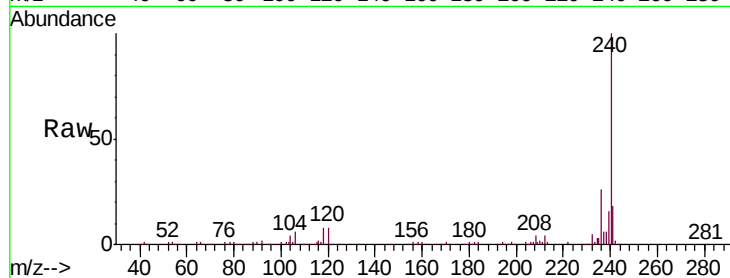

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

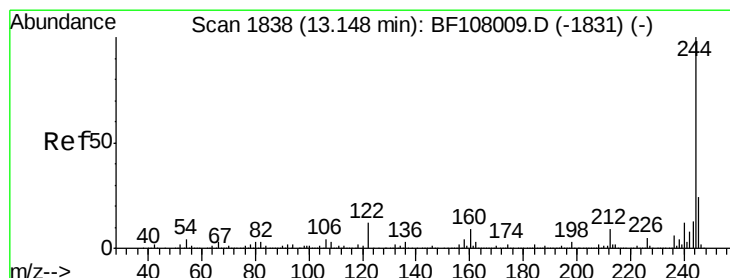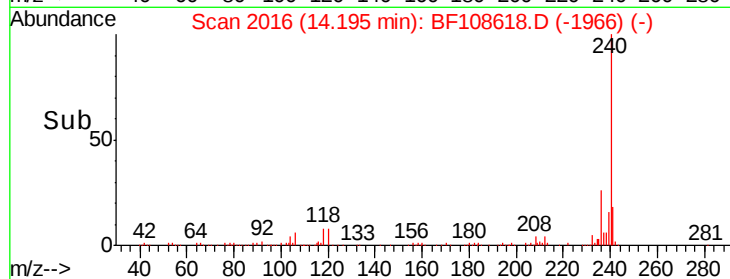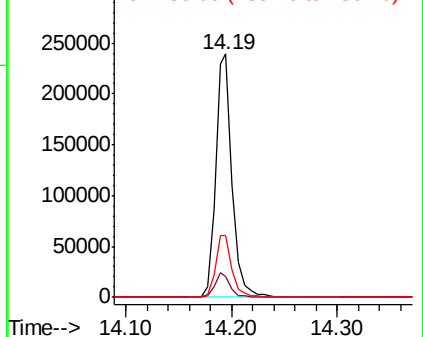

#78

Terphenyl-d14

Concen: 92.074 ng

RT: 13.12 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BF108618.D

Acq: 29 Aug 2018 21:29


Tgt Ion:244 Resp: 944639

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0



122 8.5 11.0 16.4#

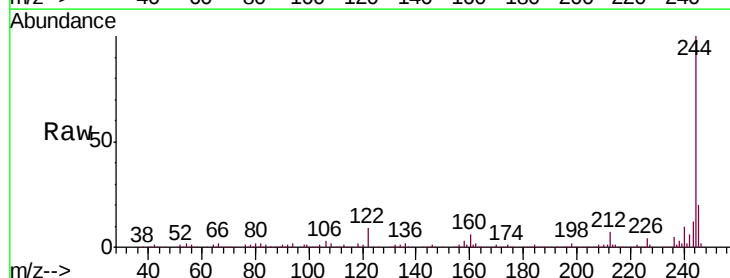


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

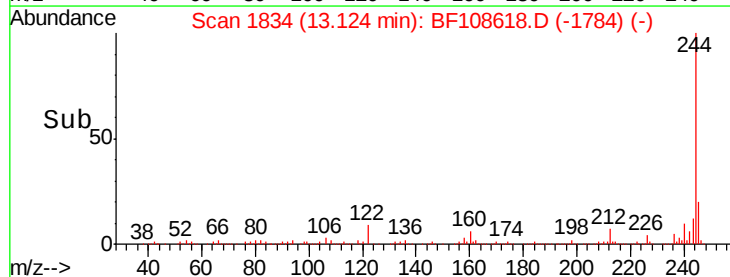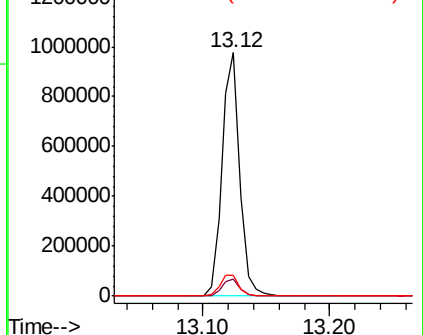

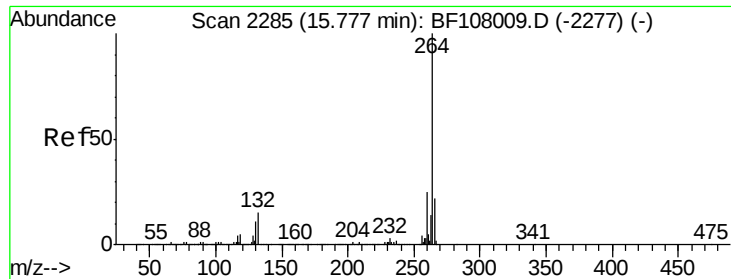

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.75 min Scan# 2280
Delta R.T. -0.01 min
Lab File: BF108618.D
Acq: 29 Aug 2018 21:29

Instrument :
BNA_F
ClientSampleId :
082718-DBRI-F-D-S

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	22.2	17.5	26.3

