
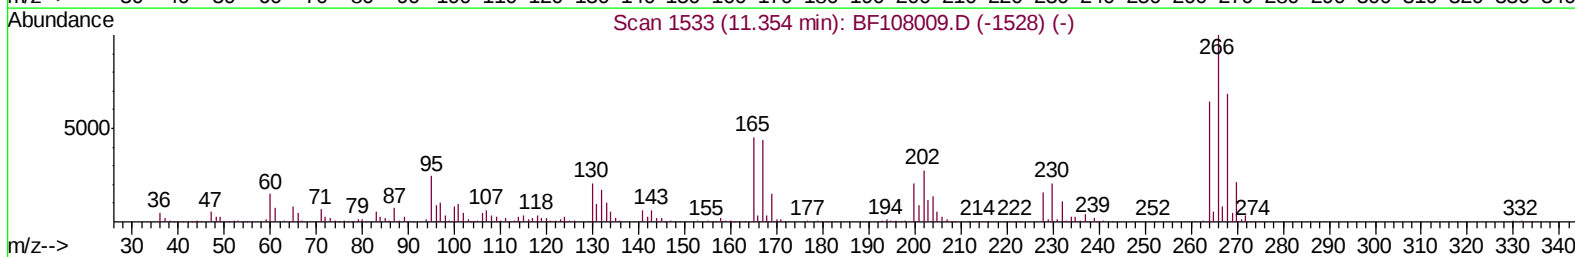
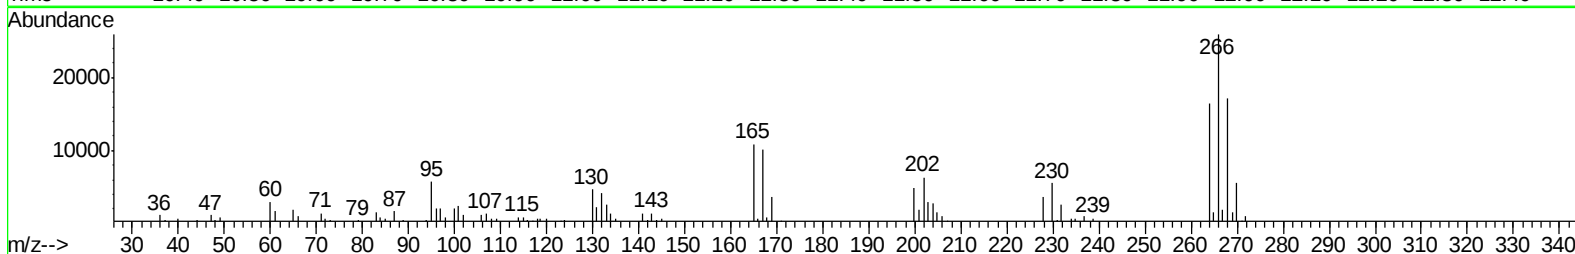


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082918\
Data File : BF108619.D
Acq On : 29 Aug 2018 22:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 04:56:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

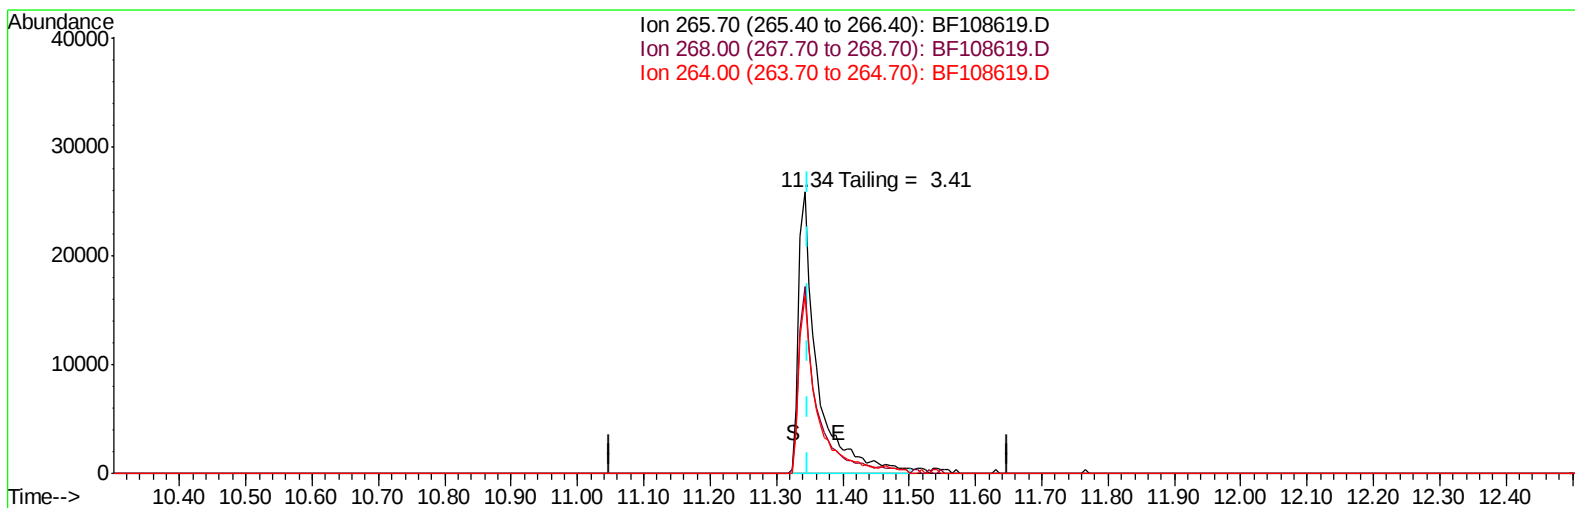

TIC: BF108619.D

(69) Pentachlorophenol (C)




11.342min (-0.006) 53554.17ng

response 49240

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.44
264.00	61.90	63.38
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082918\
Data File : BF108619.D
Acq On : 29 Aug 2018 22:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 04:56:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

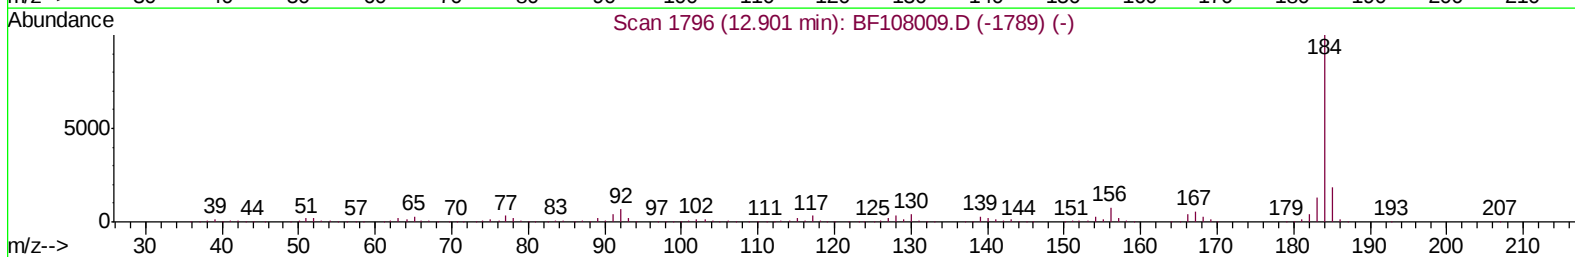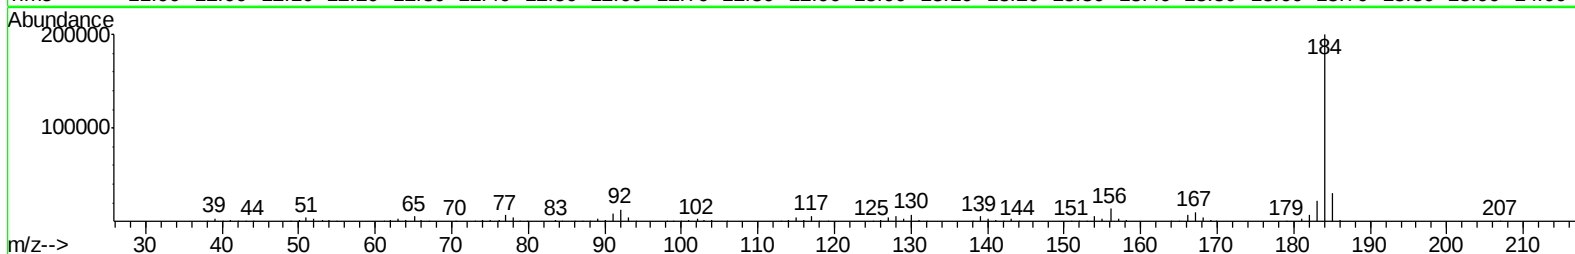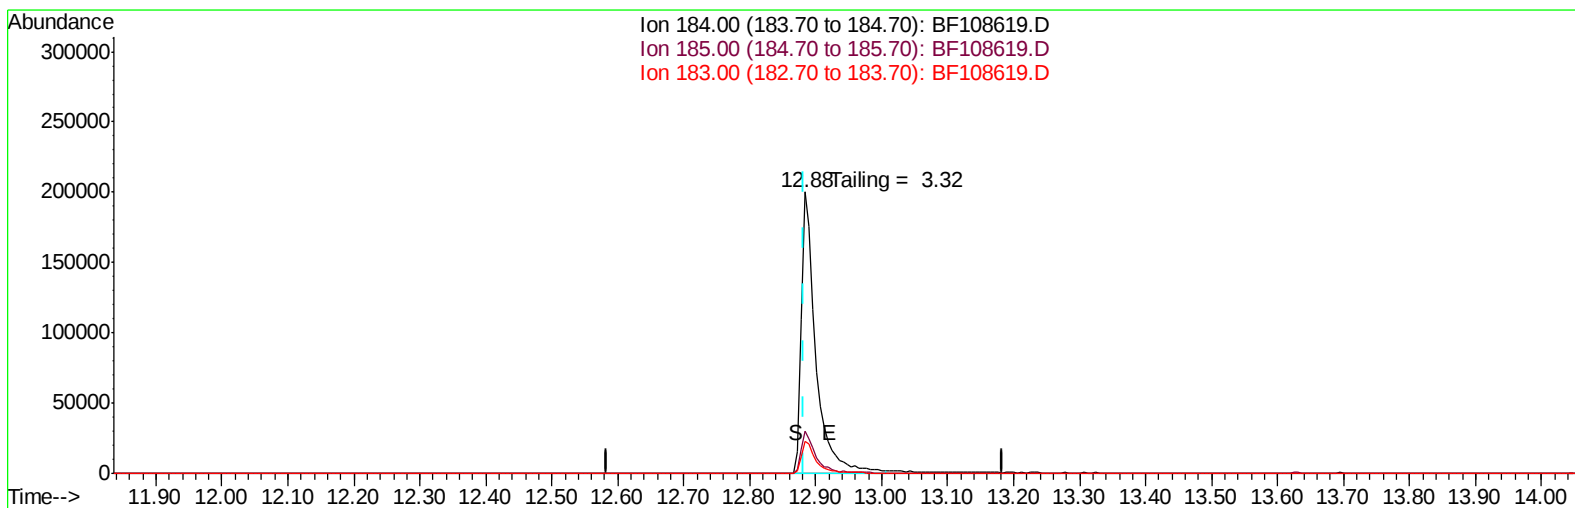

TIC: BF108619.D

(76) Benzidine

12.883min (-0.000) 35510.17ng

response 314439

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.97
183.00	11.60	11.38
0.00	0.00	0.00