

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082918\
 Data File : BF108627.D
 Acq On : 30 Aug 2018 2:33
 Operator : JU/SJ
 Sample : J4683-18
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082718-TIPC-F-U-S

Quant Time: Aug 30 04:33:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	116952	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	438447	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	196060	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	315352	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	259461	20.00	ng	-0.01
86) Perylene-d12	15.75	264	257693	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	220465	34.13	ng	0.00
7) Phenol-d6	6.62	99	199273	23.21	ng	0.00
23) Nitrobenzene-d5	7.57	82	832857	106.00	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	174504	89.23	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	1491134	122.10	ng	-0.01
78) Terphenyl-d14	13.12	244	999728	97.97	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.74	163	132643	9.712	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082918\
Data File : BF108627.D
Acq On : 30 Aug 2018 2:33
Operator : JU/SJ
Sample : J4683-18
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082718-TIPC-F-U-S

Quant Time: Aug 30 04:33:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

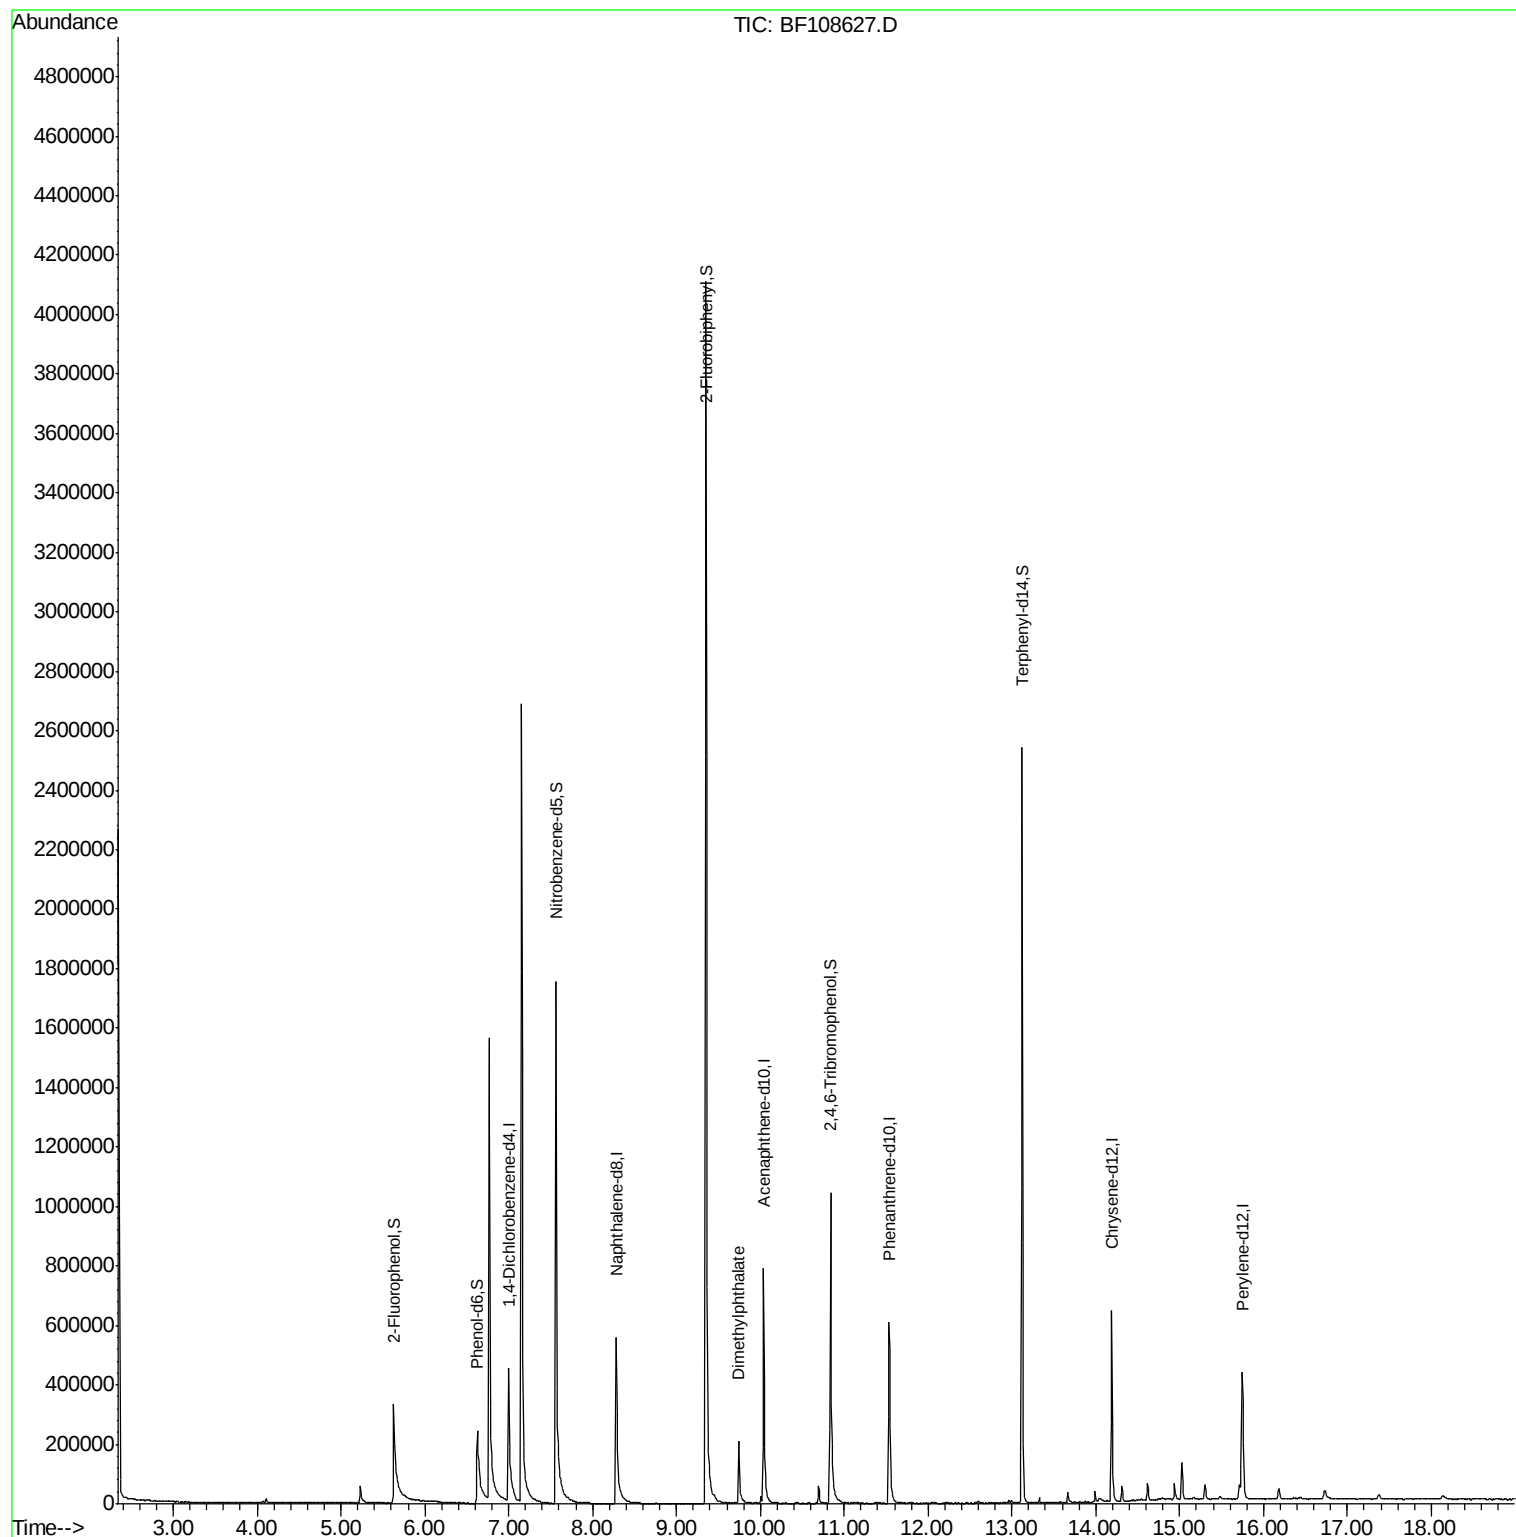







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF108627.D
Acq: 30 Aug 2018 2:33

Instrument :
BNA_F
ClientSampleId :
082718-TIPC-F-U-S




Tot Ion	Ratio	Lower	Upper
152	100		
150	155.9	124.6	186.8
115	57.0	50.1	75.1

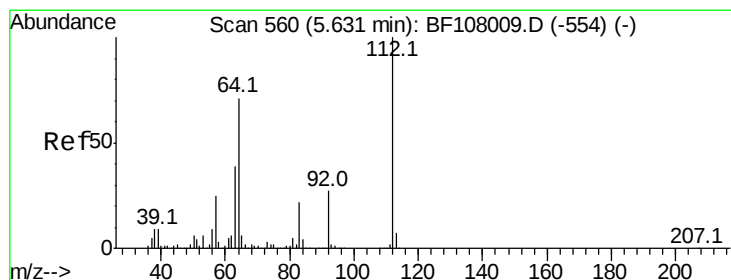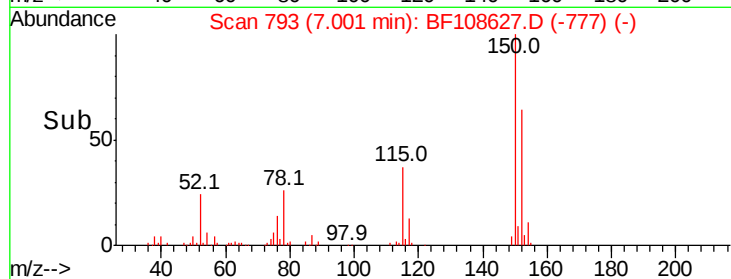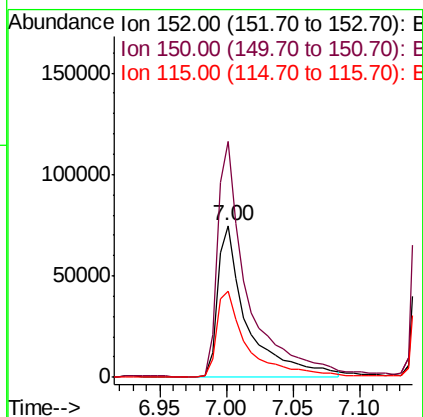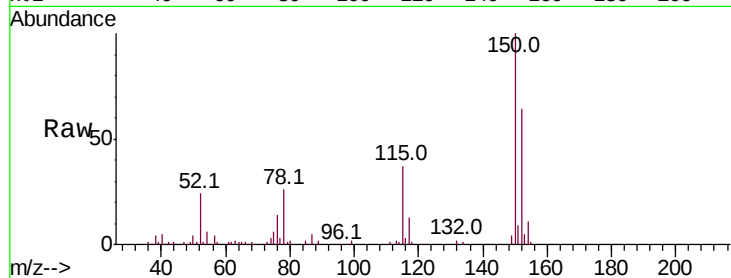

#5

2-Fluorophenol
Concen: 34.129 ng
RT: 5.63 min Scan# 560
Delta R.T. -0.00 min
Lab File: BF108627.D
Acq: 30 Aug 2018 2:33

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.8	47.9	71.9
63	35.3	23.7	35.5

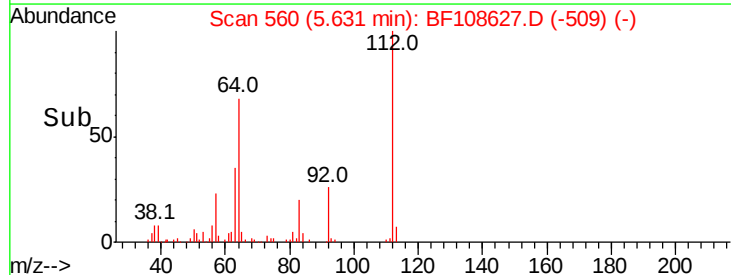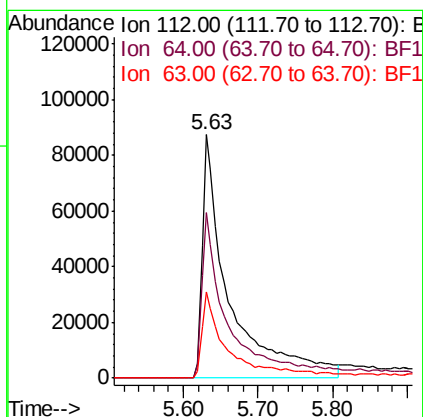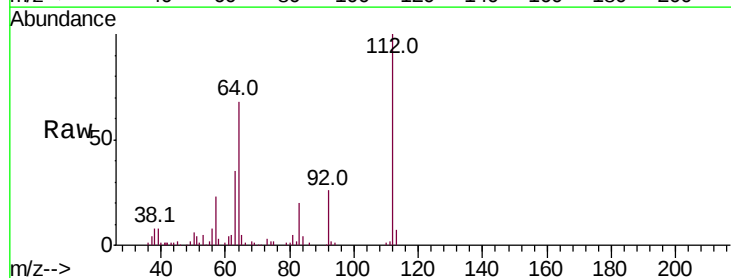



#7

Phenol-d6

Concen: 23.214 ng

RT: 6.62 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF108627.D

Acq: 30 Aug 2018 2:33

Instrument :

BNA_F

ClientSampleId :

082718-TIPC-F-U-S


Tot Ion: 99 Resp: 199273

Ion Ratio Lower Upper




99 100

42 22.1 14.5 21.7#

71 35.3 25.4 38.0

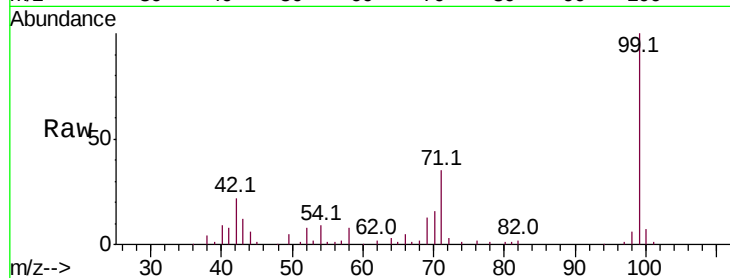

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

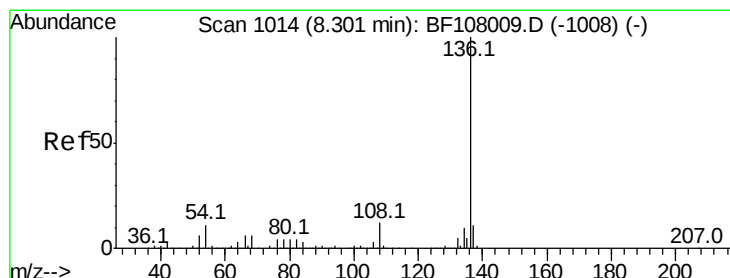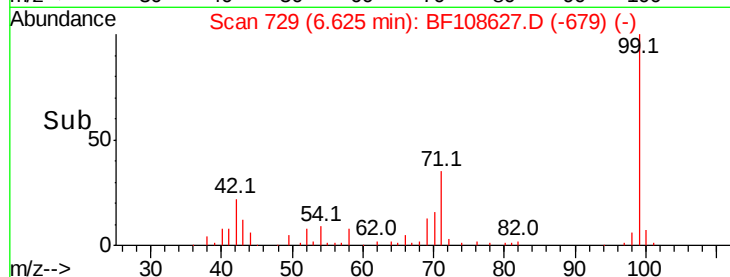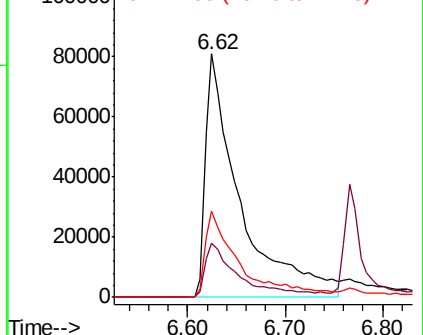

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF108627.D

Acq: 30 Aug 2018 2:33

Tgt Ion: 136 Resp: 438447


Ion Ratio Lower Upper

136 100



137 11.4 8.9 13.3

54 9.1 6.6 9.8

68 5.8 5.0 7.4

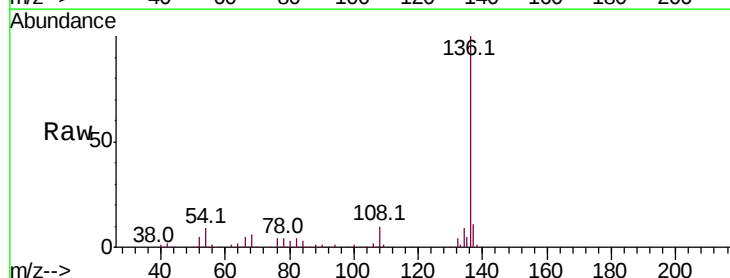

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

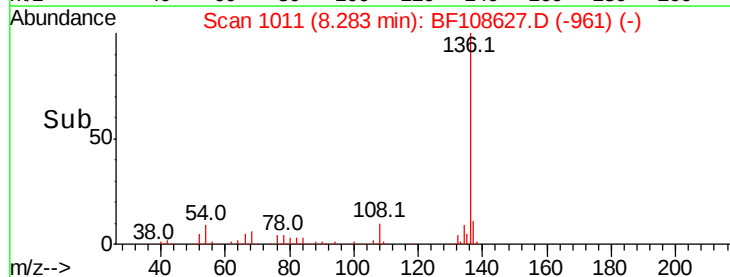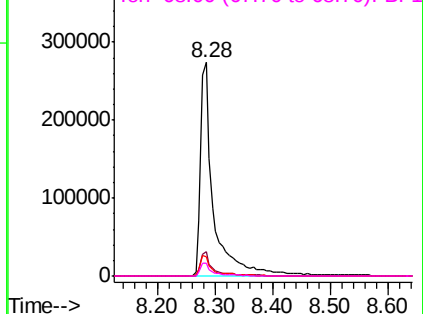






#23
 Nitrobenzene-d5
 Concen: 105.998 ng
 RT: 7.57 min Scan# 889
 Delta R.T. -0.01 min
 Lab File: BF108627.D
 Acq: 30 Aug 2018 2:33

Instrument :
 BNA_F
 ClientSampleId :
 082718-TIPC-F-U-S

Tot Ion	Ratio	Lower	Upper
82	100		
128	42.3	36.1	54.1
54	57.0	41.4	62.2

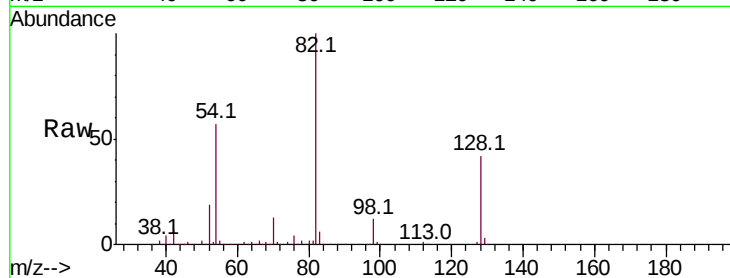


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

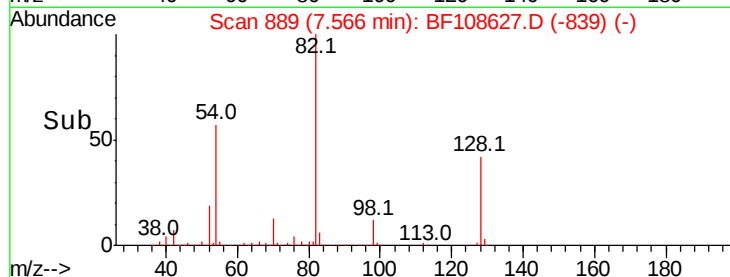
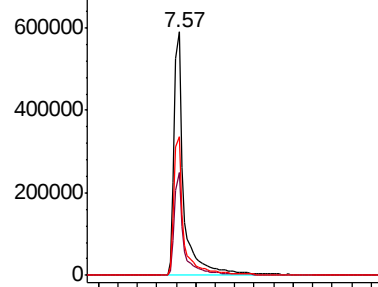


#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.04 min Scan# 1310
 Delta R.T. -0.01 min
 Lab File: BF108627.D
 Acq: 30 Aug 2018 2:33

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.5	86.1	129.1
160	46.5	38.3	57.5

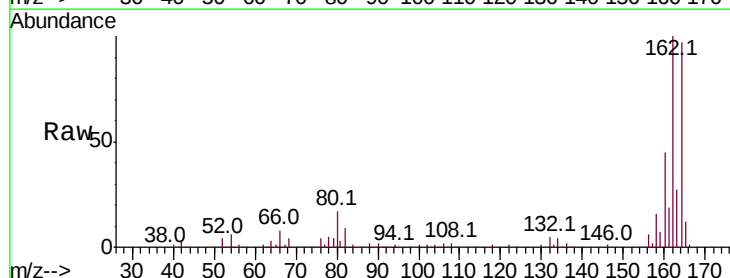

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

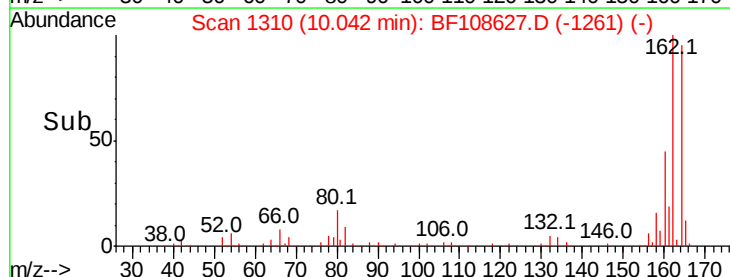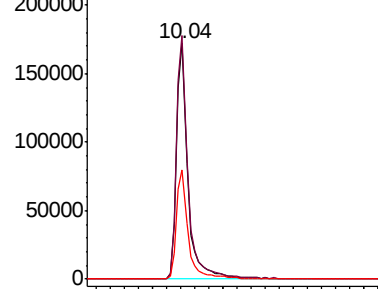






#41
 2,4,6-Tribromophenol
 Concen: 89.231 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108627.D
 Acq: 30 Aug 2018 2:33

Instrument :
 BNA_F
 ClientSampleId :
 082718-TIPC-F-U-S

Tot Ion:330 Resp: 174504
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.0 115.6
 141 33.4 29.9 44.9

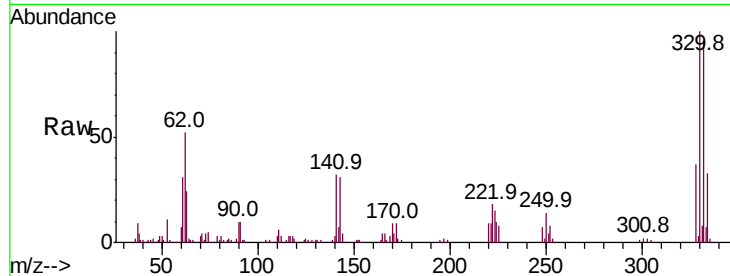


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

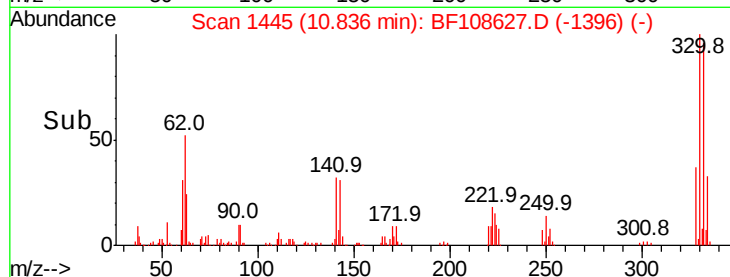
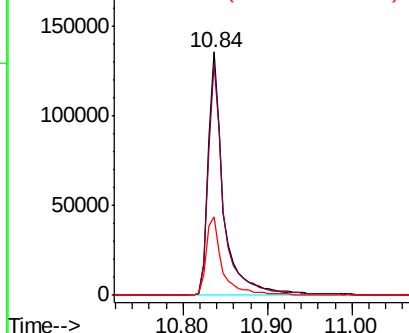


#44
 2-Fluorobiphenyl
 Concen: 122.104 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108627.D
 Acq: 30 Aug 2018 2:33

Tgt Ion:172 Resp: 1491134
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.7 44.5
 170 24.7 19.6 29.4

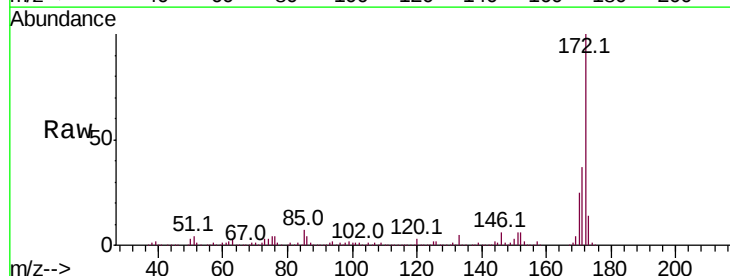

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

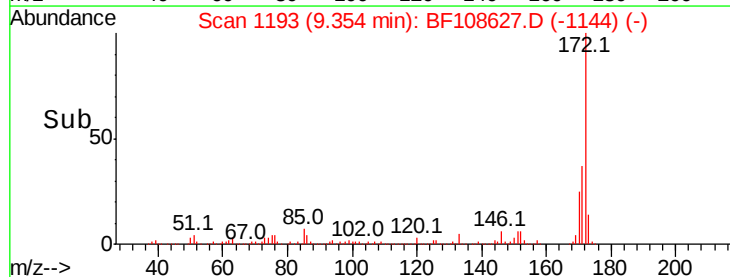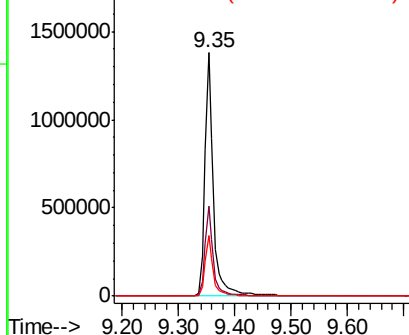



#49

Dimethylphthalate

Concen: 9.712 ng

RT: 9.74 min Scan# 1259

Delta R.T. -0.02 min

Lab File: BF108627.D

Acq: 30 Aug 2018 2:33

Instrument :

BNA_F

ClientSampleId :

082718-TIPC-F-U-S


Tot Ion:163 Resp: 132643

Ion Ratio Lower Upper




163 100

194 3.8 2.7 4.1

164 9.7 8.2 12.2

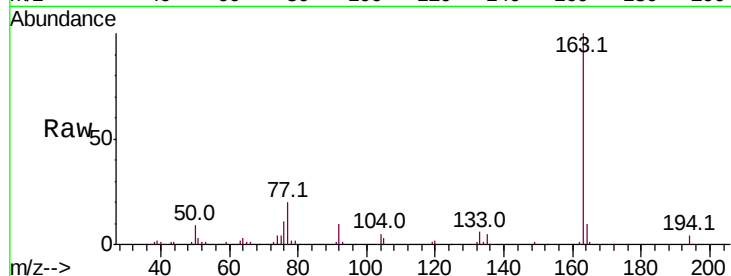

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

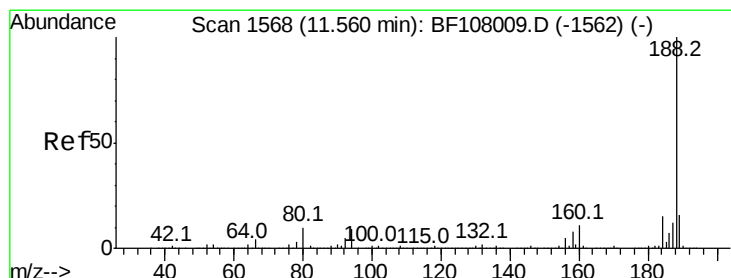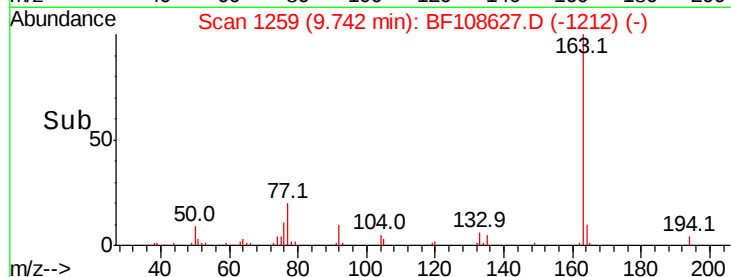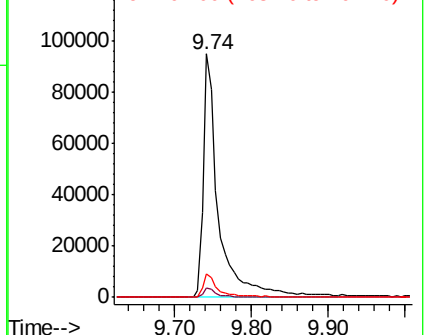

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.54 min Scan# 1564

Delta R.T. -0.01 min

Lab File: BF108627.D

Acq: 30 Aug 2018 2:33


Tgt Ion:188 Resp: 315352

Ion Ratio Lower Upper



188 100


94 8.4 8.5 12.7#

80 9.7 9.2 13.8

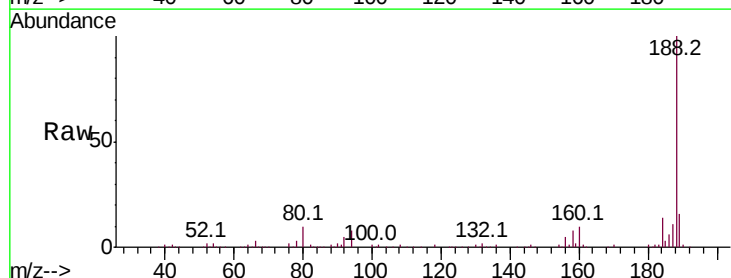

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

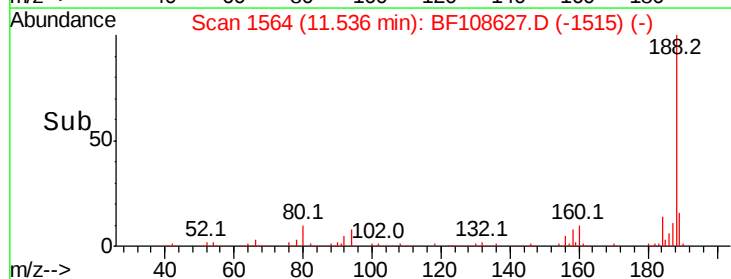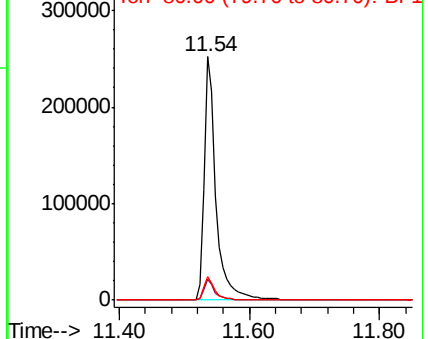

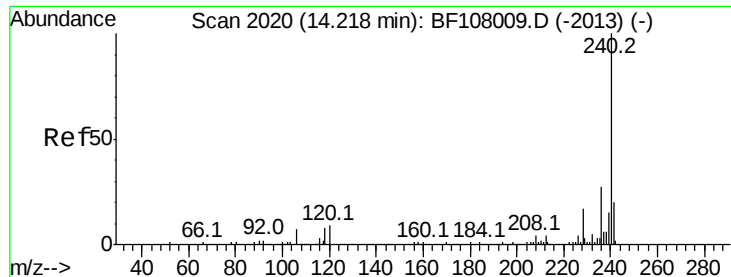

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2015

Delta R.T. -0.01 min

Lab File: BF108627.D

Acq: 30 Aug 2018 2:33

Instrument :

BNA_F

ClientSampleId :

082718-TIPC-F-U-S


Tot Ion:240 Resp: 259461

Ion Ratio Lower Upper

240 100

120 10.3 9.5 14.3



236 25.5 20.7 31.1

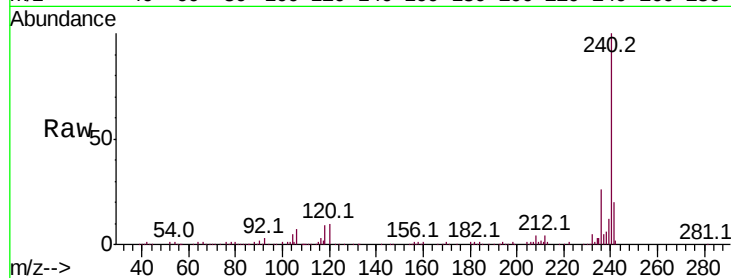

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

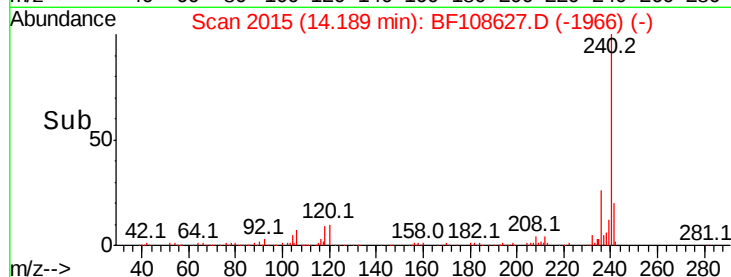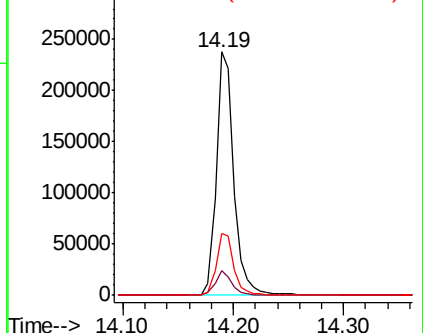

#78

Terphenyl-d14

Concen: 97.968 ng

RT: 13.12 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BF108627.D

Acq: 30 Aug 2018 2:33


Tgt Ion:244 Resp: 999728

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0



122 8.6 11.0 16.4#

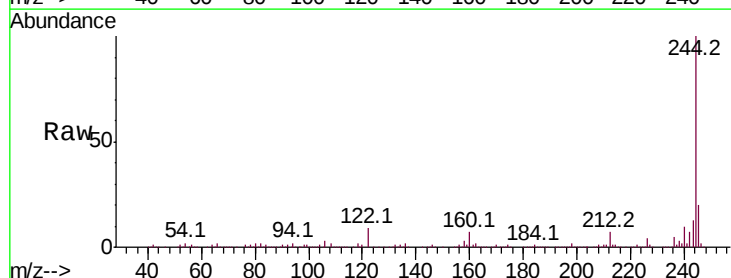


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

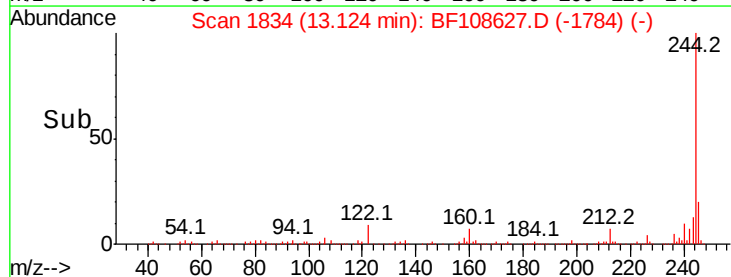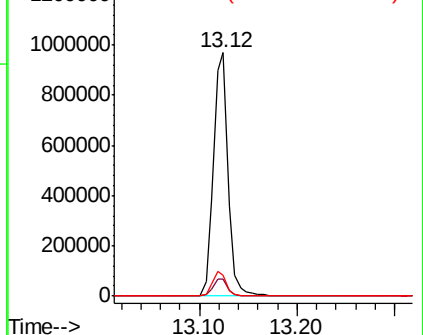

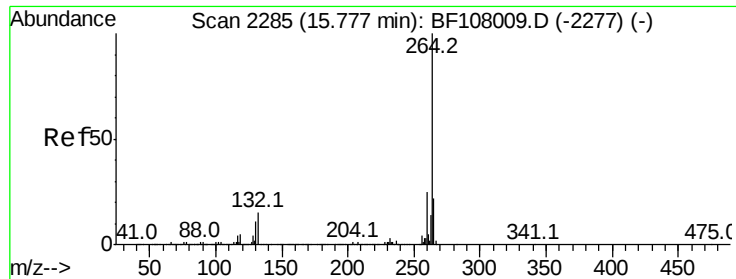

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.75 min Scan# 2280
Delta R.T. -0.01 min
Lab File: BF108627.D
Acq: 30 Aug 2018 2:33

Instrument :
BNA_F
ClientSampleId :
082718-TIPC-F-U-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.2	28.8
265	21.3	17.5	26.3

