


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082918\
 Data File : BF108593.D
 Acq On : 29 Aug 2018 9:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

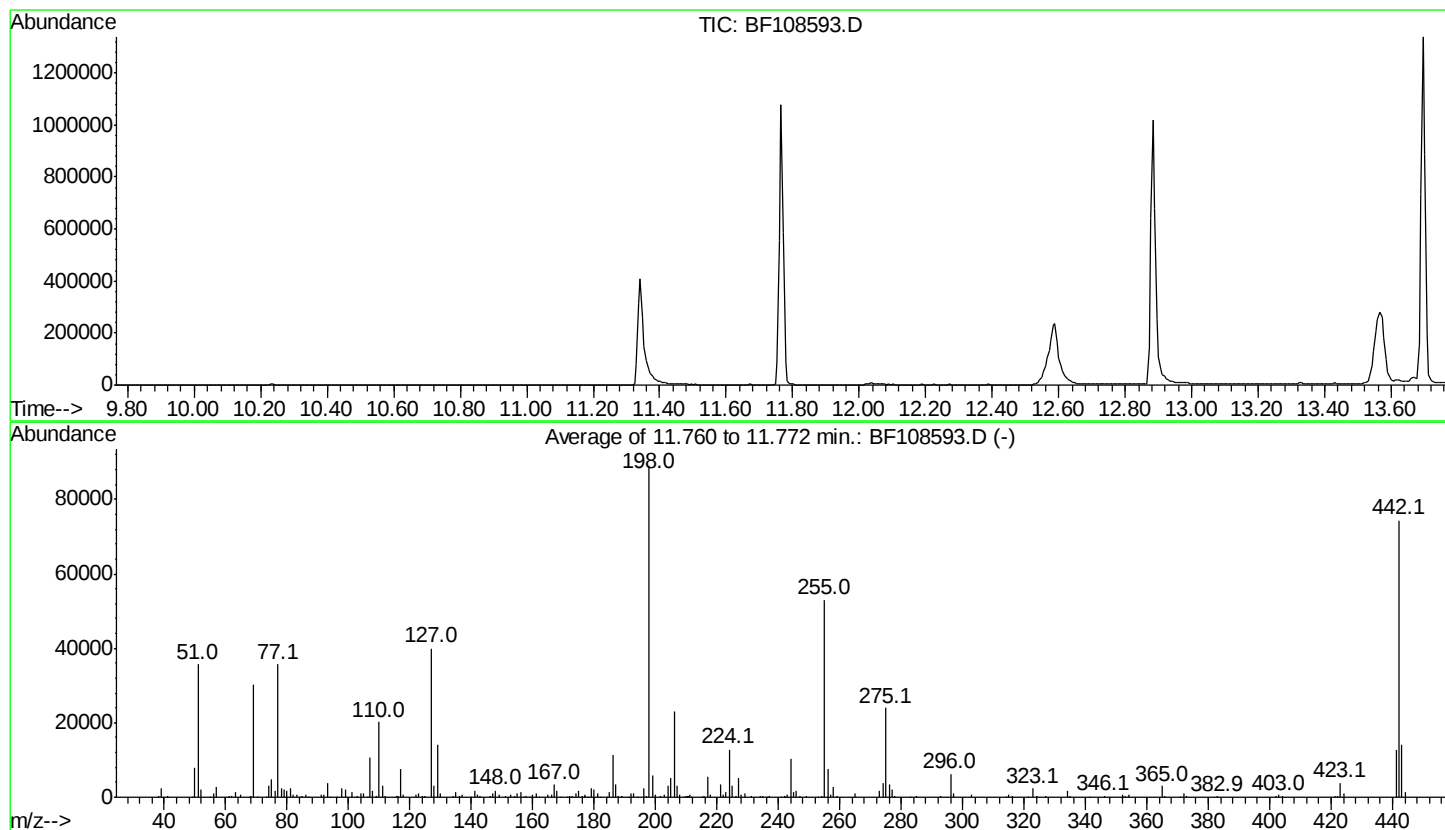

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	35600	PASS
68	69	0.00	2	1.2	360	PASS
69	198	0.00	100	34.2	30421	PASS
70	69	0.00	2	0.5	159	PASS
127	198	10	80	44.8	39893	PASS
197	198	0.00	2	0.6	519	PASS
198	198	100	100	100.0	89066	PASS
199	198	5	9	6.8	6025	PASS
275	198	10	60	27.0	24066	PASS
365	198	1	100	3.4	3063	PASS
441	198	0.01	100	14.1	12598	PASS
442	198	50	100	83.6	74421	PASS
443	442	15	24	18.8	14028	PASS