


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082918\
 Data File : BF108619.D
 Acq On : 29 Aug 2018 22:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

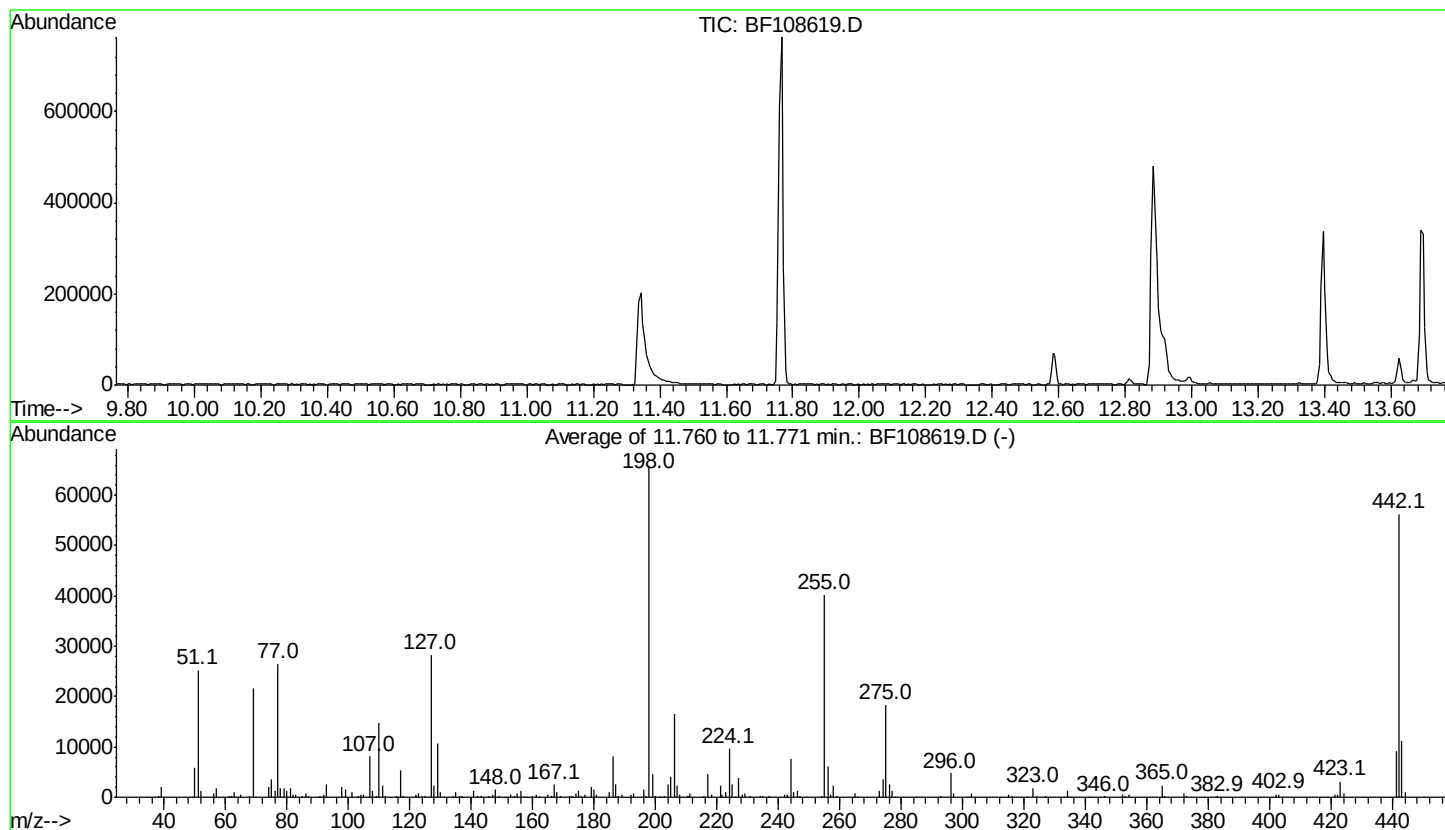

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	25275	PASS
68	69	0.00	2	1.6	335	PASS
69	198	0.00	100	32.8	21606	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	28326	PASS
197	198	0.00	2	0.5	309	PASS
198	198	100	100	100.0	65880	PASS
199	198	5	9	6.8	4470	PASS
275	198	10	60	27.9	18372	PASS
365	198	1	100	3.5	2323	PASS
441	198	0.01	100	14.1	9289	PASS
442	198	50	100	85.5	56336	PASS
443	442	15	24	19.9	11217	PASS