
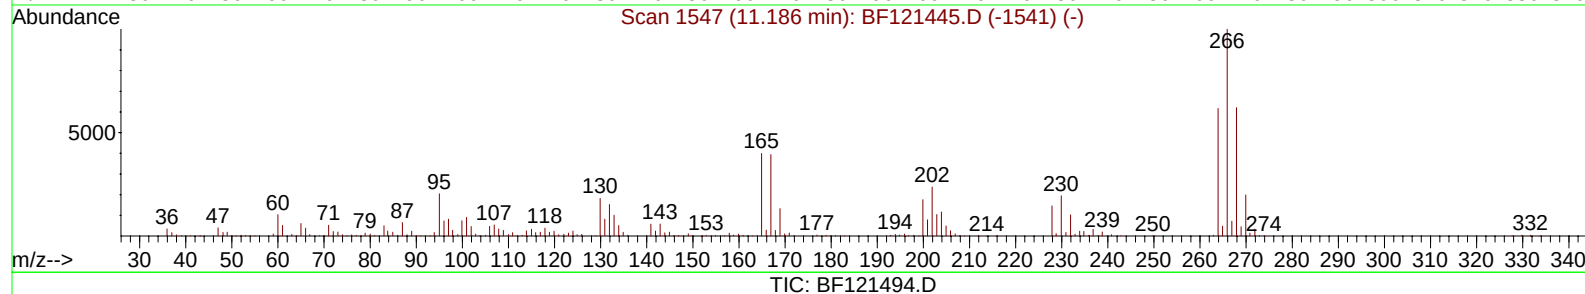
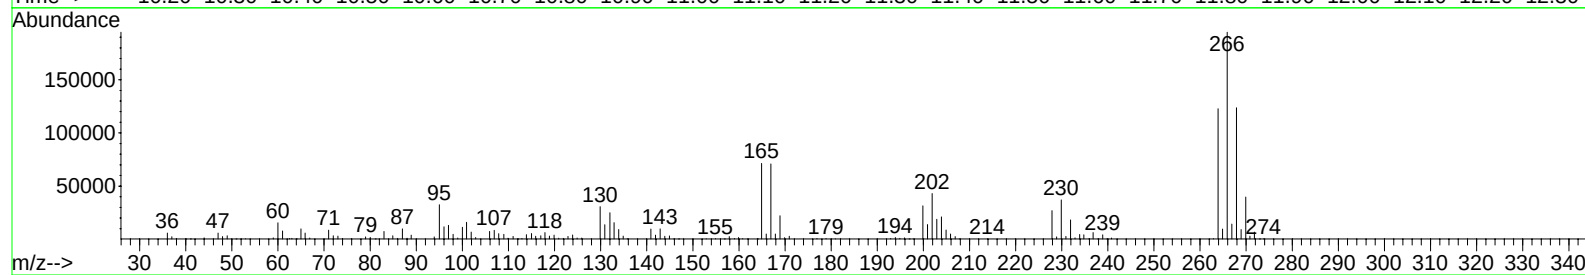


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090120\
Data File : BF121494.D
Acq On : 1 Sep 2020 13:41
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 18:11:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 09:25:49 2020
Response via : Initial Calibration

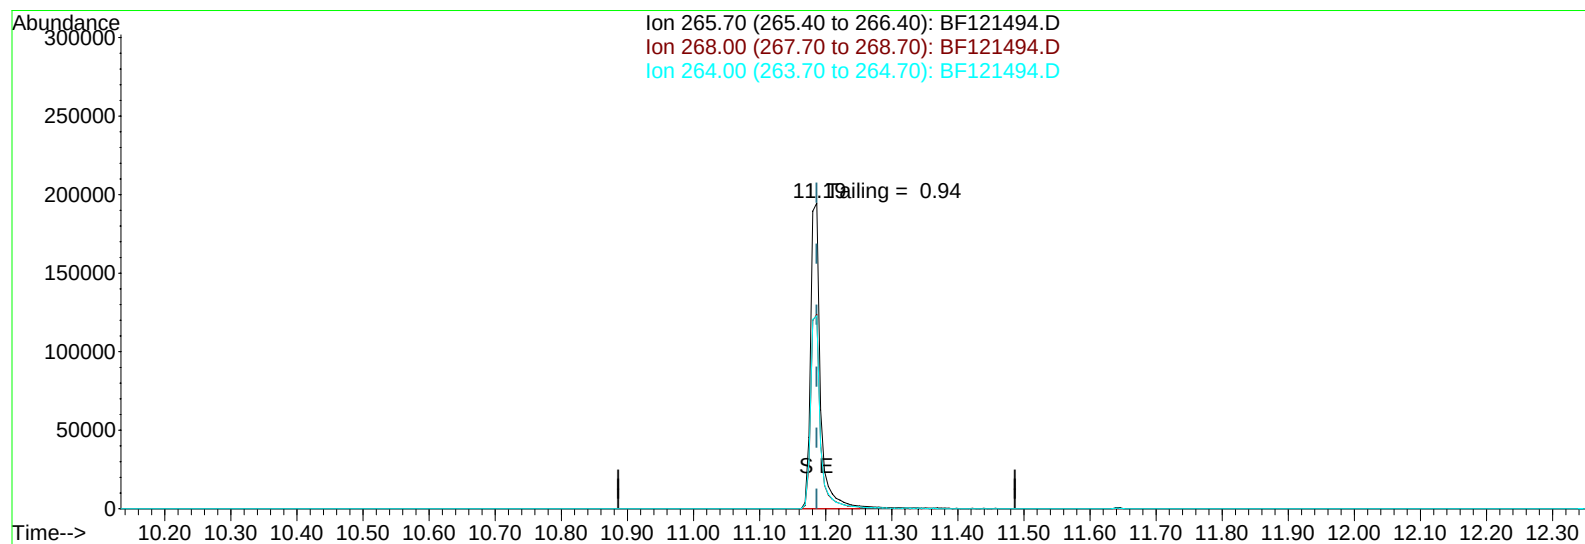

(70) Pentachlorophenol (C)




11.186min (+0.000) 37720.34ng m

response 201067

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	63.50
264.00	61.70	63.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090120\
 Data File : BF121494.D
 Acq On : 1 Sep 2020 13:41
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 18:11:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 28 09:25:49 2020
 Response via : Initial Calibration

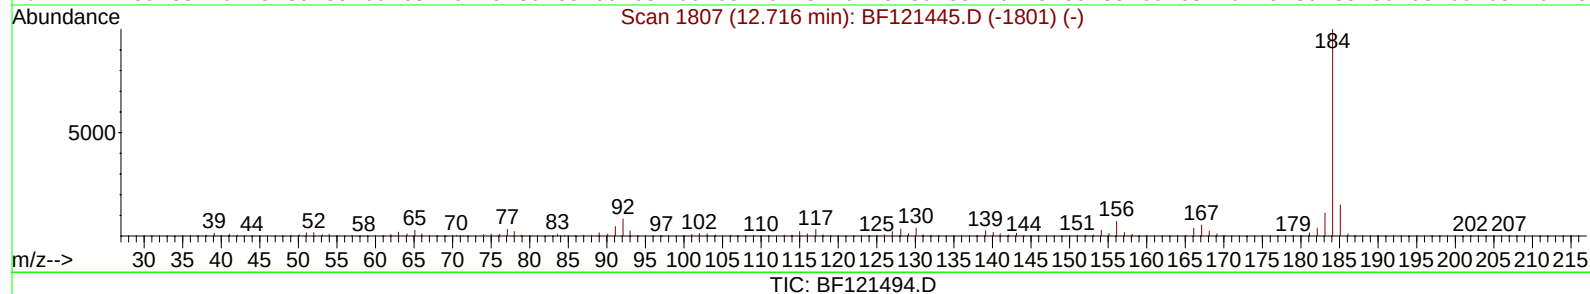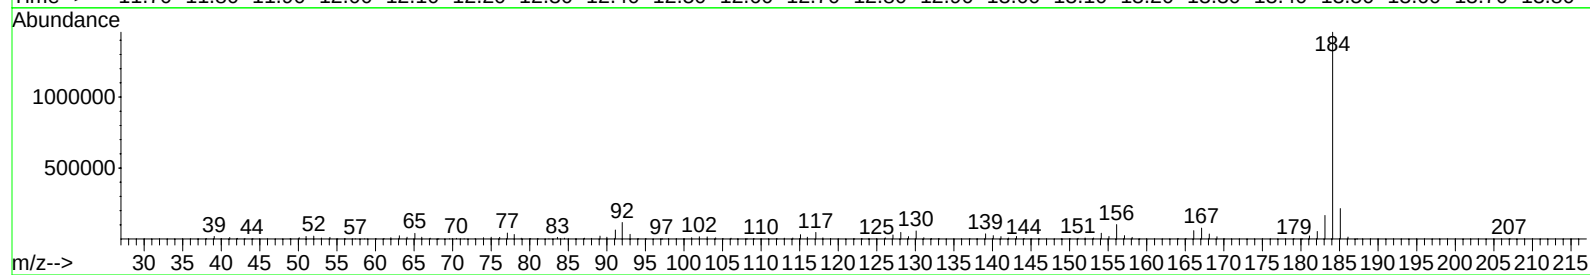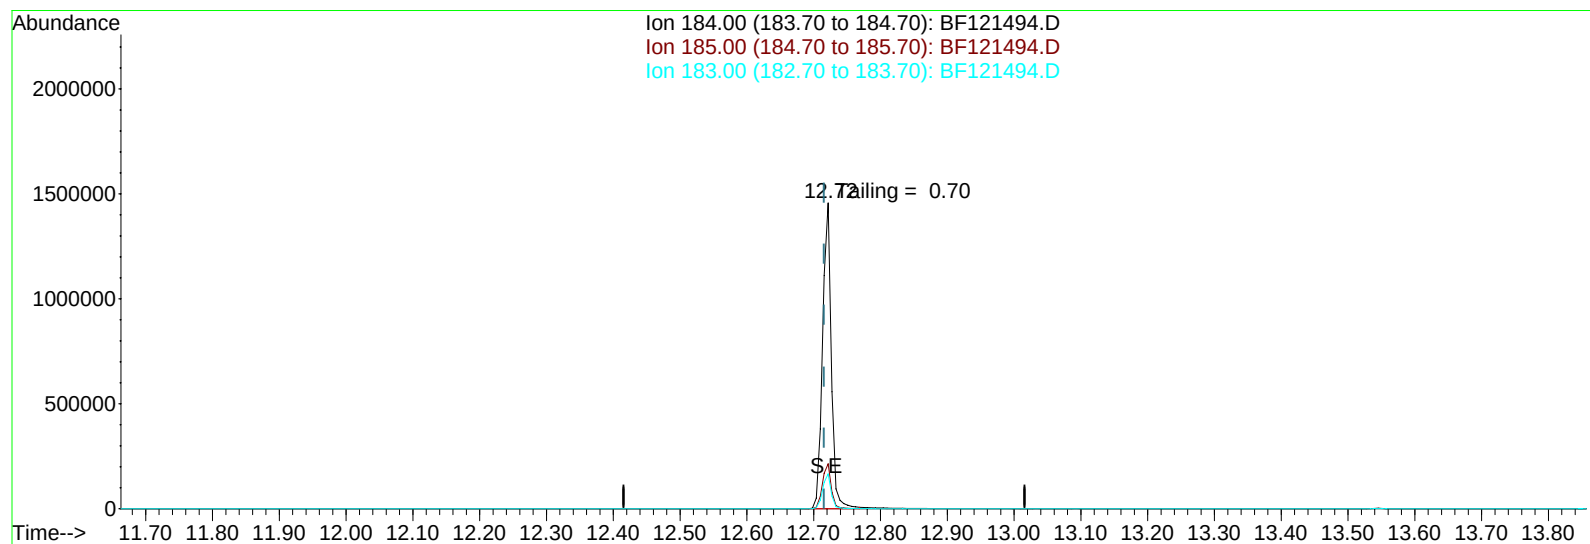

(77) Benzidine

12.722min (+0.006) 0.00ng

response 1344238

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.71
183.00	11.10	11.39
0.00	0.00	0.00