

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090120\
 Data File : BF121506.D
 Acq On : 1 Sep 2020 20:10
 Operator : JU/CG
 Sample : L3848-01 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LINDEN-BH-03-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	502	505	511	rVB	32364	37551	1.59%	0.151%
2	5.463	570	574	585	rVB	1737373	1631885	69.00%	6.568%
3	6.475	742	746	754	rBV	1952222	1713022	72.43%	6.895%
4	6.681	778	781	787	rBV	83518	92893	3.93%	0.374%
5	6.857	807	811	814	rBV	1837202	1584204	66.98%	6.377%
6	7.410	902	905	911	rBV	1222500	1138296	48.13%	4.582%
7	8.139	1025	1029	1035	rBV	2442142	2049301	86.65%	8.249%
8	9.216	1208	1212	1223	rBV	2959824	2365154	100.00%	9.520%
9	9.610	1276	1279	1286	rVB	316022	271569	11.48%	1.093%
10	9.898	1324	1328	1332	rBV	2776280	2275240	96.20%	9.158%
11	10.680	1458	1461	1468	rBV	1338264	1224426	51.77%	4.928%
12	10.804	1479	1482	1487	rBV3	31348	48919	2.07%	0.197%
13	11.280	1561	1563	1569	rVB2	32055	36276	1.53%	0.146%
14	11.386	1577	1581	1583	rBV	2478585	2158645	91.27%	8.689%
15	11.410	1583	1585	1588	rVV	232002	197402	8.35%	0.795%
16	11.457	1591	1593	1597	rVB	53403	47544	2.01%	0.191%
17	11.886	1663	1666	1668	rBV	52231	48148	2.04%	0.194%
18	11.910	1668	1670	1675	rVB2	205149	192170	8.13%	0.773%
19	11.998	1682	1685	1687	rBV	73248	74717	3.16%	0.301%
20	12.180	1714	1716	1719	rBV	40439	48375	2.05%	0.195%
21	12.439	1757	1760	1762	rBV	61531	65890	2.79%	0.265%
22	12.474	1763	1766	1768	rVV3	53160	60517	2.56%	0.244%
23	12.522	1771	1774	1778	rBV3	43184	52665	2.23%	0.212%
24	12.598	1784	1787	1790	rBV	419892	341136	14.42%	1.373%
25	12.692	1801	1803	1806	rBV3	33361	36970	1.56%	0.149%
26	12.827	1821	1826	1828	rBV	408360	390157	16.50%	1.570%
27	12.969	1847	1850	1856	rVB	2471556	2135589	90.29%	8.596%
28	13.874	2001	2004	2011	rBV2	399700	550134	23.26%	2.214%
29	14.027	2025	2030	2033	rBV	2183479	2110693	89.24%	8.496%
30	14.051	2033	2034	2036	rVB	185354	94021	3.98%	0.378%
31	15.504	2277	2281	2285	rBV	1498281	1770847	74.87%	7.128%


Sum of corrected areas: 24844356

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090120\
Data File : BF121506.D
Acq On : 1 Sep 2020 20:10
Operator : JU/CG
Sample : L3848-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LINDEN-BH-03-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

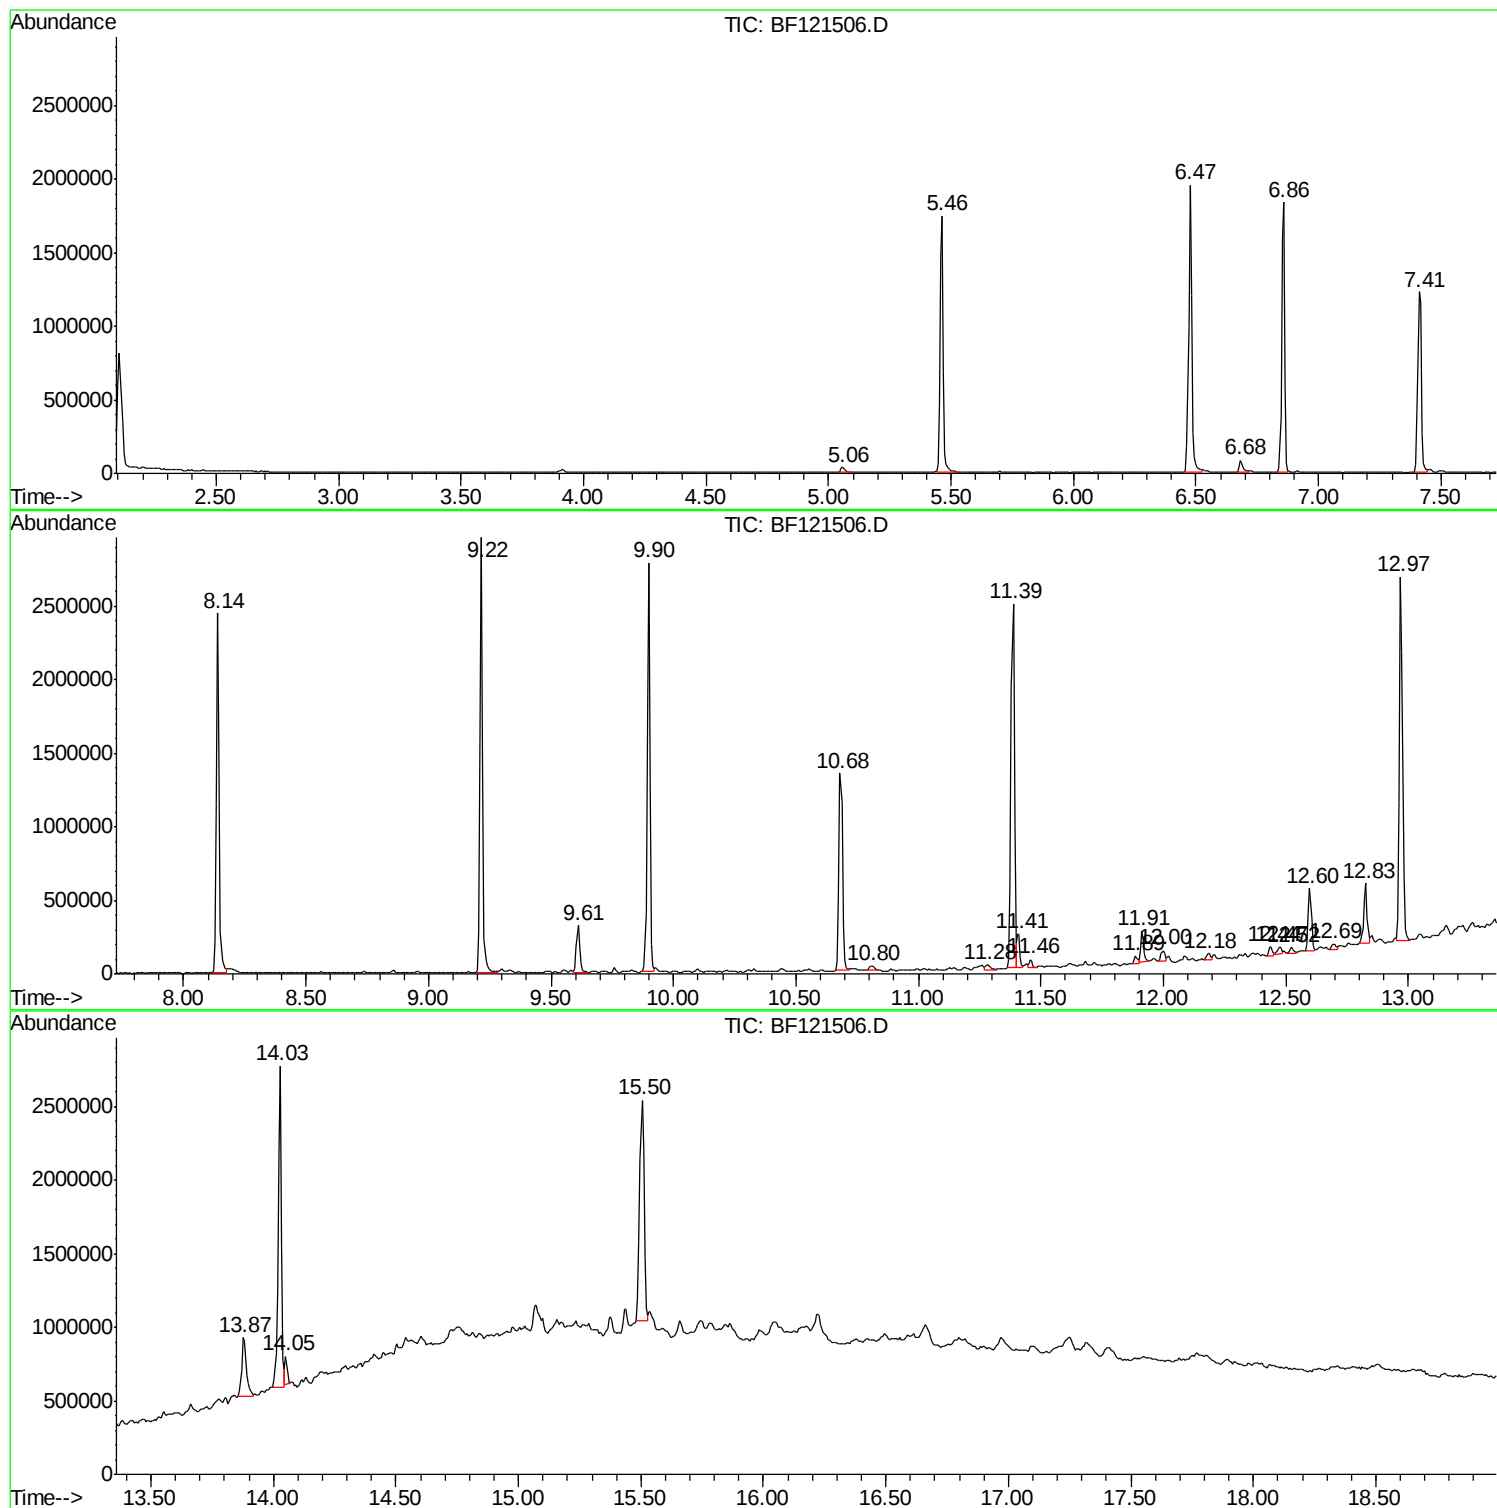

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090120\
Data File : BF121506.D
Acq On : 1 Sep 2020 20:10
Operator : JU/CG
Sample : L3848-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LINDEN-BH-03-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Heptadecyl heptafluorobutyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.87	5.21 ng	550134	Chrysene-d12	14.03

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
2		1-Heneicosyl formate	340	C22H44O2	077899-03-7	94
3		Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
4		Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
5		Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	91

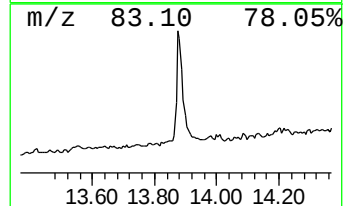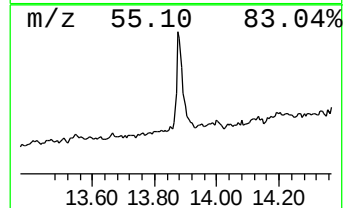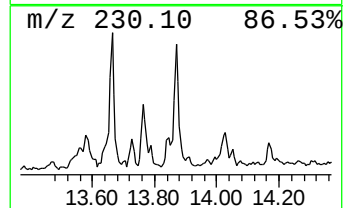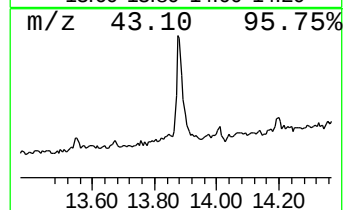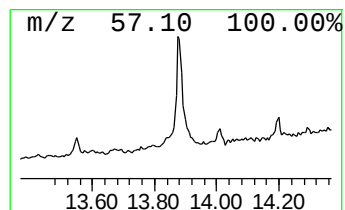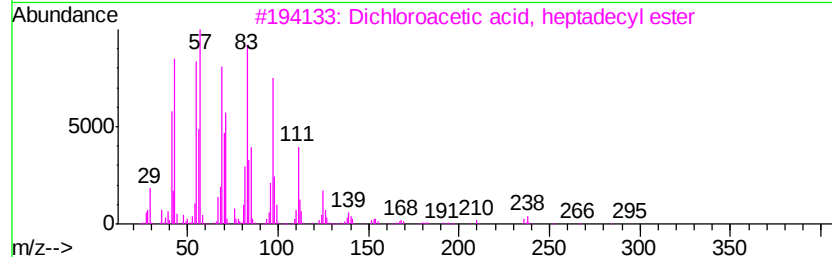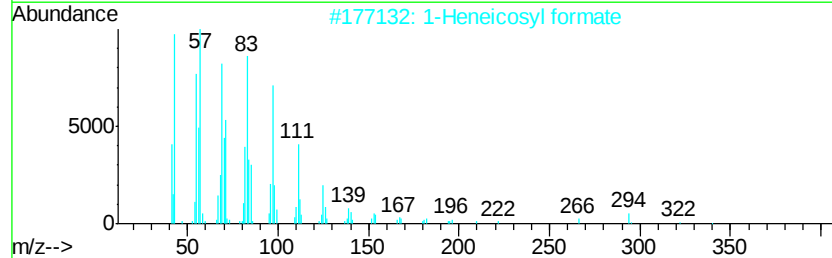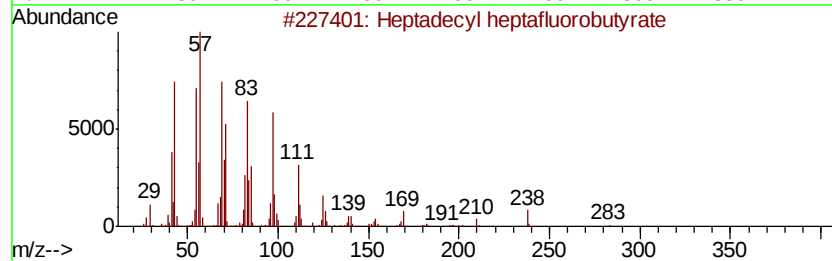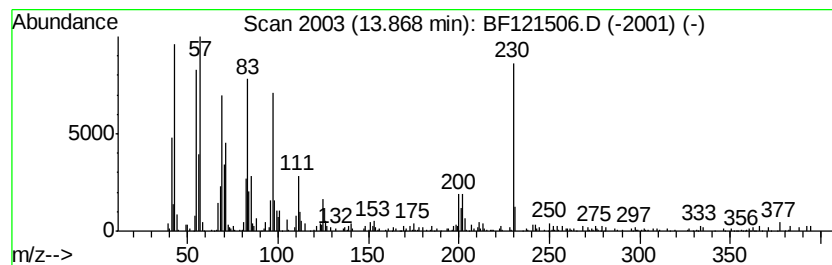

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090120\
Data File : BF121506.D
Acq On : 1 Sep 2020 20:10
Operator : JU/CG
Sample : L3848-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LINDEN-BH-03-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Heptadecyl heptaf...	13.87	5.2	ng	550134	5	14.03	2110690	20.0