


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090120\
 Data File : BF121494.D
 Acq On : 1 Sep 2020 13:41
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 28 09:25:49 2020

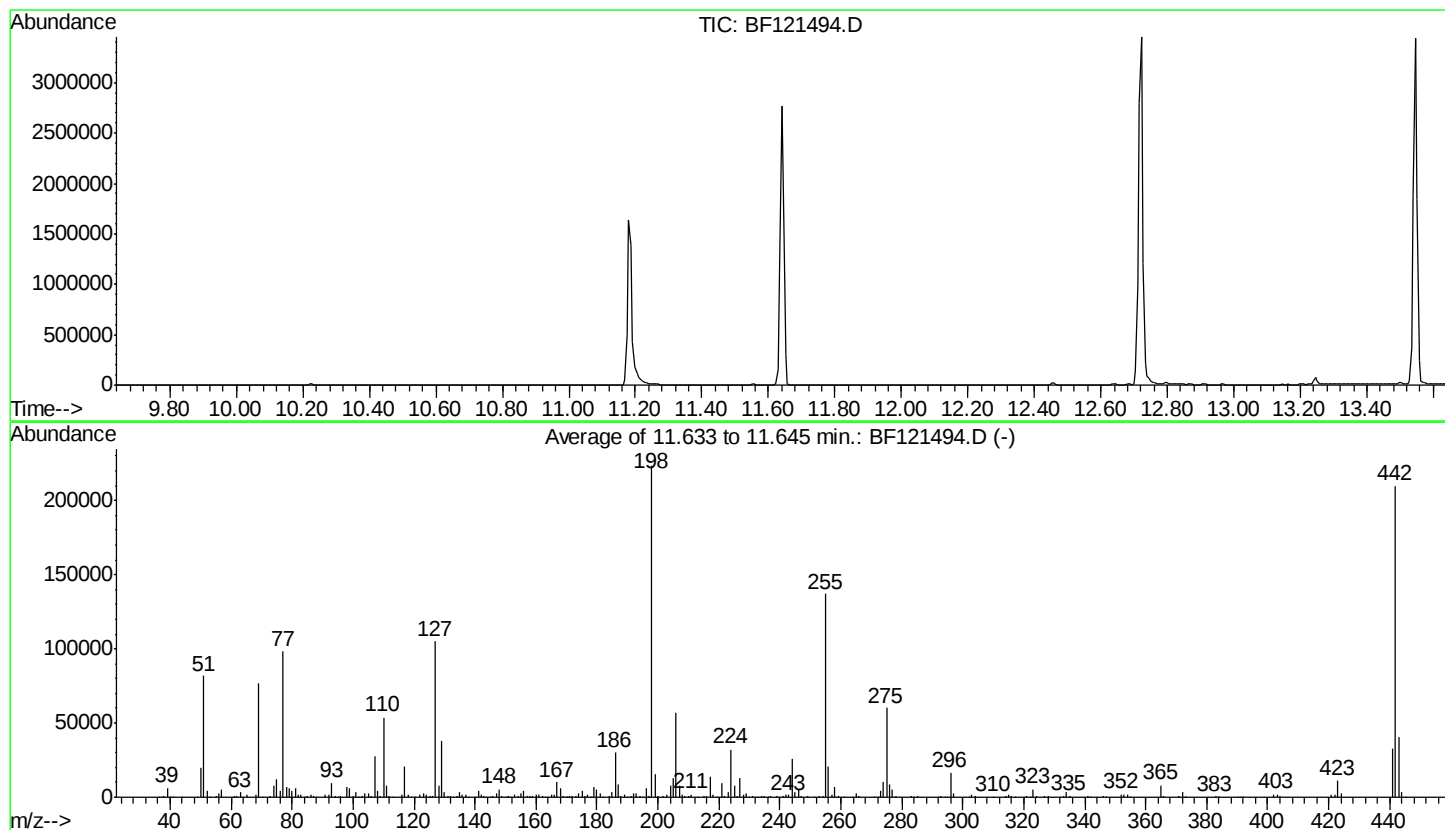

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	81941	PASS
68	69	0.00	2	1.8	1403	PASS
69	198	0.00	100	34.2	76501	PASS
70	69	0.00	2	0.4	315	PASS
127	198	10	80	47.1	105194	PASS
197	198	0.00	2	0.5	1219	PASS
198	198	100	100	100.0	223477	PASS
199	198	5	9	6.8	15291	PASS
275	198	10	60	26.9	60125	PASS
365	198	1	100	3.5	7927	PASS
441	198	0.01	100	14.8	32980	PASS
442	198	50	100	94.0	209970	PASS
443	442	15	24	19.3	40457	PASS