
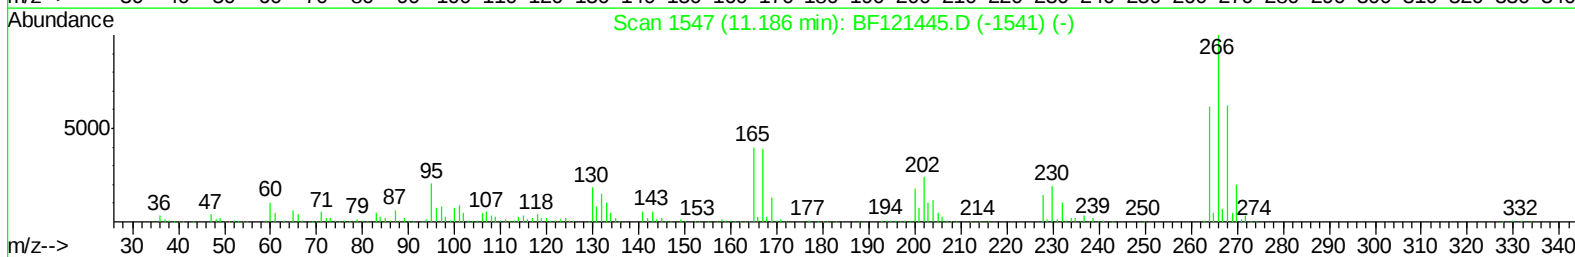
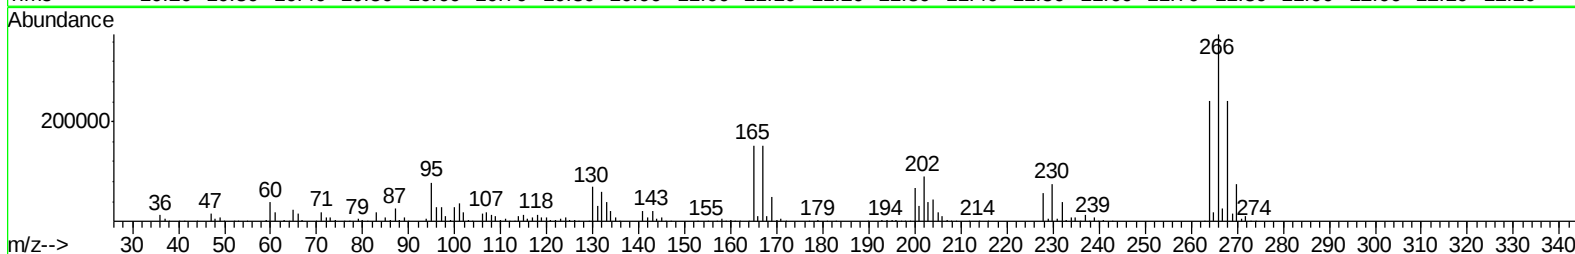


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090220\
Data File : BF121514.D
Acq On : 2 Sep 2020 14:49
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 08:26:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 17:52:18 2020
Response via : Initial Calibration

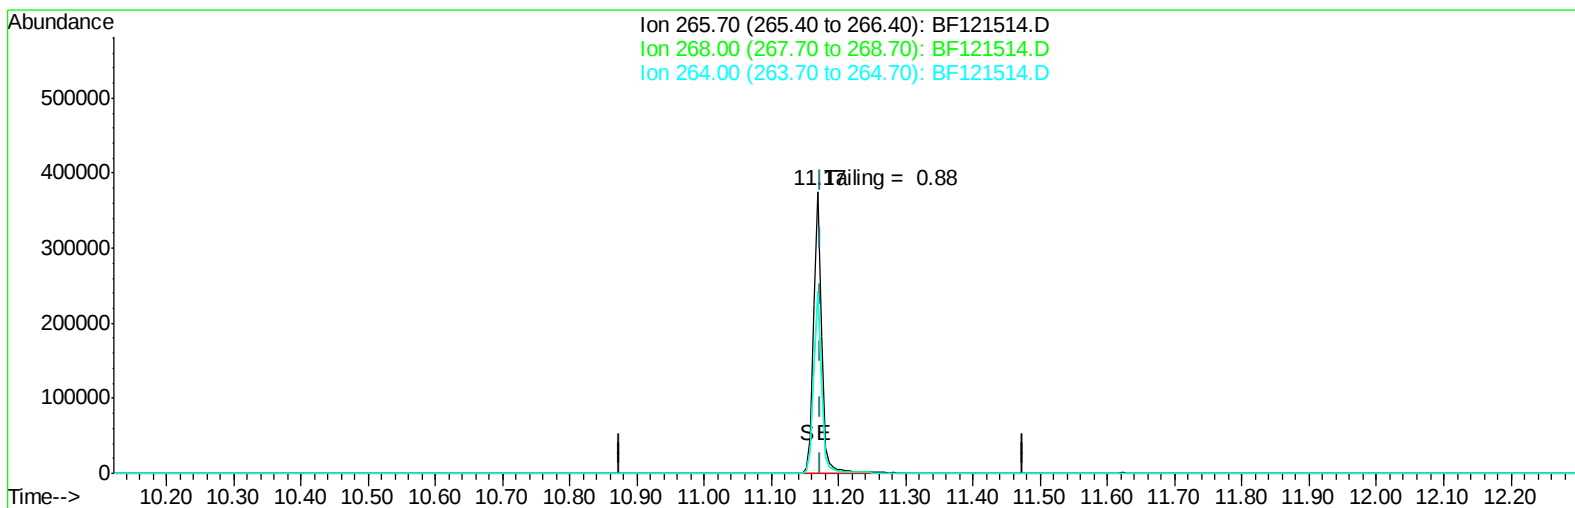

TIC: BF121514.D

(70) Pentachlorophenol (C)




11.169min (-0.006) 367196.79ng

response 328020

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.77
264.00	62.60	64.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090220\
 Data File : BF121514.D
 Acq On : 2 Sep 2020 14:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 08:26:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 17:52:18 2020
 Response via : Initial Calibration

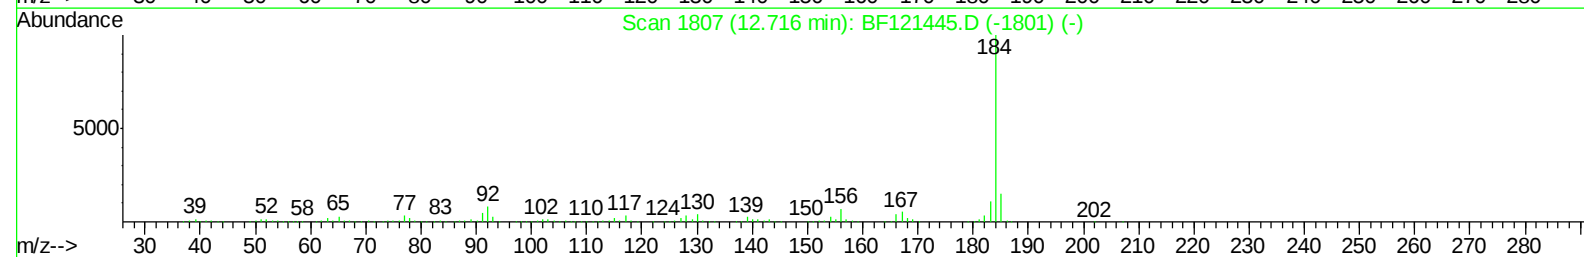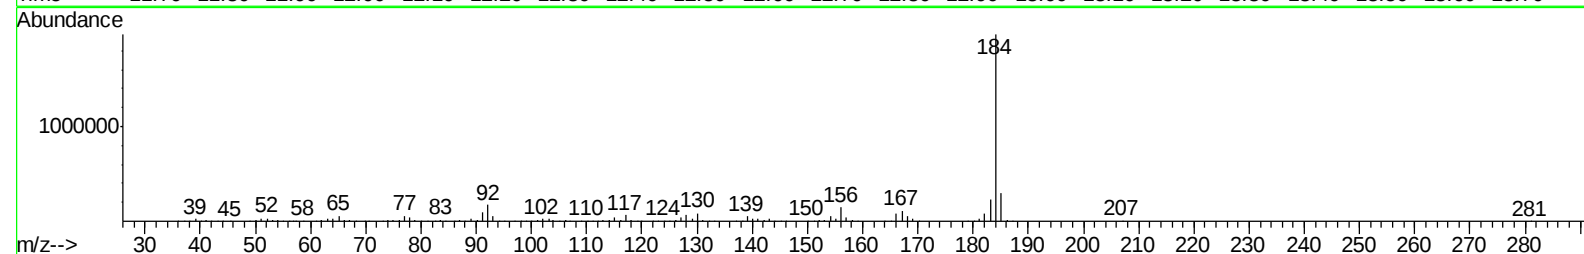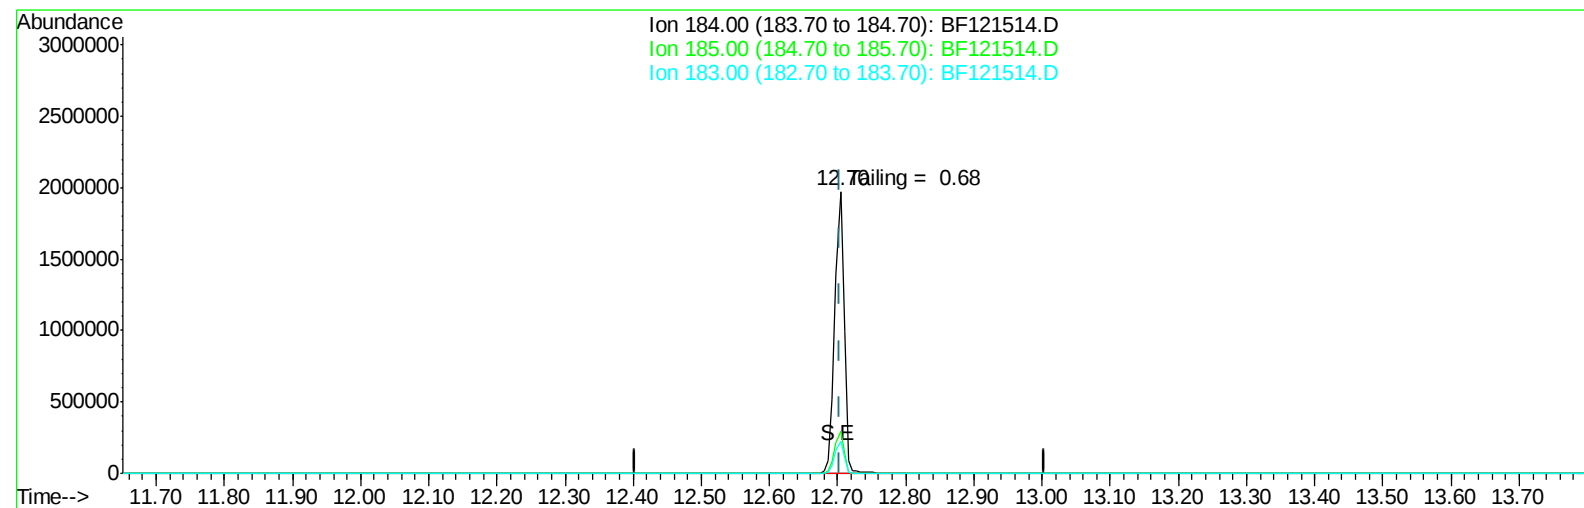

TIC: BF121514.D

(77) Benzidine

12.704min (+0.000) 78010.35ng

response 1822150

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	15.03
183.00	11.30	11.56
0.00	0.00	0.00