


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090220\
 Data File : BF121514.D
 Acq On : 2 Sep 2020 14:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 17:52:18 2020

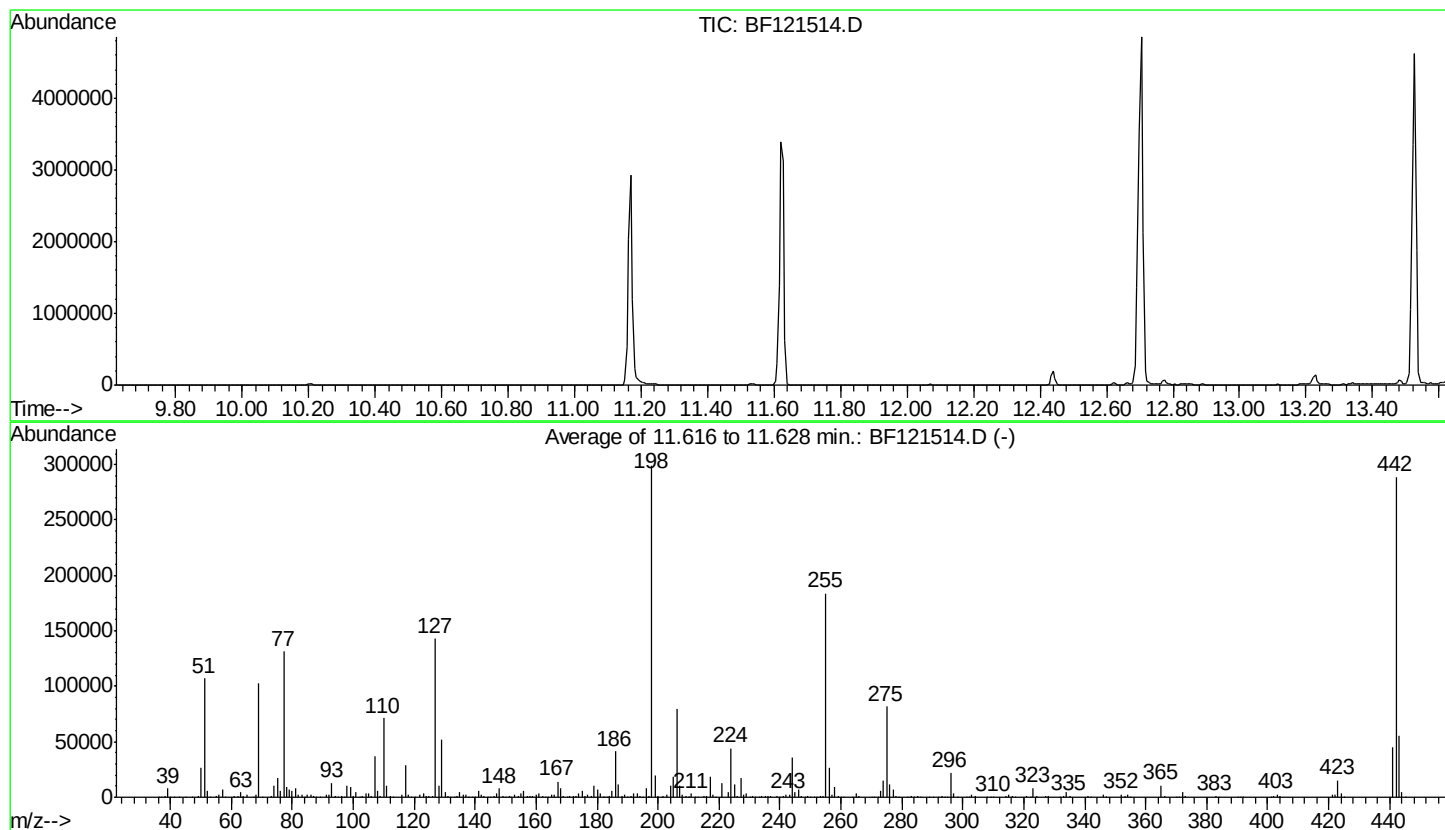

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	107128	PASS
68	69	0.00	2	1.8	1826	PASS
69	198	0.00	100	34.2	102234	PASS
70	69	0.00	2	0.6	583	PASS
127	198	10	80	47.8	142880	PASS
197	198	0.00	2	0.5	1620	PASS
198	198	100	100	100.0	299072	PASS
199	198	5	9	6.7	20100	PASS
275	198	10	60	27.4	81861	PASS
365	198	1	100	3.6	10710	PASS
441	198	0.01	100	15.0	44832	PASS
442	198	50	100	96.7	289136	PASS
443	442	15	24	19.3	55859	PASS