

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091319\
 Data File : BF117043.D
 Acq On : 14 Sep 2019 00:38
 Operator : HP/JU
 Sample : K4863-04 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CSA-4-6

Quant Time: Sep 14 01:41:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 13 16:23:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	62943	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	276082	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	137039	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	181190	20.00	ng	0.00
76) Chrysene-d12	13.96	240	129782	20.00	ng	-0.01
87) Perylene-d12	15.41	264	109943	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	4025	1.00	ng	0.00
7) Phenol-d6	6.46	99	7069	1.36	ng	0.00
23) Nitrobenzene-d5	7.39	82	3561	0.68	ng	0.00
42) 2,4,6-Tribromophenol	10.65	330	1007	0.88	ng	0.00
45) 2-Fluorobiphenyl	9.18	172	10990	1.25	ng	0.00
79) Terphenyl-d14	12.91	244	7748	1.12	ng	0.00
Target Compounds						
51) 2,6-Dinitrotoluene	9.85	165	17657	8.935	ng	# 24
57) 2,4-Dinitrotoluene	9.85	165	17657	6.883	ng	# 18

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091319\
Data File : BF117043.D
Acq On : 14 Sep 2019 00:38
Operator : HP/JU
Sample : K4863-04 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CSA-4-6

Quant Time: Sep 14 01:41:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

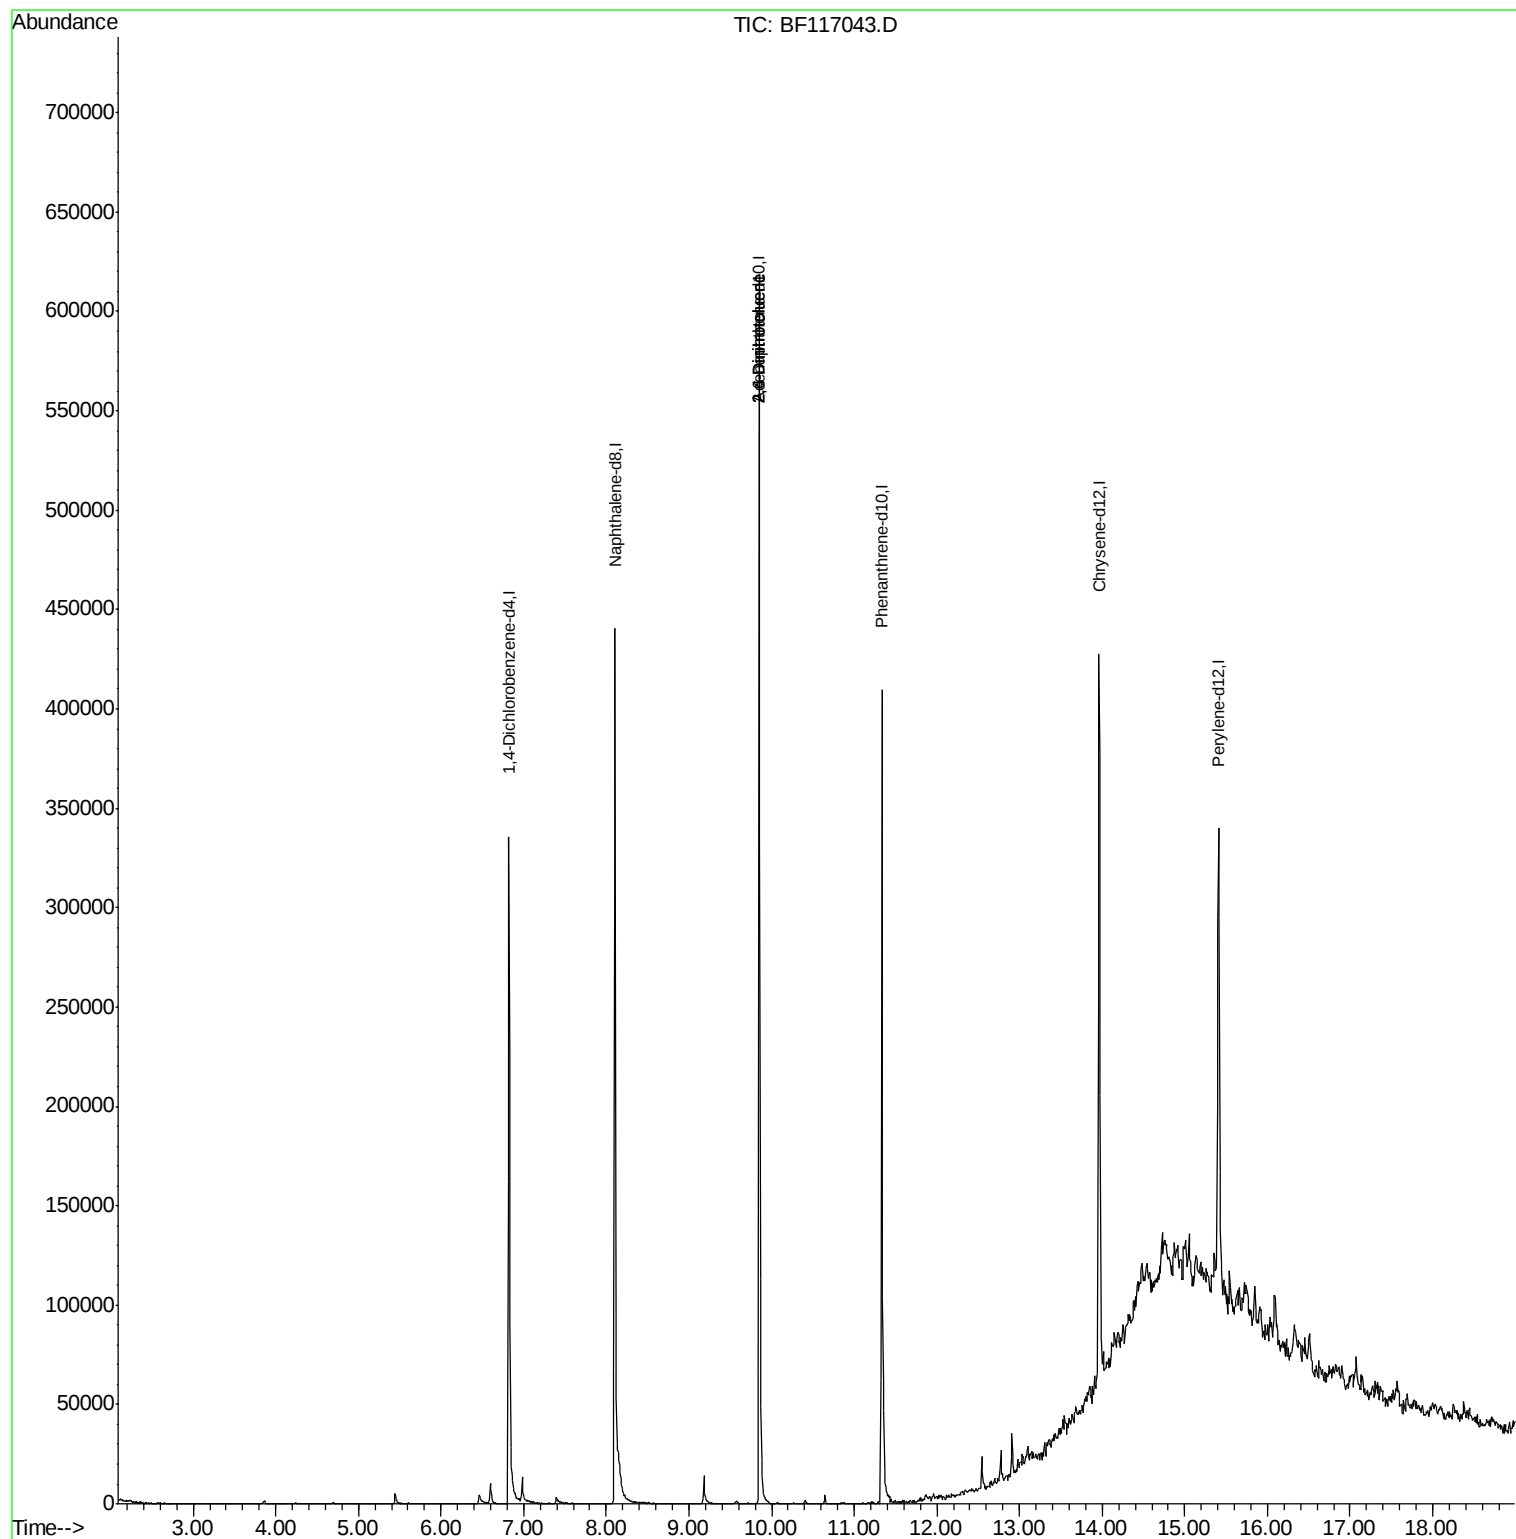




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. 0.00 min
Lab File: BF117043.D
Acq: 14 Sep 2019 00:38

Instrument :
BNA_F
ClientSampleId :
CSA-4-6

Tot Ion:152 Resp: 62943
Ion Ratio Lower Upper
152 100
150 157.3 127.5 191.3
115 64.7 55.0 82.4

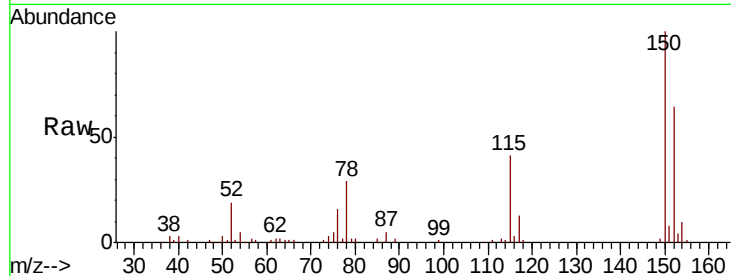


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

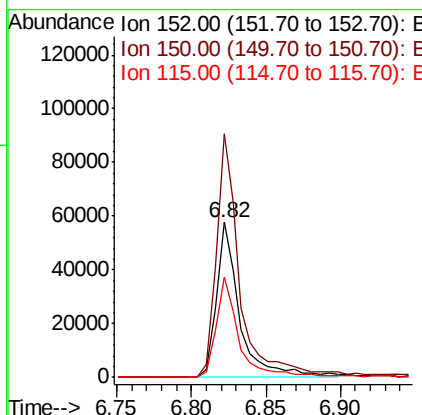



#5

2-Fluorophenol
Concen: 0.998 ng
RT: 5.45 min Scan# 571
Delta R.T. 0.01 min
Lab File: BF117043.D
Acq: 14 Sep 2019 00:38

Tgt Ion:112 Resp: 4025
Ion Ratio Lower Upper
112 100
64 38.5 45.7 68.5#
63 37.0 24.9 37.3

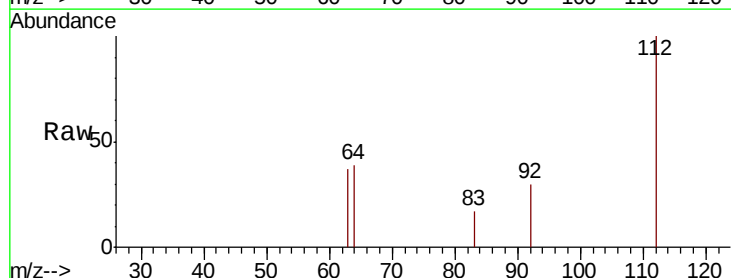

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

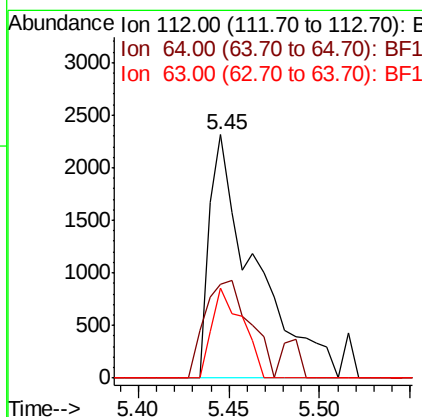



#7

Phenol-d6

Concen: 1.357 ng

RT: 6.46 min Scan# 744

Delta R.T. 0.01 min

Lab File: BF117043.D

Acq: 14 Sep 2019 00:38

Instrument :


BNA_F

ClientSampleId :




CSA-4-6

Tot Ion: 99 Resp: 7069

Ion	Ratio	Lower	Upper
99	100		
42	11.9	12.2	18.2#
71	34.6	29.8	44.8

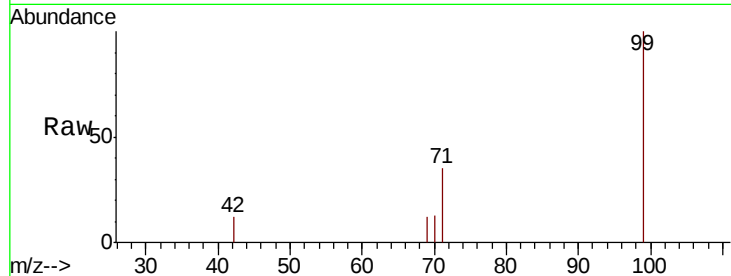

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

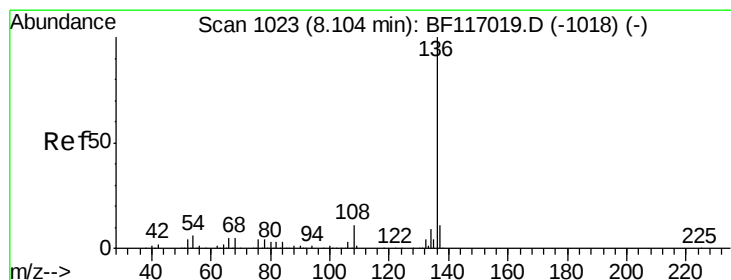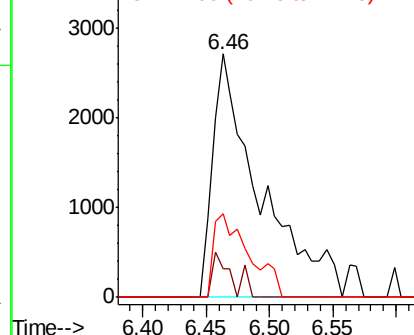

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1023


Delta R.T. 0.00 min

Lab File: BF117043.D



Acq: 14 Sep 2019 00:38

Tgt Ion: 136 Resp: 276082

Ion	Ratio	Lower	Upper
136	100		
137	10.3	9.0	13.4
54	5.3	4.5	6.7
68	4.8	4.0	6.0

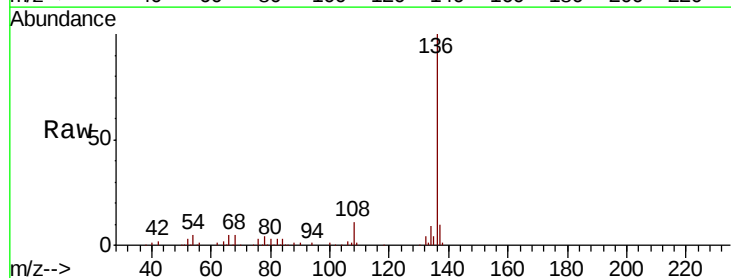

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1




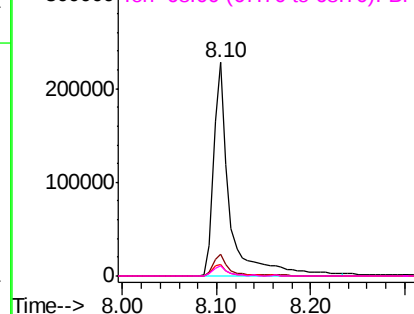




#23
 Nitrobenzene-d5
 Concen: 0.678 ng
 RT: 7.39 min Scan# 902
 Delta R.T. 0.01 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38




Instrument :
 BNA_F
 ClientSampled :
 CSA-4-6

Tot Ion: 82 Resp: 3561
 Ion Ratio Lower Upper
 82 100
 128 42.3 32.3 48.5
 54 39.4 33.3 49.9

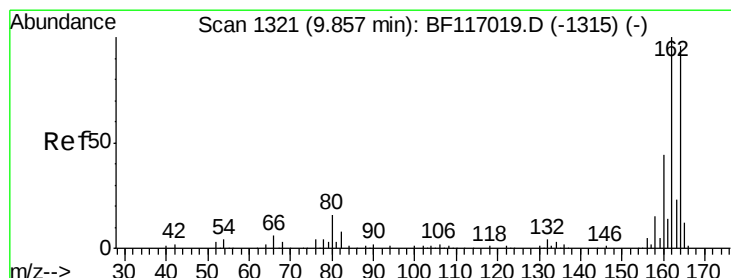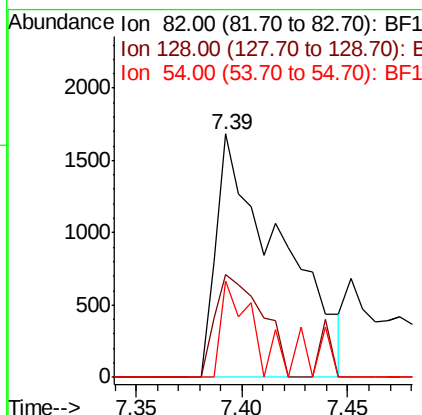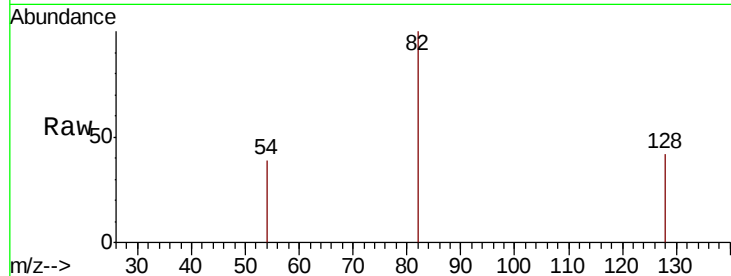

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. -0.01 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38

Tgt Ion: 164 Resp: 137039
 Ion Ratio Lower Upper
 164 100
 162 100.7 83.4 125.2
 160 44.0 36.4 54.6

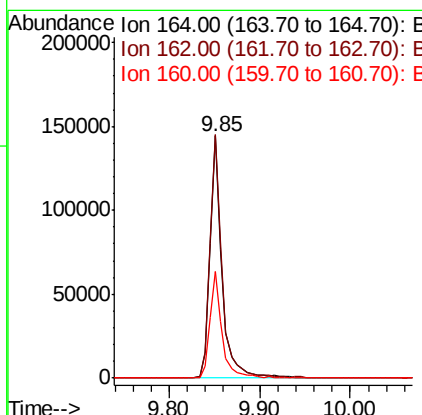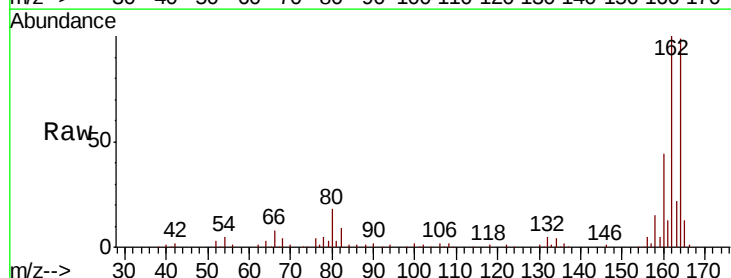







#42
 2,4,6-Tribromophenol
 Concen: 0.879 ng
 RT: 10.65 min Scan# 1455
 Delta R.T. 0.00 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38

Instrument :
 BNA_F
 ClientSampleId :
 CSA-4-6

Tot Ion:330 Resp: 1007
 Ion Ratio Lower Upper
 330 100
 332 67.9 78.0 117.0#
 141 27.3 35.8 53.6#

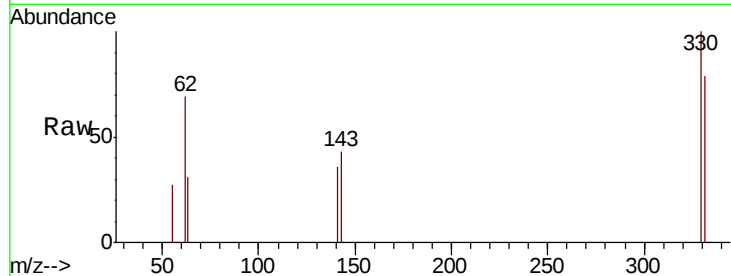


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

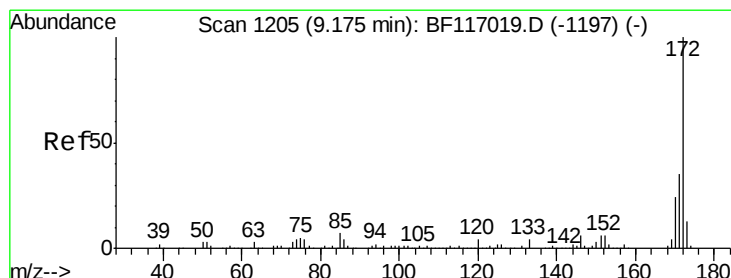
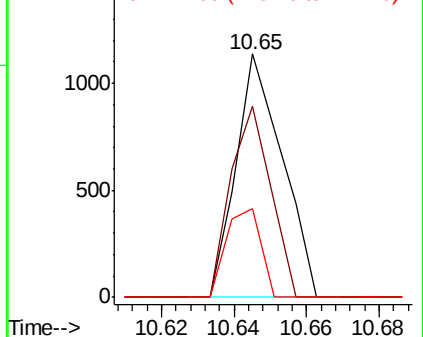



#45
 2-Fluorobiphenyl
 Concen: 1.254 ng
 RT: 9.18 min Scan# 1206
 Delta R.T. 0.01 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38

Tgt Ion:172 Resp: 10990
 Ion Ratio Lower Upper
 172 100
 171 35.3 28.2 42.2
 170 27.1 18.9 28.3

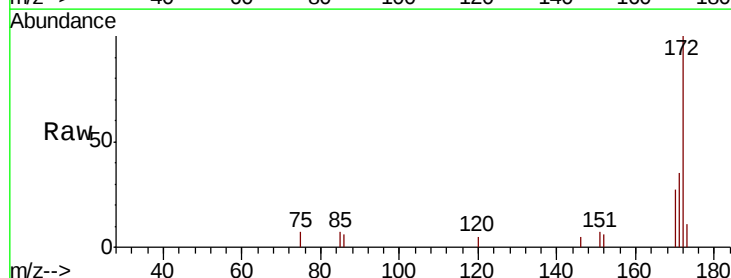

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

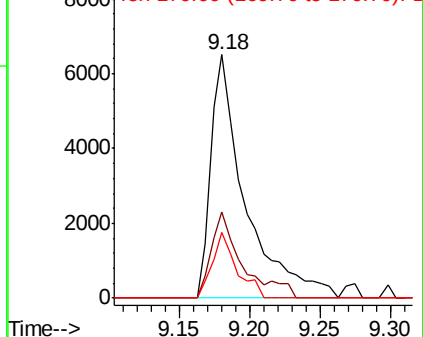


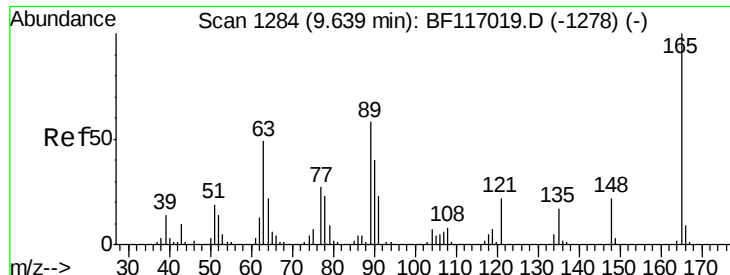




#51
 2,6-Dinitrotoluene
 Concen: 8.935 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. 0.21 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38

Instrument :
 BNA_F
 ClientSampleId :
 CSA-4-6

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	41.8	62.8#
89	0.0	46.5	69.7#

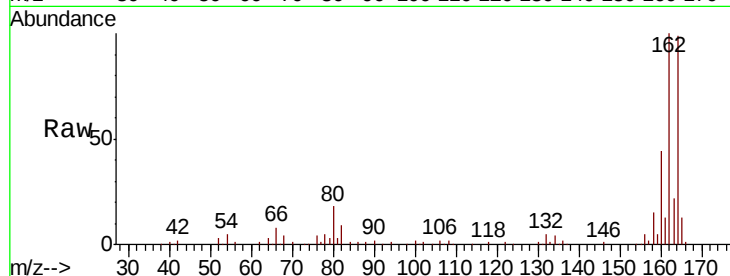




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

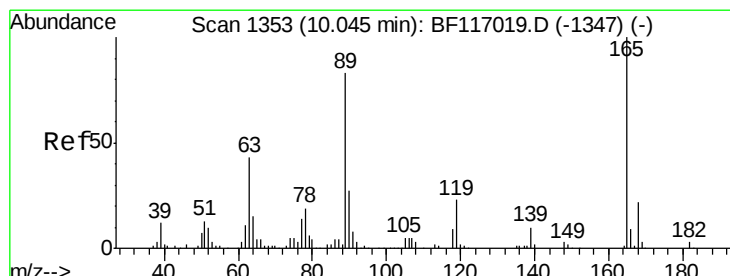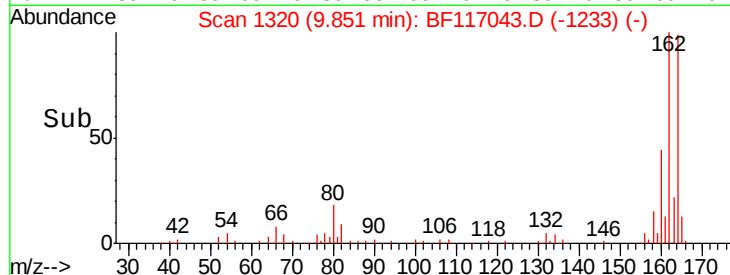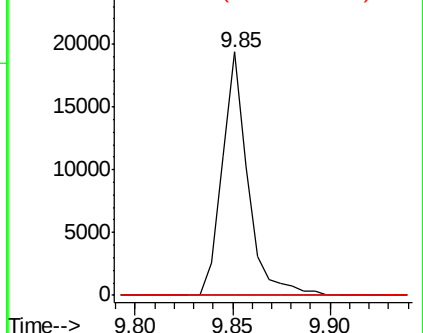


#57
 2,4-Dinitrotoluene
 Concen: 6.883 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. -0.19 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	35.0	52.4#
89	0.0	66.1	99.1#
182	0.0	2.0	3.0#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

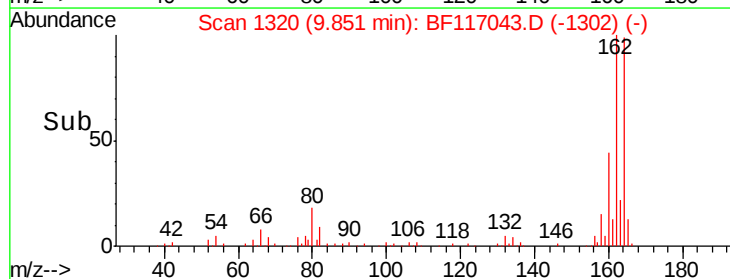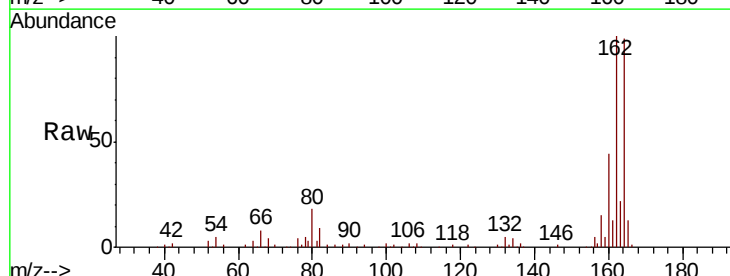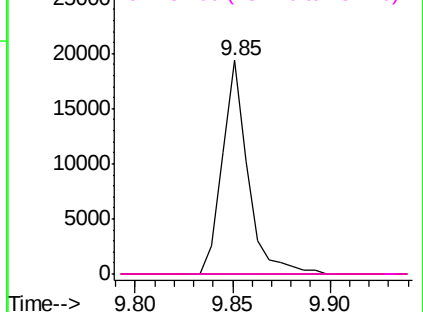

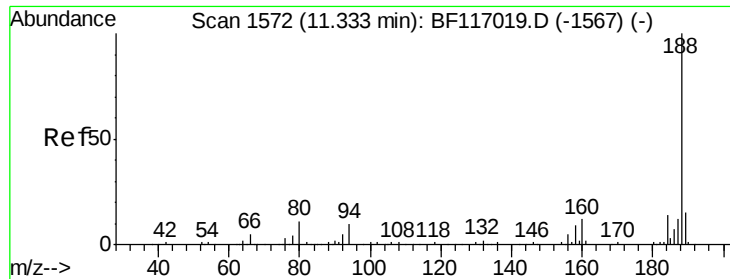

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.33 min Scan# 1572

Delta R.T. 0.00 min

Lab File: BF117043.D

Acq: 14 Sep 2019 00:38

Instrument :

BNA_F

ClientSampleId :

CSA-4-6


Tot Ion:188 Resp: 181190

Ion Ratio Lower Upper

188 100

94 8.4 8.2 12.2




80 9.3 9.0 13.6

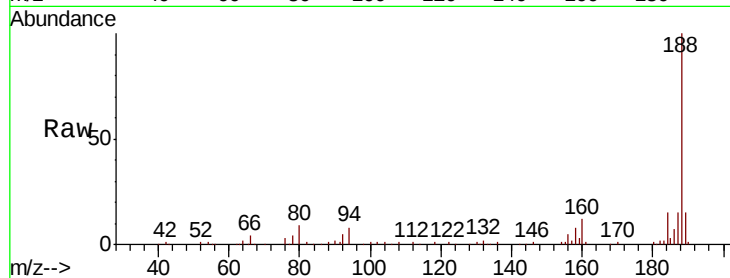

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

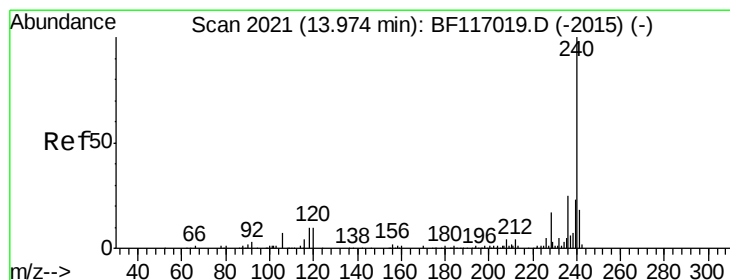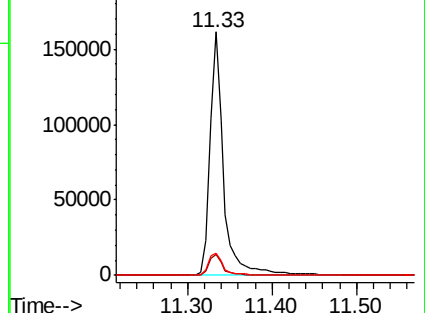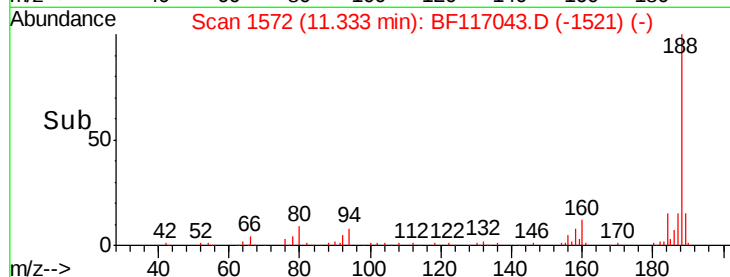

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.96 min Scan# 2019

Delta R.T. -0.01 min

Lab File: BF117043.D

Acq: 14 Sep 2019 00:38


Tgt Ion:240 Resp: 129782

Ion Ratio Lower Upper

240 100

120 11.2 8.3 12.5



236 26.6 20.3 30.5

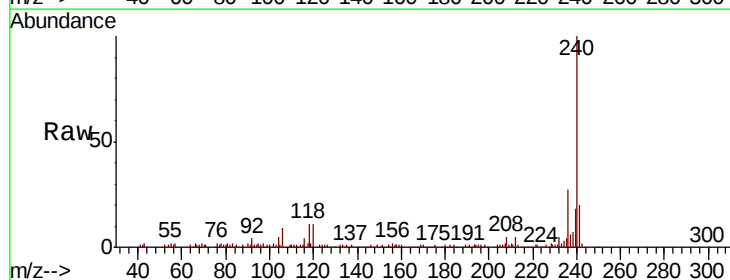


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

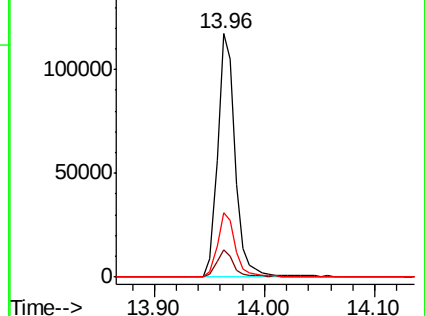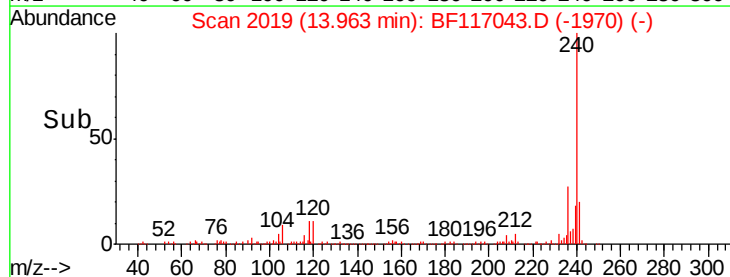







#79
 Terphenyl-d14
 Concen: 1.116 ng
 RT: 12.91 min Scan# 1840
 Delta R.T. -0.01 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38

Instrument :
 BNA_F
 ClientSampleId :
 CSA-4-6

Tot Ion:244 Resp: 7748
 Ion Ratio Lower Upper
 244 100
 212 9.3 5.8 8.8#
 122 10.4 11.3 16.9#

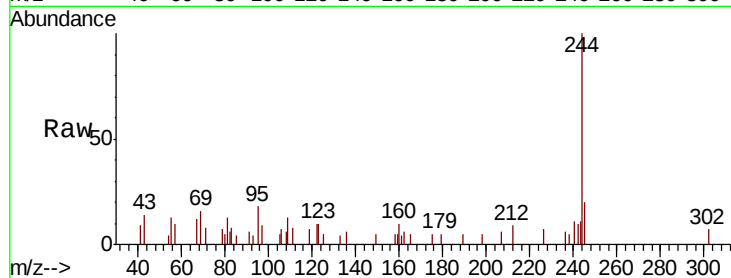


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

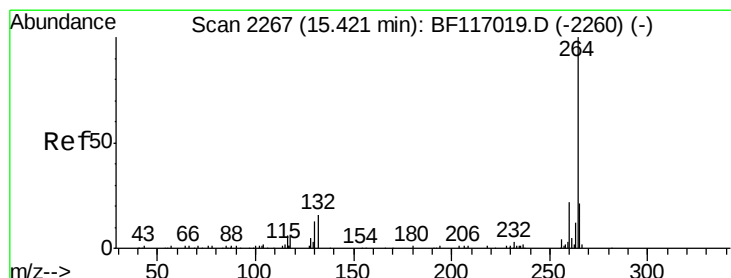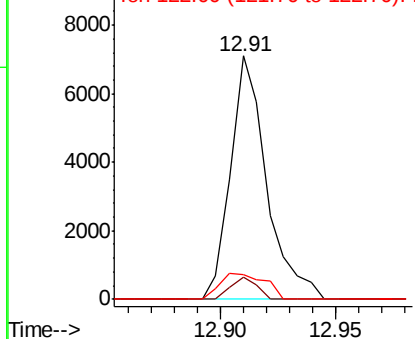

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.41 min Scan# 2265
 Delta R.T. -0.01 min
 Lab File: BF117043.D
 Acq: 14 Sep 2019 00:38

Tgt Ion:264 Resp: 109943
 Ion Ratio Lower Upper
 264 100
 260 23.8 17.6 26.4
 265 22.0 16.6 24.8

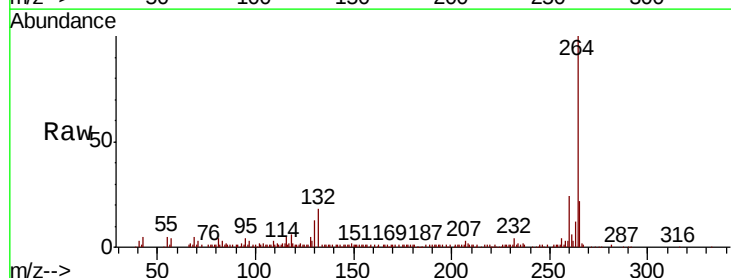

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

