

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091319\
 Data File : BF117033.D
 Acq On : 13 Sep 2019 20:12
 Operator : HP/JU
 Sample : K4851-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3D-(9-10)

Quant Time: Sep 14 01:02:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 13 16:23:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	64499	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	257254	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	135196	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	226647	20.00	ng	0.00
76) Chrysene-d12	13.97	240	171804	20.00	ng	0.00
87) Perylene-d12	15.42	264	148794	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	469256	113.59	ng	0.00
7) Phenol-d6	6.46	99	655920	122.85	ng	0.00
23) Nitrobenzene-d5	7.38	82	412051	84.16	ng	0.00
42) 2,4,6-Tribromophenol	10.64	330	143386	126.90	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	688743	79.65	ng	0.00
79) Terphenyl-d14	12.92	244	672368	73.15	ng	0.00
Target Compounds						
10) Phenol	6.47	94	30667	5.210	ng	89
50) Dimethylphthalate	9.56	163	87365	9.127	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091319\
Data File : BF117033.D
Acq On : 13 Sep 2019 20:12
Operator : HP/JU
Sample : K4851-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3D-(9-10)

Quant Time: Sep 14 01:02:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

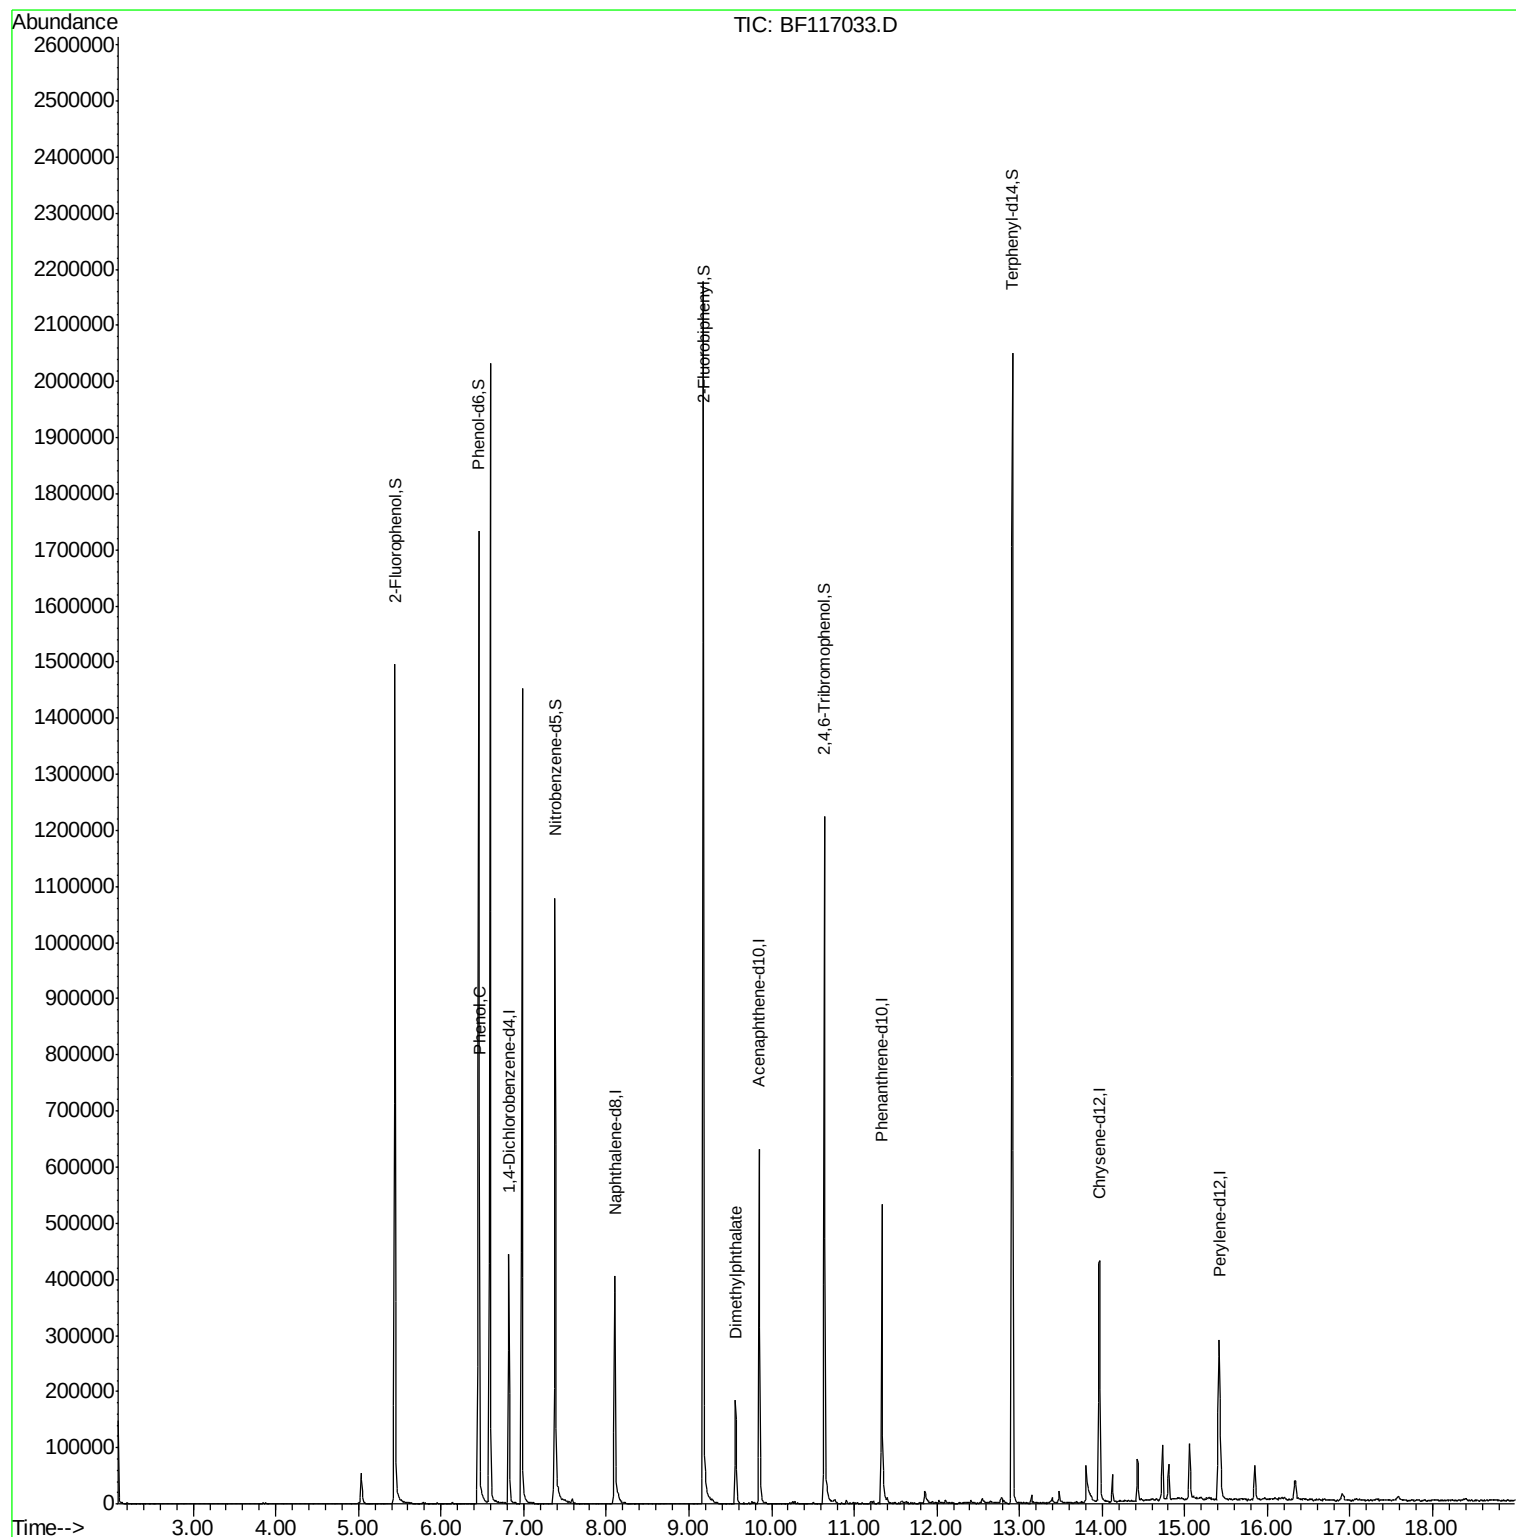

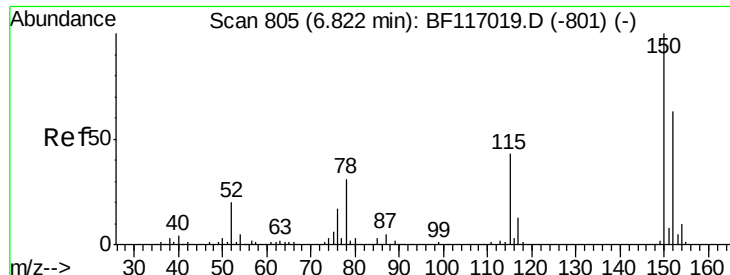


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. 0.00 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12

Instrument :
BNA_F
ClientSampleId :
SB-3D-(9-10)

Tot Ion:152 Resp: 64499
Ion Ratio Lower Upper
152 100
150 159.1 127.5 191.3
115 65.9 55.0 82.4

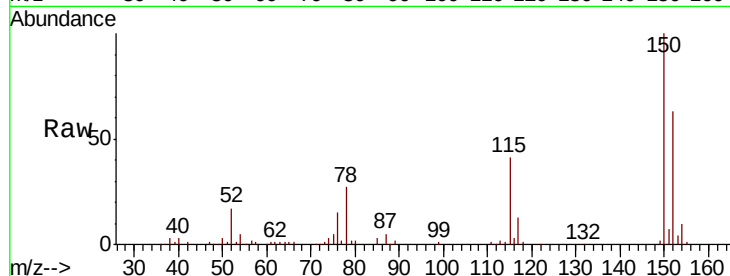


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

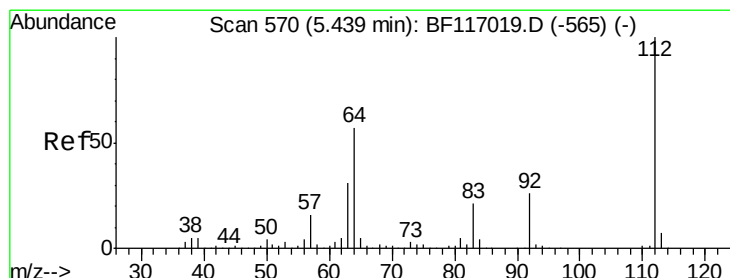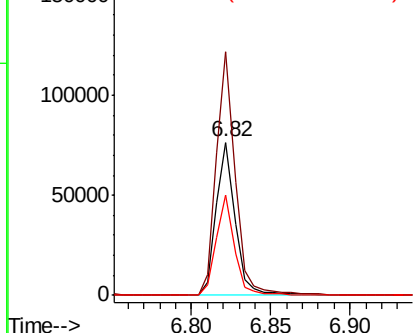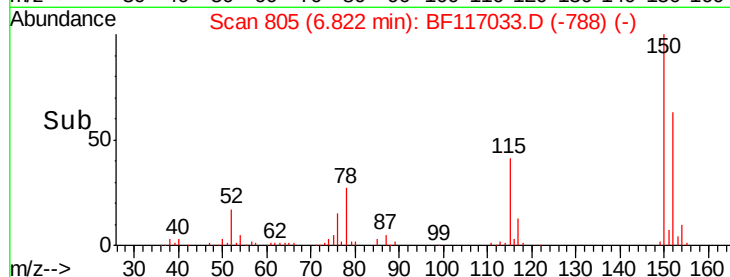



#5


2-Fluorophenol
Concen: 113.587 ng
RT: 5.45 min Scan# 571
Delta R.T. 0.01 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12

Tgt Ion:112 Resp: 469256
Ion Ratio Lower Upper
112 100
64 53.2 45.7 68.5
63 28.6 24.9 37.3

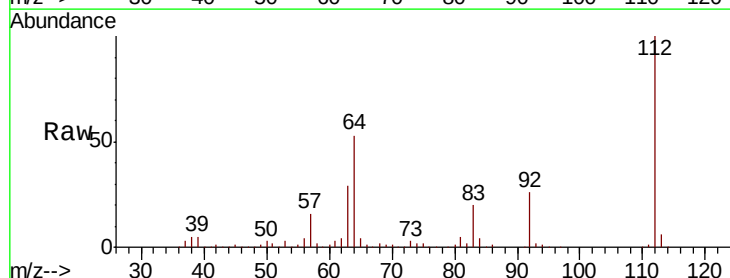

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

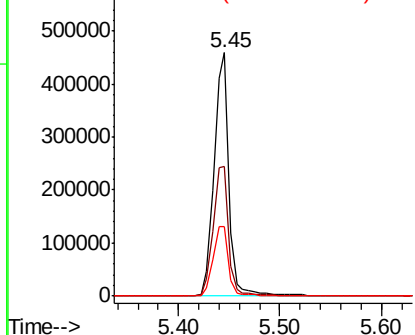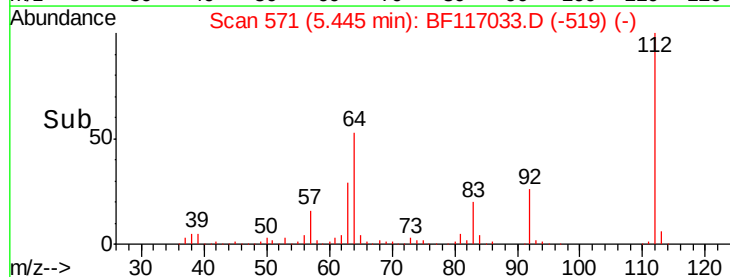

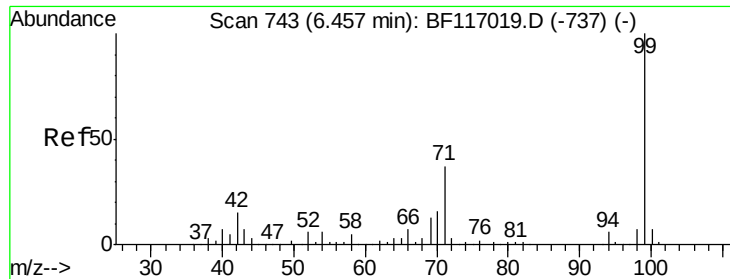

#7

Phenol-d6

Concen: 122.853 ng

RT: 6.46 min Scan# 743

Delta R.T. 0.00 min

Lab File: BF117033.D

Acq: 13 Sep 2019 20:12

Instrument :

BNA_F

ClientSampleId :

SB-3D-(9-10)


Tot Ion: 99 Resp: 655920

Ion Ratio Lower Upper




99 100

42 15.7 12.2 18.2

71 37.6 29.8 44.8

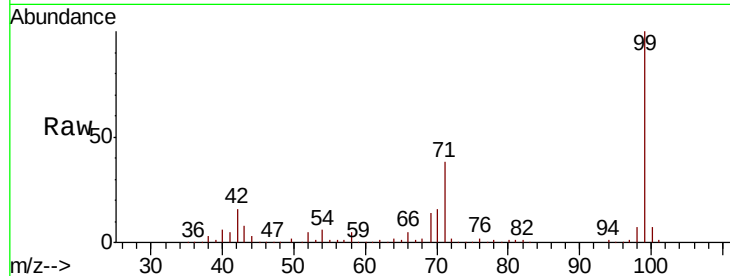

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

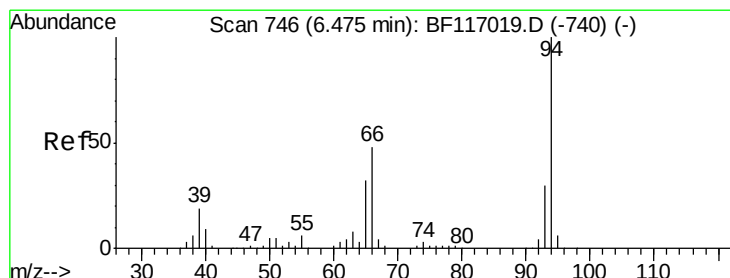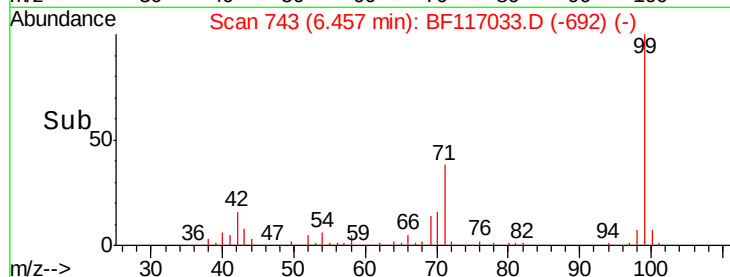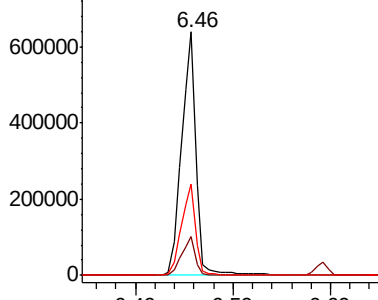

#10

Phenol

Concen: 5.210 ng

RT: 6.47 min Scan# 745

Delta R.T. -0.01 min

Lab File: BF117033.D

Acq: 13 Sep 2019 20:12


Tgt Ion: 94 Resp: 30667

Ion Ratio Lower Upper



94 100


65 27.2 12.5 52.5

66 40.9 28.9 68.9

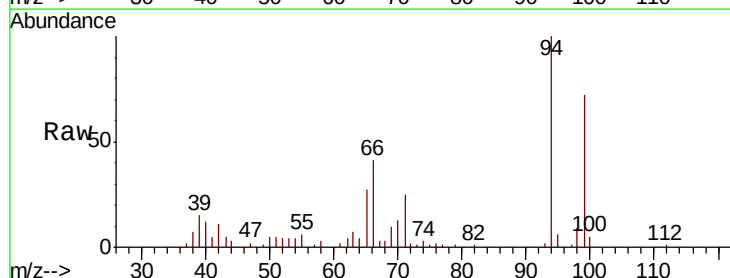

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

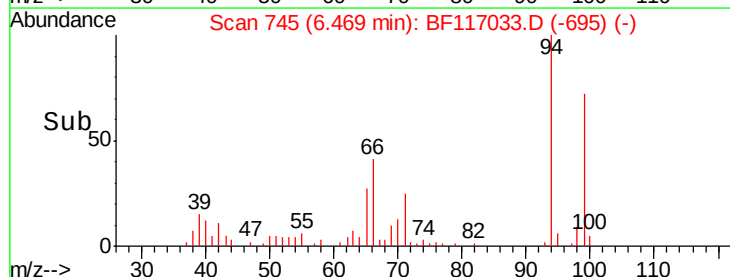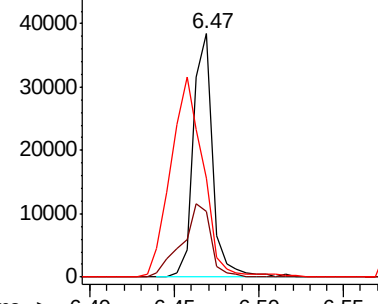

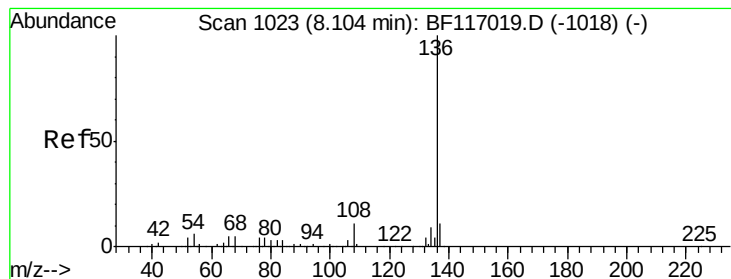

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1023

Delta R.T. 0.00 min

Lab File: BF117033.D

Acq: 13 Sep 2019 20:12

Instrument :

BNA_F

ClientSampleId :

SB-3D-(9-10)

Tot Ion:136 Resp: 257254





Ion Ratio Lower Upper

136 100

137 9.7 9.0 13.4

54 5.0 4.5 6.7

68 5.0 4.0 6.0

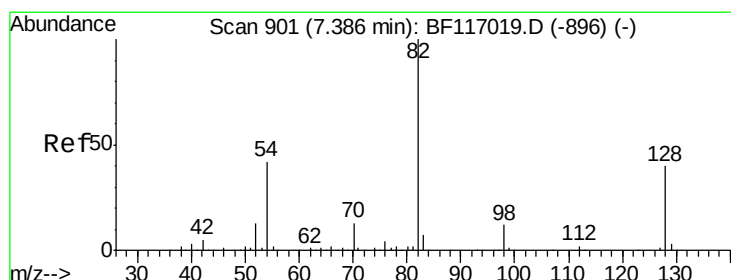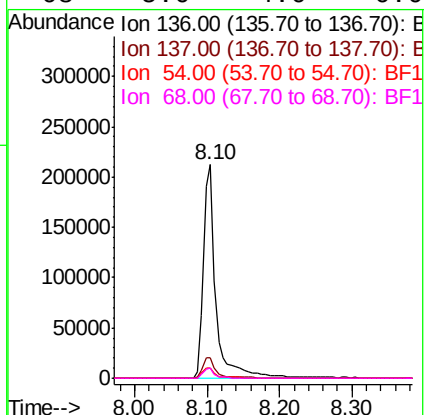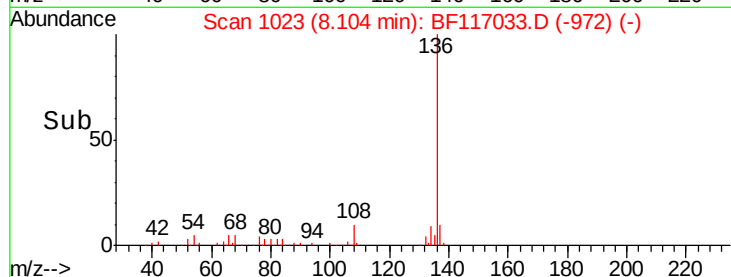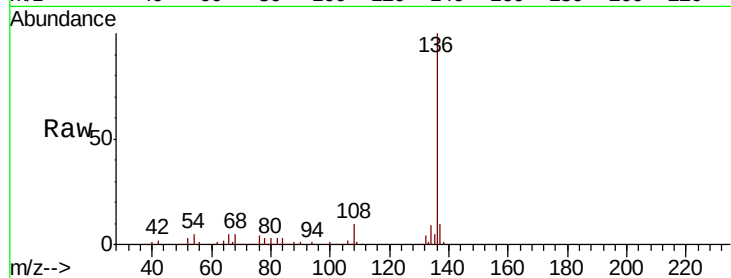

#23

Nitrobenzene-d5

Concen: 84.159 ng

RT: 7.38 min Scan# 900

Delta R.T. -0.01 min

Lab File: BF117033.D

Acq: 13 Sep 2019 20:12




Tgt Ion: 82 Resp: 412051


Ion Ratio Lower Upper

82 100

128 40.5 32.3 48.5

54 40.8 33.3 49.9

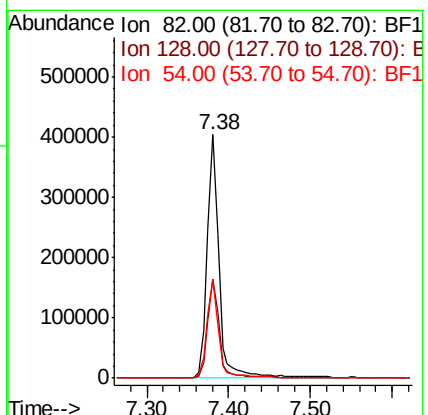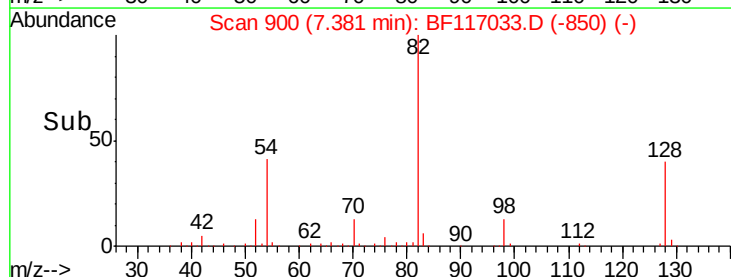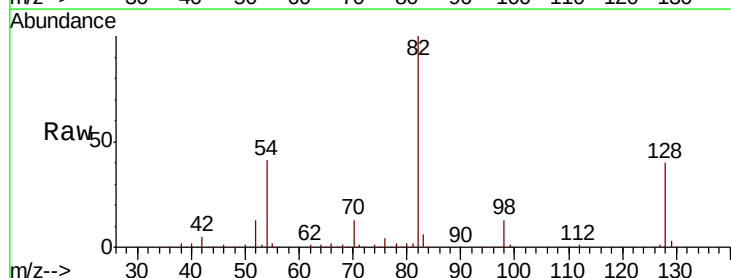


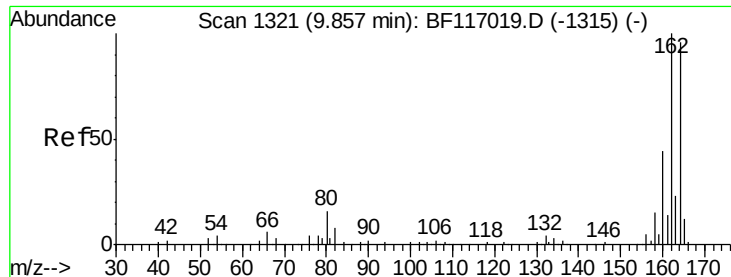




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.85 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12

Instrument :
BNA_F
ClientSampleId :
SB-3D-(9-10)

Tot Ion:164 Resp: 135196
Ion Ratio Lower Upper
164 100
162 99.1 83.4 125.2
160 43.4 36.4 54.6

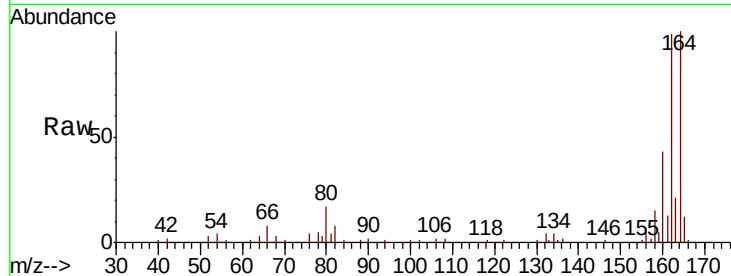


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

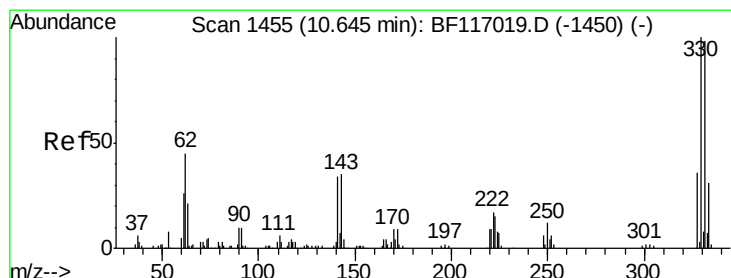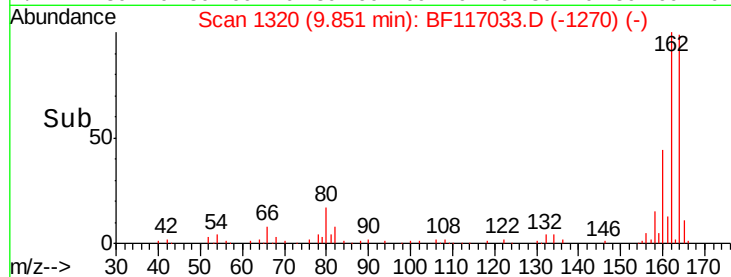
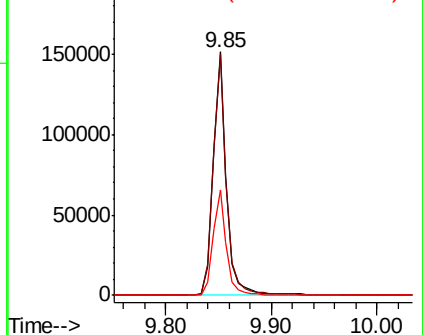



#42
2,4,6-Tribromophenol
Concen: 126.898 ng
RT: 10.64 min Scan# 1454
Delta R.T. -0.01 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12

Tgt Ion:330 Resp: 143386
Ion Ratio Lower Upper
330 100
332 95.6 78.0 117.0
141 44.6 35.8 53.6

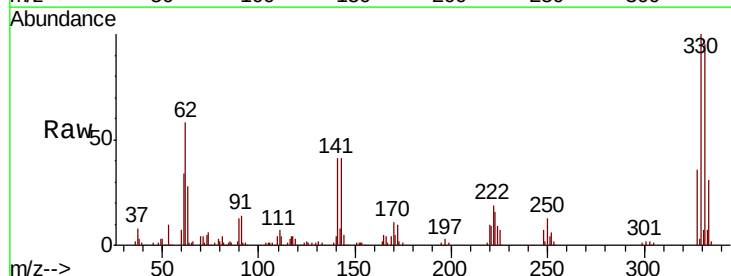

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



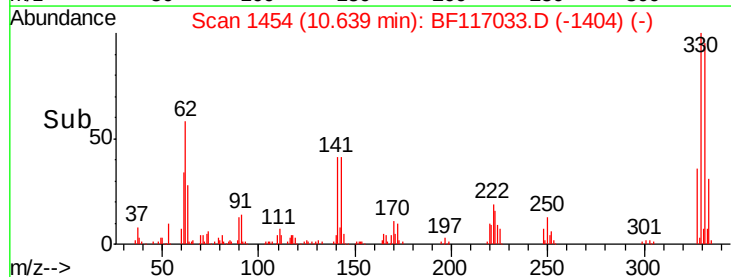
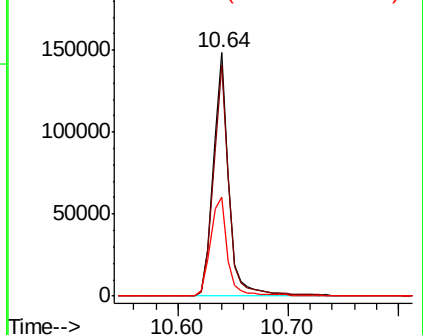


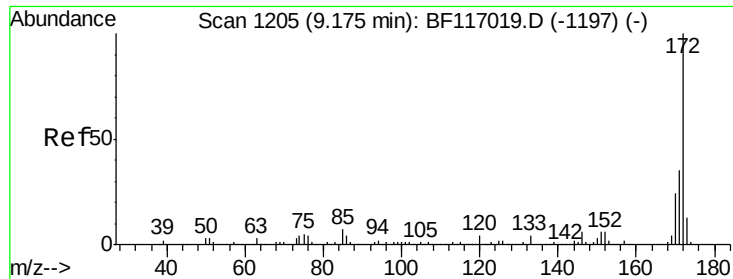

#45
2-Fluorobiphenyl
Concen: 79.655 ng
RT: 9.17 min Scan# 1205
Delta R.T. 0.00 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12




Instrument :
BNA_F
ClientSampleId :
SB-3D-(9-10)


Tot Ion:172 Resp: 688743
Ion Ratio Lower Upper
172 100
171 34.9 28.2 42.2
170 24.0 18.9 28.3

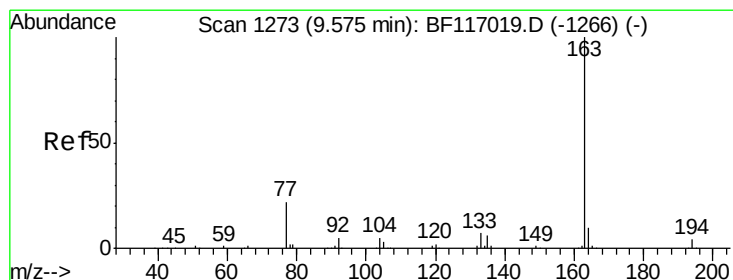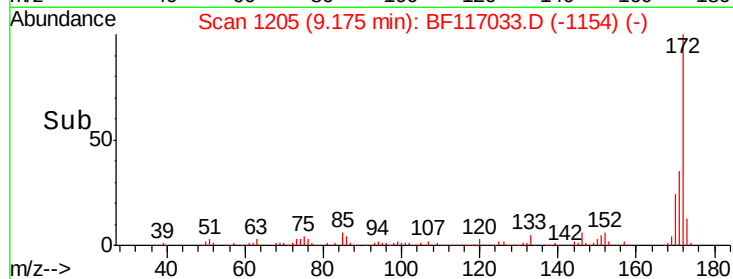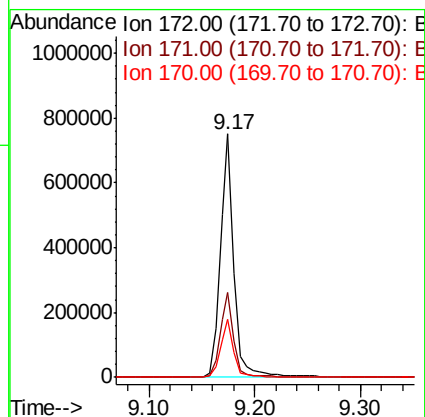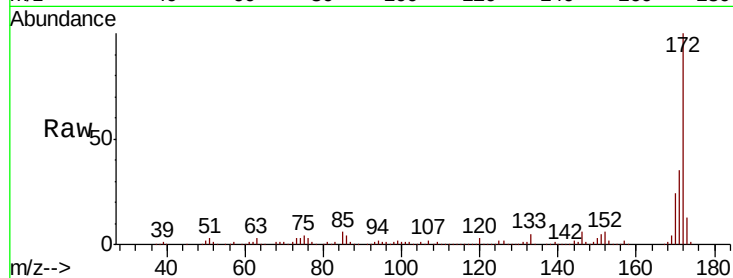

#50
Dimethylphthalate
Concen: 9.127 ng
RT: 9.56 min Scan# 1271
Delta R.T. -0.01 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12

Tgt Ion:163 Resp: 87365
Ion Ratio Lower Upper
163 100
194 3.5 2.9 4.3
164 10.0 8.2 12.4

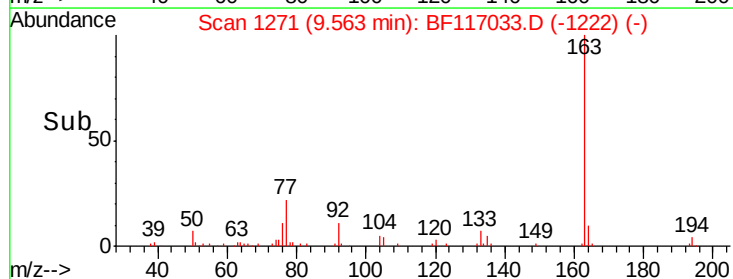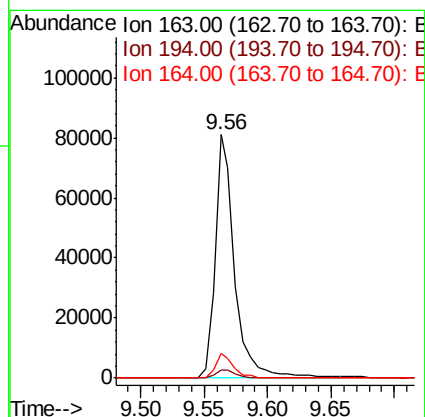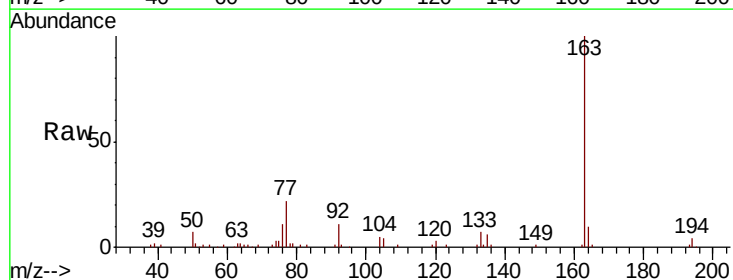


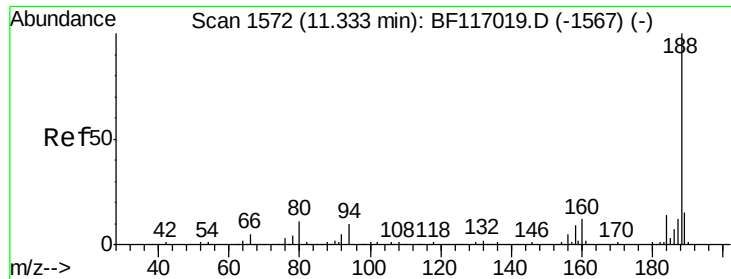




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.33 min Scan# 1572
Delta R.T. 0.00 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12

Instrument :
BNA_F
ClientSampled :
SB-3D-(9-10)

Tot Ion	Ratio	Lower	Upper
188	100		
94	8.4	8.2	12.2
80	10.3	9.0	13.6

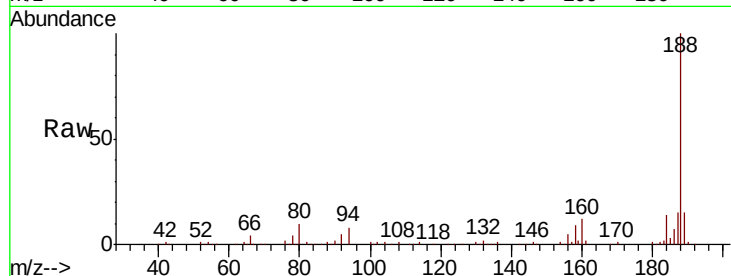


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

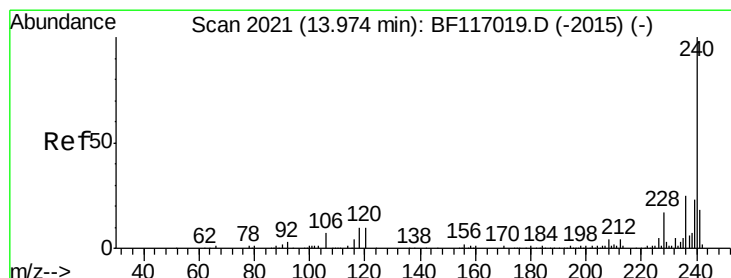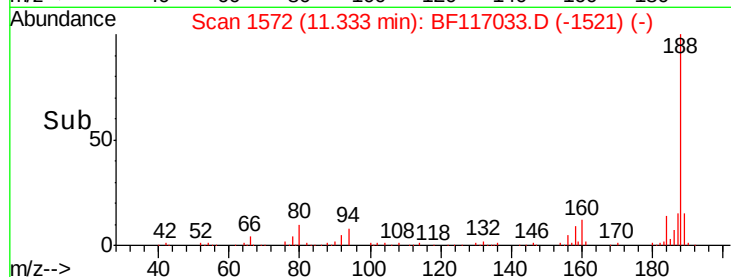
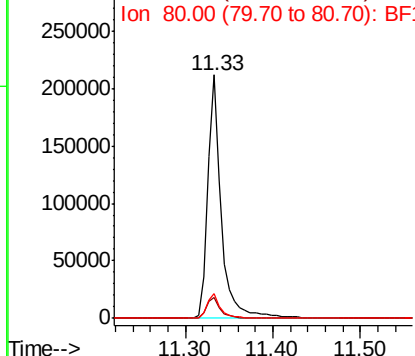



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.01 min
Lab File: BF117033.D
Acq: 13 Sep 2019 20:12

Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.7	8.3	12.5
236	26.4	20.3	30.5

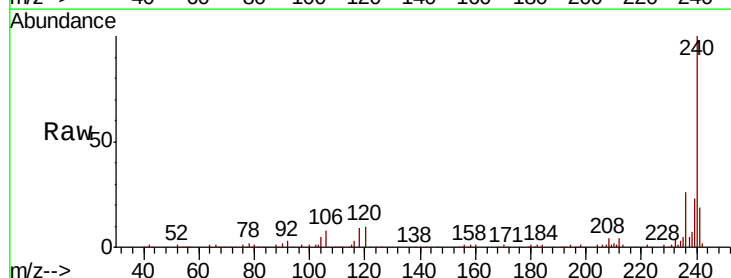

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



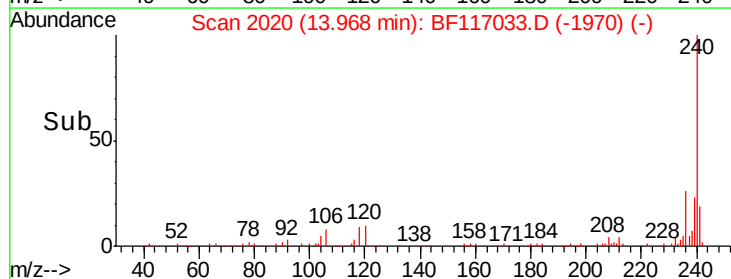
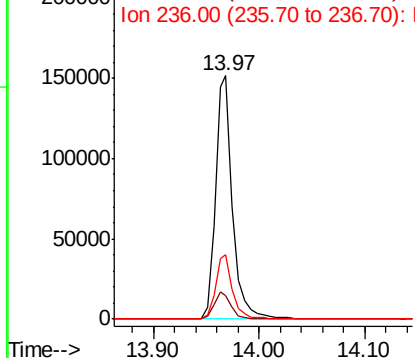


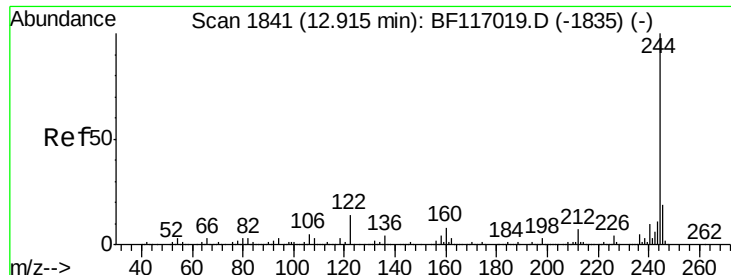

#79
 Terphenyl-d14
 Concen: 73.153 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BF117033.D
 Acq: 13 Sep 2019 20:12

Instrument :
 BNA_F
 ClientSampleId :
 SB-3D-(9-10)

Tot Ion	Ratio	Lower	Upper
244	100		
212	7.0	5.8	8.8
122	12.0	11.3	16.9

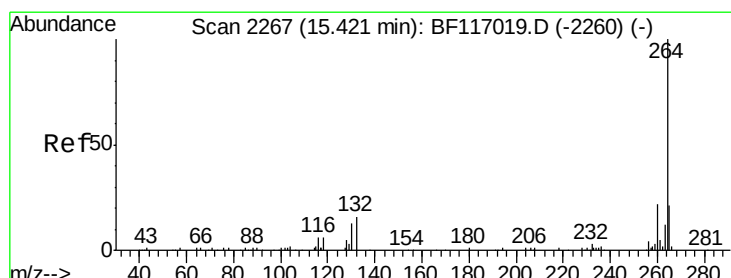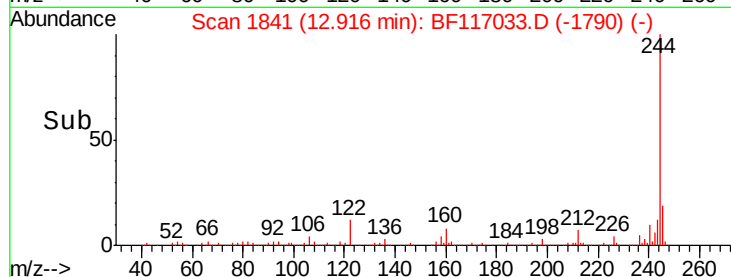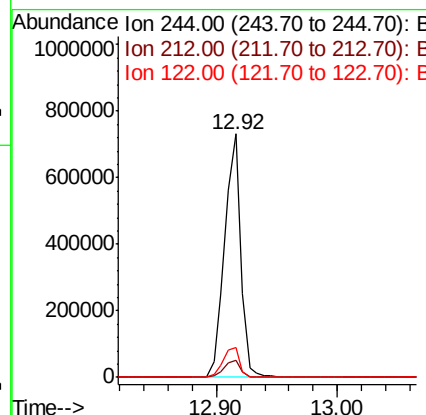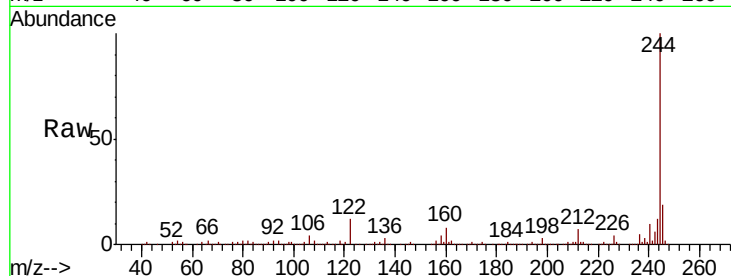

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.42 min Scan# 2266
 Delta R.T. -0.01 min
 Lab File: BF117033.D
 Acq: 13 Sep 2019 20:12

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.9	17.6	26.4
265	20.7	16.6	24.8

