


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091319\
 Data File : BF117016.D
 Acq On : 13 Sep 2019 12:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

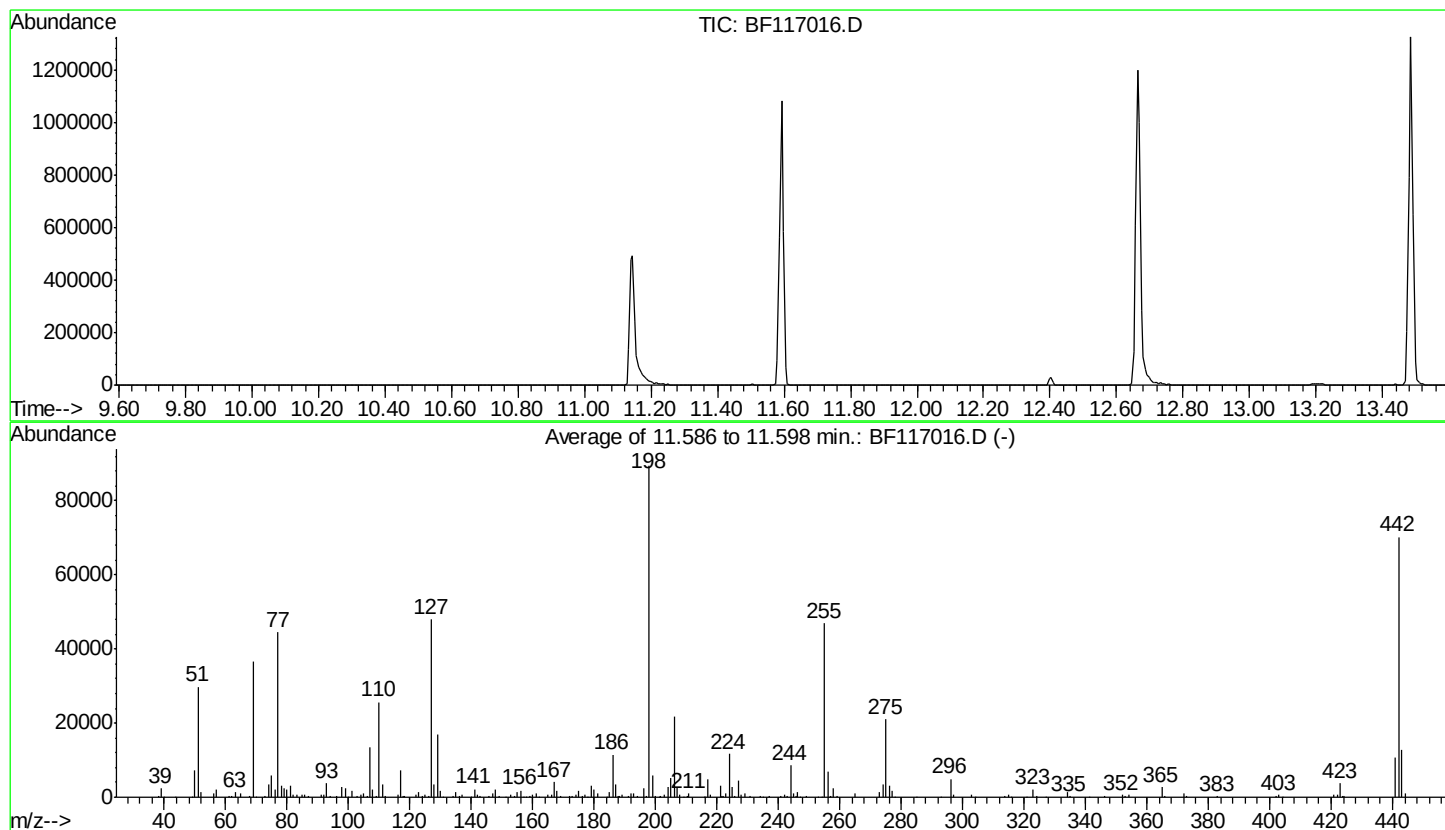

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	29705	PASS
68	69	0.00	2	1.4	514	PASS
69	198	0.00	100	40.9	36616	PASS
70	69	0.00	2	0.3	105	PASS
127	198	10	80	53.6	47893	PASS
197	198	0.00	2	0.5	408	PASS
198	198	100	100	100.0	89434	PASS
199	198	5	9	6.6	5876	PASS
275	198	10	60	23.5	21034	PASS
365	198	1	100	3.0	2668	PASS
441	198	0.01	100	11.9	10635	PASS
442	198	50	100	78.4	70122	PASS
443	442	15	24	18.2	12739	PASS