
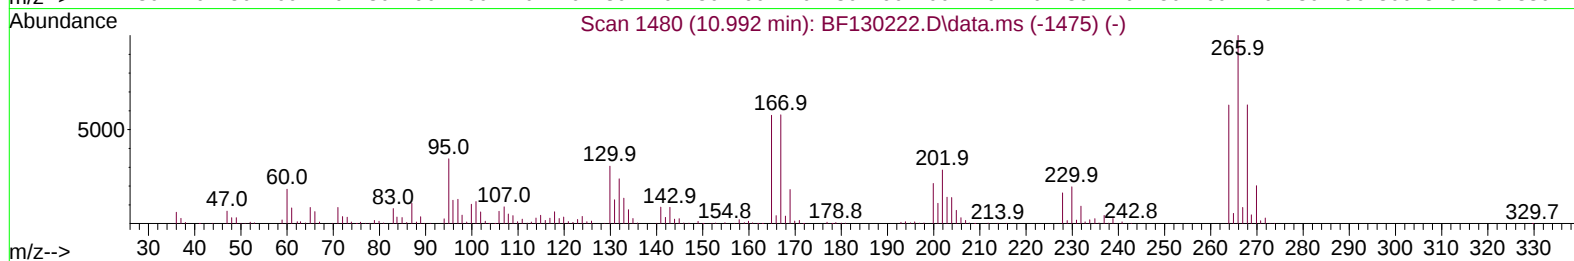
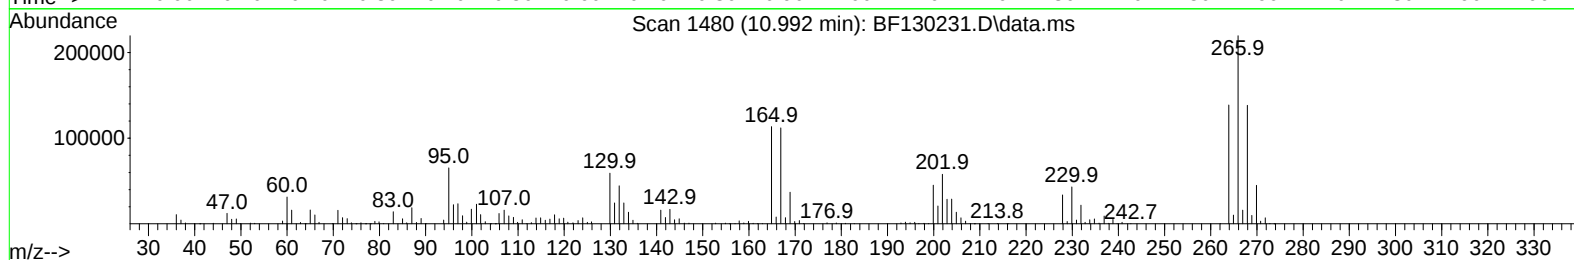


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\  
Data File : BF130231.D  
Acq On    : 14 Sep 2022  10:25  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Sep 14 13:59:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 13:52:44 2022
Response via : Initial Calibration

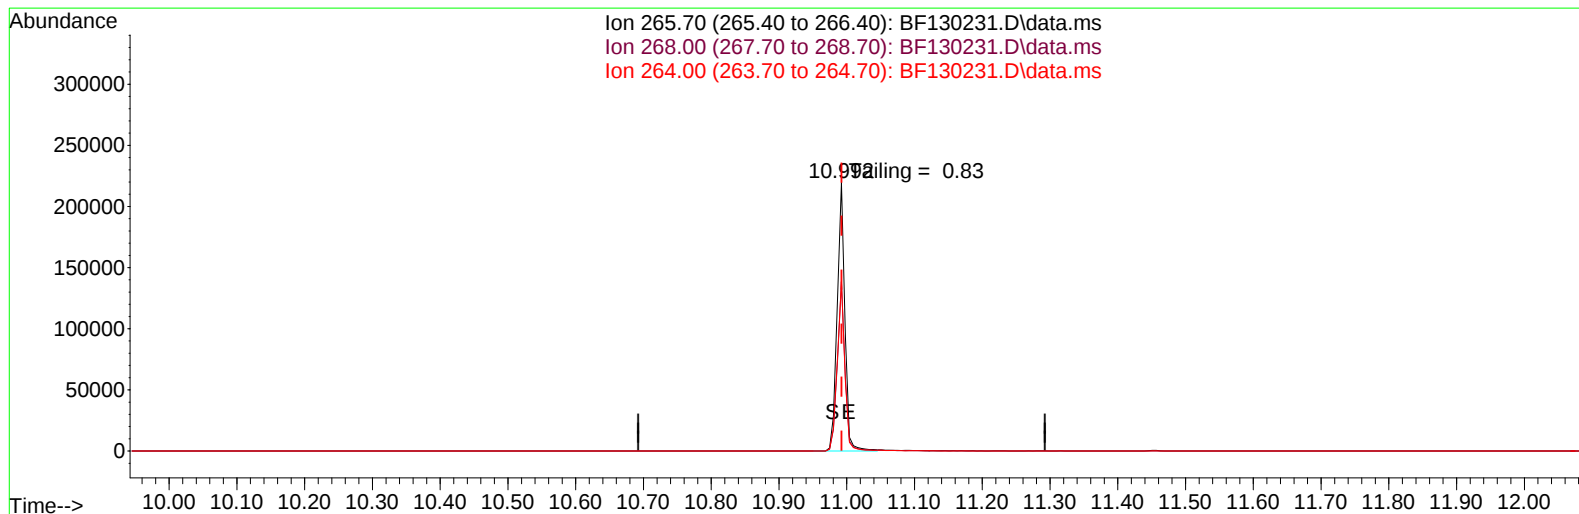

TIC: BF130231.D\data.ms

(70) Pentachlorophenol (C)




10.992min (-0.000) 30047.29 ng

response **176183**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.00
264.00	63.10	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130231.D
Acq On : 14 Sep 2022 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 13:59:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 13:52:44 2022
Response via : Initial Calibration

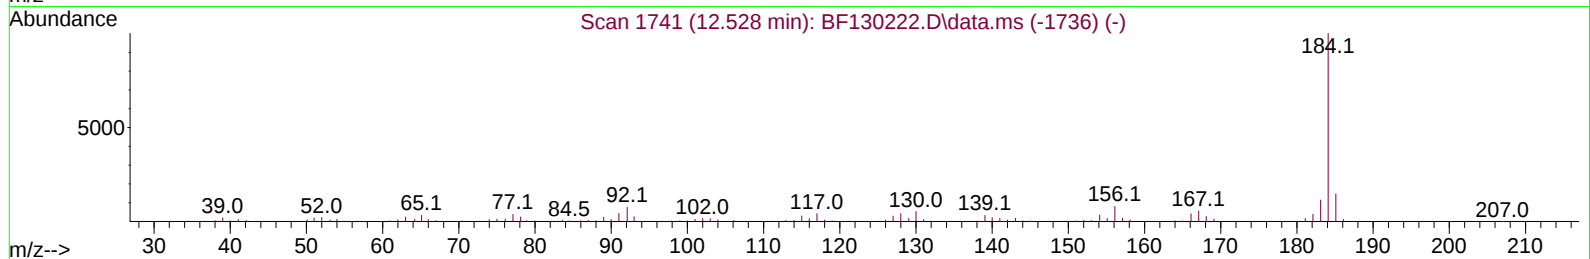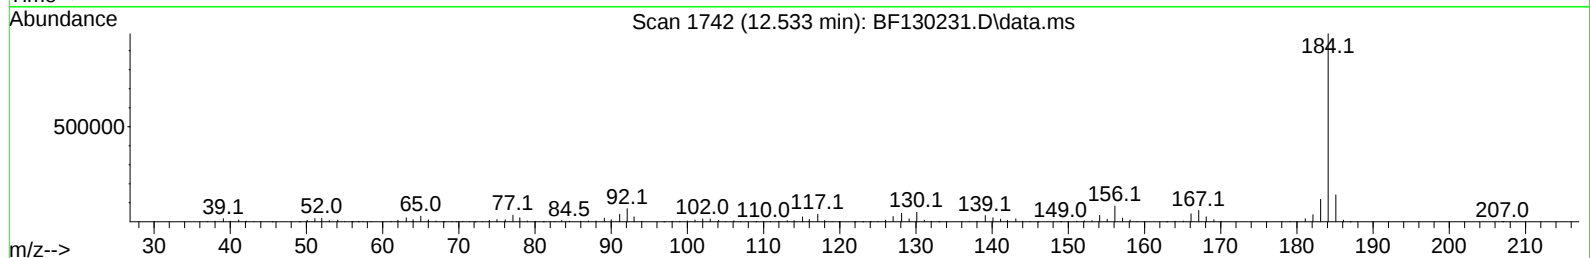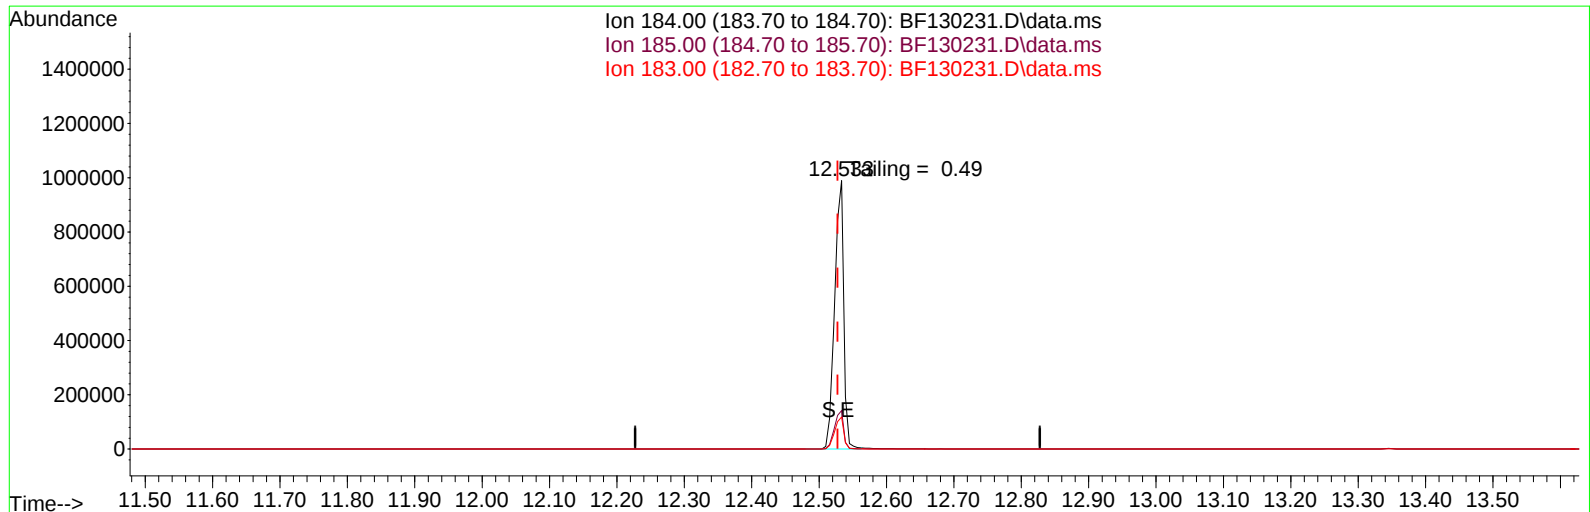

TIC: BF130231.D\data.ms

(77) Benzidine

12.533min (+ 0.006) 0.00 ng

response 932976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.32
183.00	11.40	11.92
0.00	0.00	0.00