
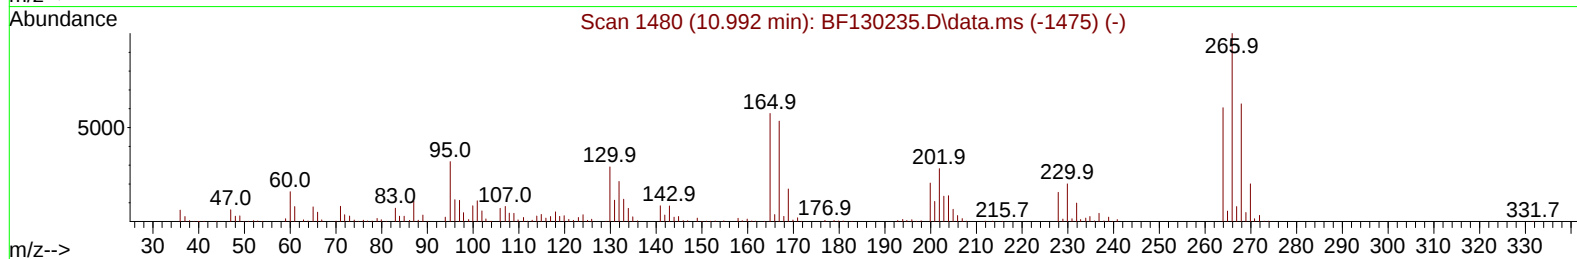
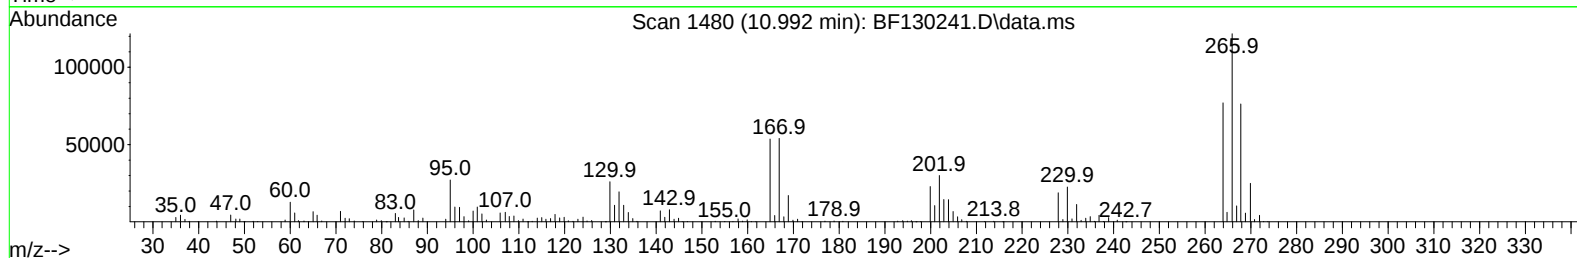


Quant Time: Sep 15 05:55:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 14:55:51 2022
Response via : Initial Calibration

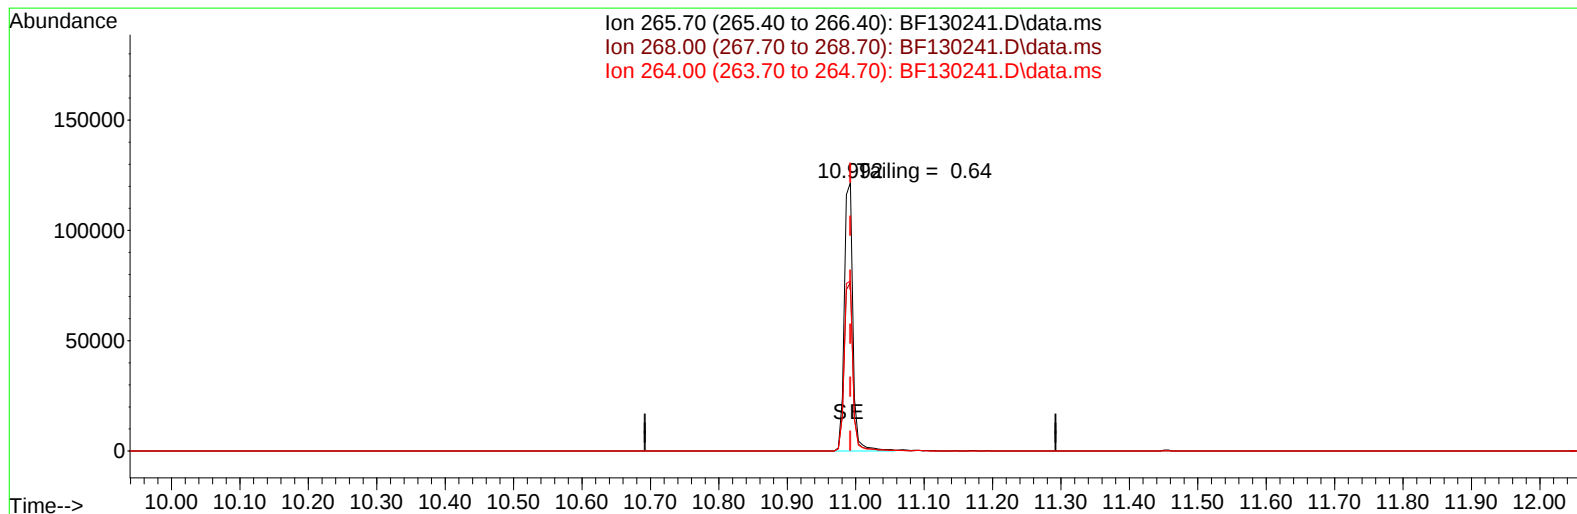

TIC: BF130241.D\data.ms

(70) Pentachlorophenol (C)




10.992min (+ 0.000) 25401.93 ng

response **106721**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.71
264.00	63.10	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130241.D
Acq On : 14 Sep 2022 15:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 05:55:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 14:55:51 2022
Response via : Initial Calibration

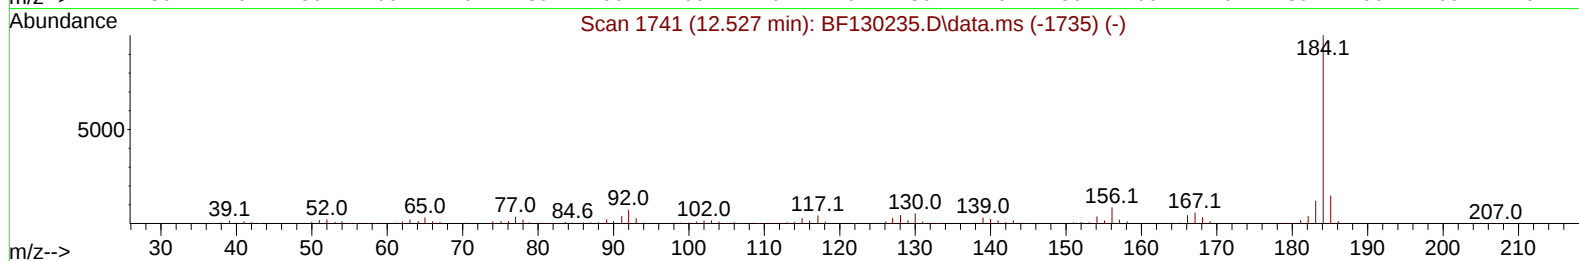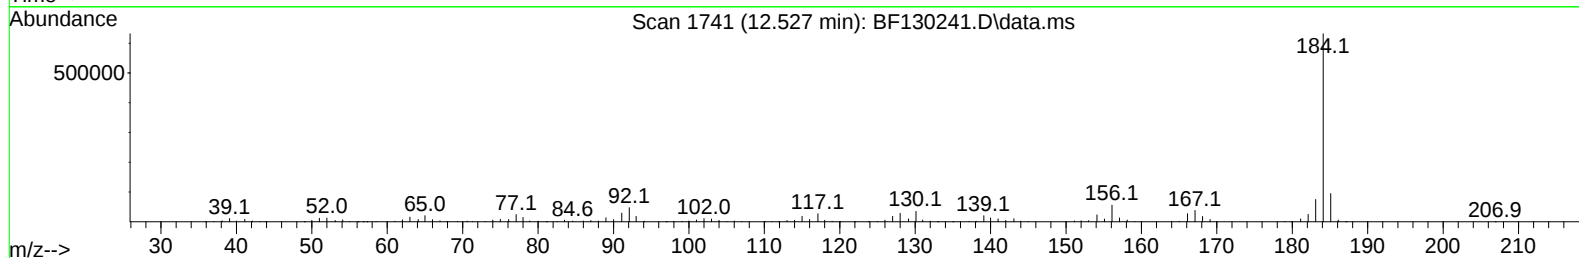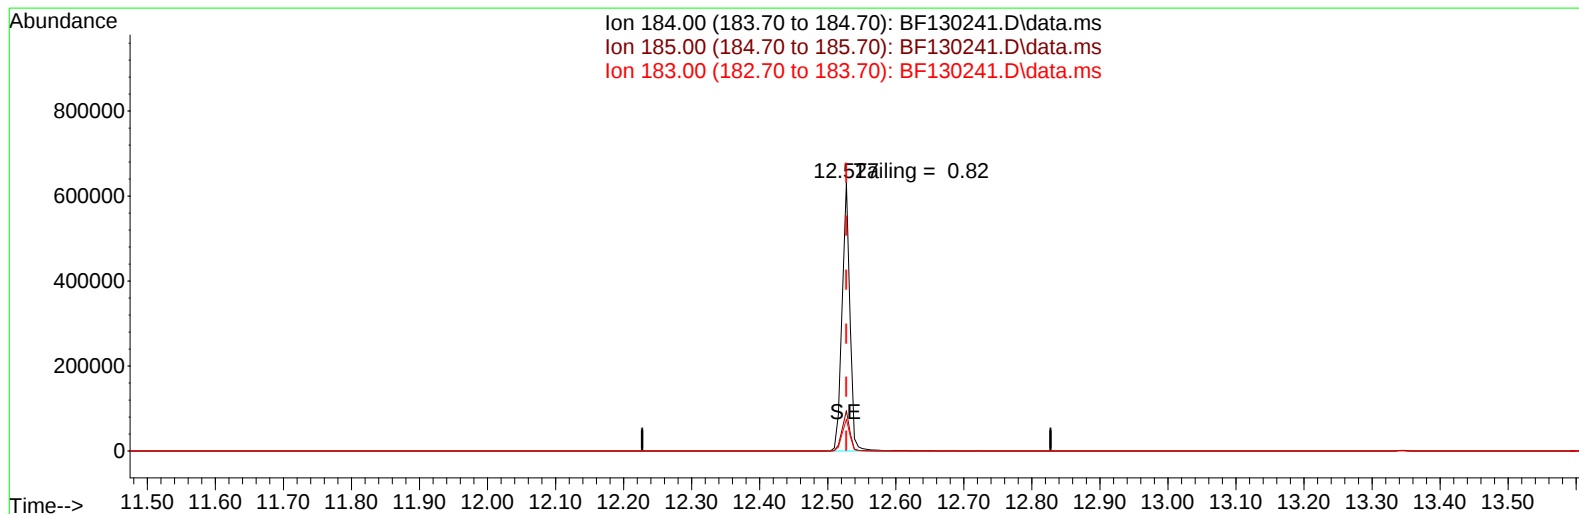

TIC: BF130241.D\data.ms

(77) Benzidine

12.527min (+ 0.000) 0.00 ng

response 507471

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.02
183.00	11.40	11.86
0.00	0.00	0.00