

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
 Data File : BF130240.D
 Acq On : 14 Sep 2022 15:20
 Operator : CG\JU
 Sample : PB147612BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147612BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	440	444	453	rVB	90879	132901	2.95%	0.500%
2	5.292	504	511	513	rBV	3041208	3561763	79.18%	13.411%
3	6.310	678	684	687	rBV	2889037	3596406	79.95%	13.541%
4	6.675	742	746	749	rBV	903118	698390	15.53%	2.630%
5	7.245	836	843	846	rBV	2171133	2336307	51.94%	8.797%
6	7.957	959	964	967	rBV	1069933	929516	20.66%	3.500%
7	9.039	1141	1148	1151	rBV	4608664	4352045	96.75%	16.387%
8	9.710	1256	1262	1265	rBV	1124103	1028414	22.86%	3.872%
9	10.498	1388	1396	1399	rBV	3029213	2964271	65.90%	11.161%
10	11.186	1509	1513	1516	rBV	1310123	1020637	22.69%	3.843%
11	12.780	1778	1784	1787	rBV	4543552	4498216	100.00%	16.937%
12	13.815	1956	1960	1963	rBV	923380	796731	17.71%	3.000%
13	15.209	2192	2197	2202	rBV	516603	591607	13.15%	2.228%
14	15.992	2321	2330	2340	rBV7	14540	51470	1.14%	0.194%




Sum of corrected areas: 26558674

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130240.D
Acq On : 14 Sep 2022 15:20
Operator : CG\JU
Sample : PB147612BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147612BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

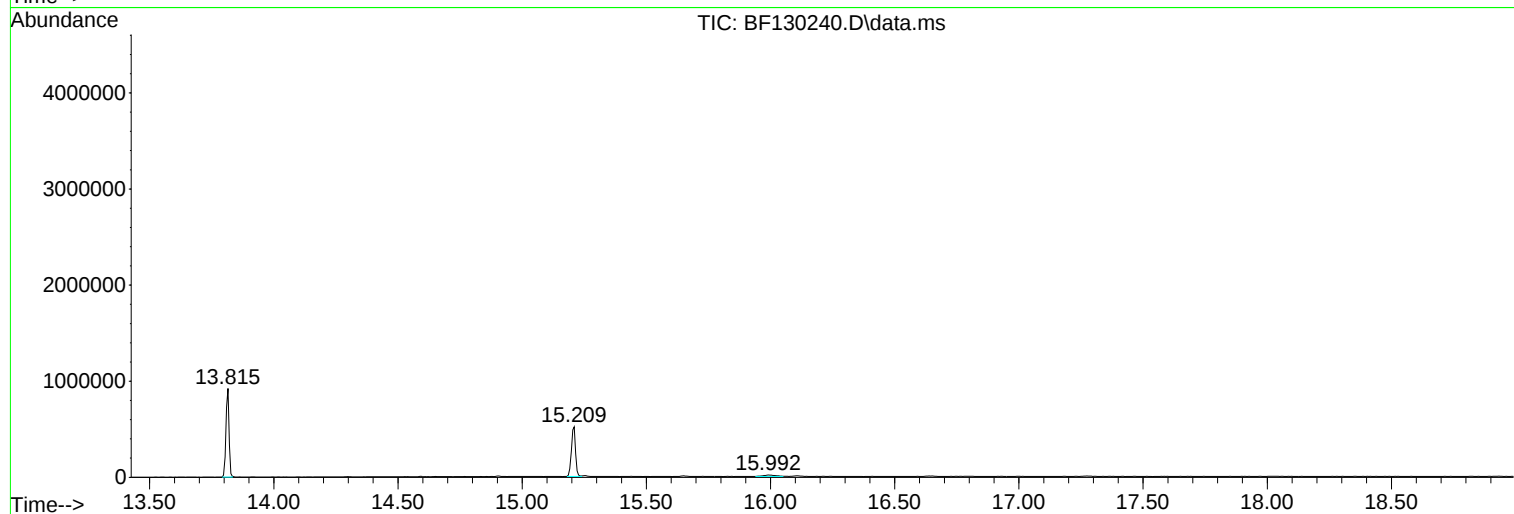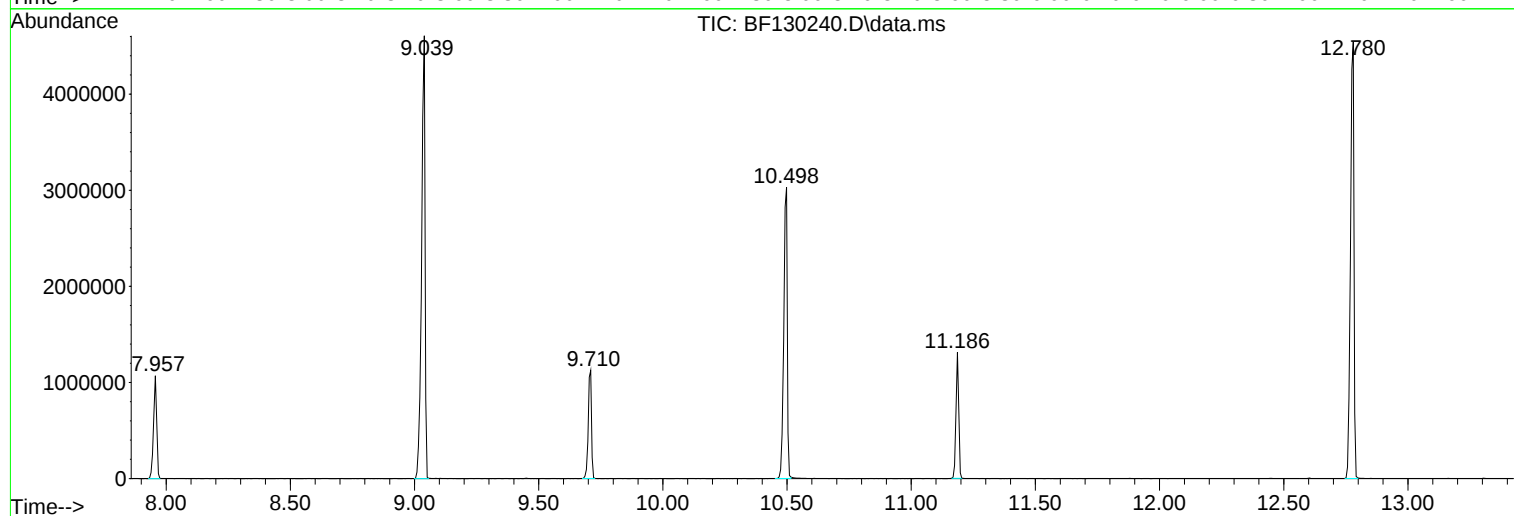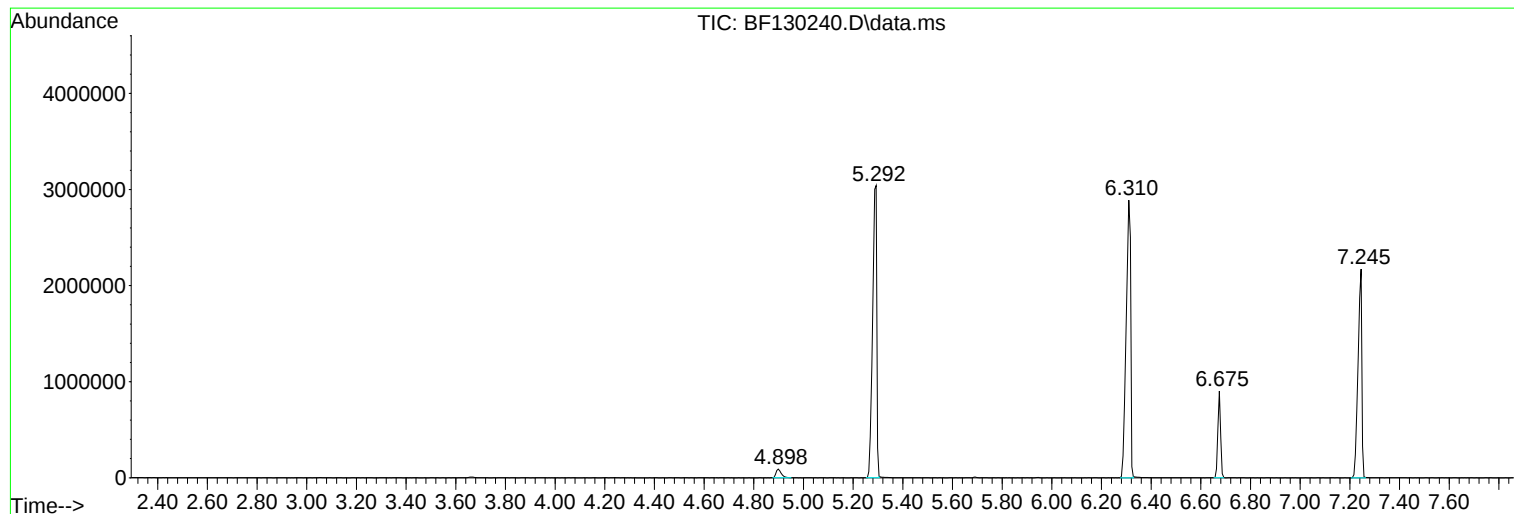

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130240.D
Acq On : 14 Sep 2022 15:20
Operator : CG\JU
Sample : PB147612BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147612BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.898	3.81 ng	132901	1,4-Dichlorobenzene-d4	6.675

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28		
3	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	28		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

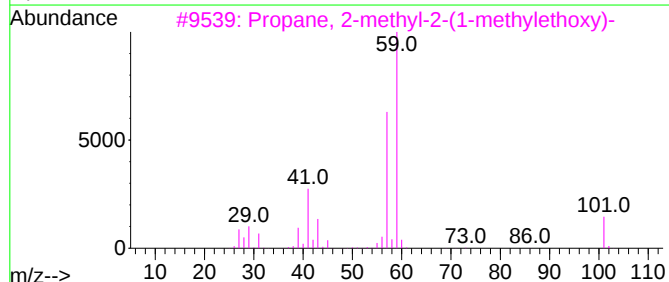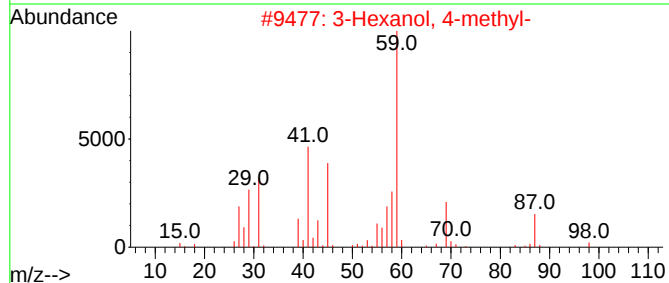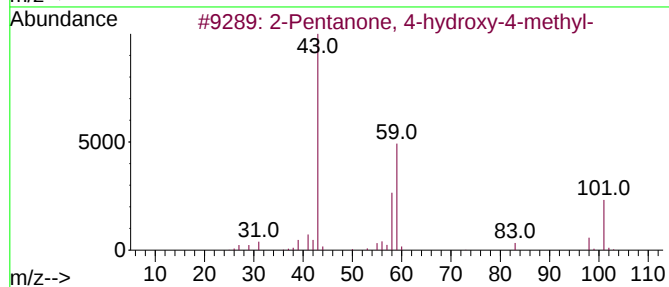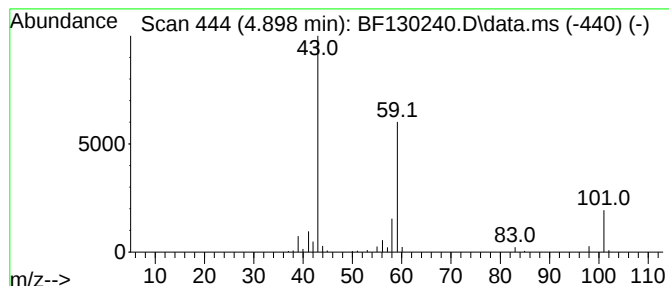

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130240.D
Acq On : 14 Sep 2022 15:20
Operator : CG\JU
Sample : PB147612BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147612BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.898	3.8	ng	132901	1	6.675	698390	20.0