

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
 Data File : BF130243.D
 Acq On : 14 Sep 2022 16:58
 Operator : CG\JU
 Sample : PB147629BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147629BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	440	444	458	rVB	72340	118264	2.57%	0.438%
2	5.287	504	510	513	rBV	3402904	3818198	82.91%	14.134%
3	6.316	678	685	688	rBV	3256672	3764905	81.76%	13.936%
4	6.675	743	746	750	rVB	840455	640829	13.92%	2.372%
5	7.245	837	843	846	rBV	2450601	2484610	53.95%	9.197%
6	7.957	959	964	967	rBV	1009088	845958	18.37%	3.131%
7	9.039	1142	1148	1151	rBV	5082555	4605038	100.00%	17.046%
8	9.710	1257	1262	1265	rBV	1092340	936518	20.34%	3.467%
9	10.498	1390	1396	1399	rBV	3684671	3211485	69.74%	11.888%
10	11.186	1509	1513	1516	rBV	1177710	928366	20.16%	3.437%
11	11.721	1598	1604	1613	rBV	52470	83658	1.82%	0.310%
12	12.780	1778	1784	1787	rBV	4824331	4518828	98.13%	16.727%
13	13.815	1956	1960	1963	rBV	683694	605763	13.15%	2.242%
14	15.204	2188	2196	2202	rBV	380044	452390	9.82%	1.675%




Sum of corrected areas: 27014810

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130243.D
Acq On : 14 Sep 2022 16:58
Operator : CG\JU
Sample : PB147629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

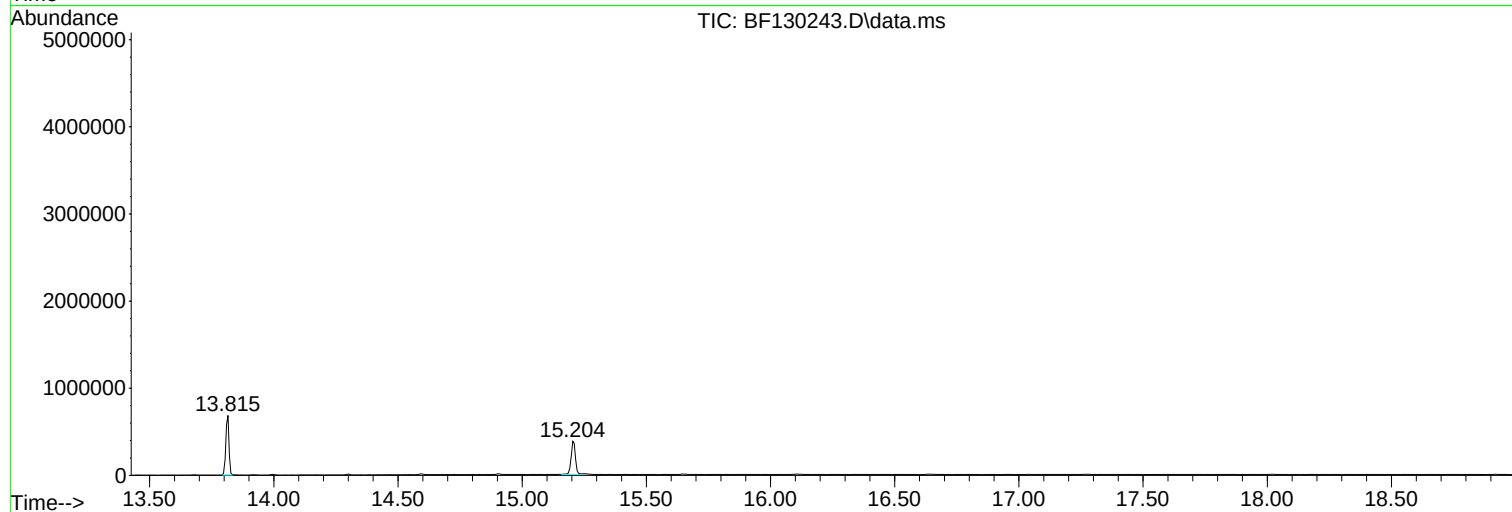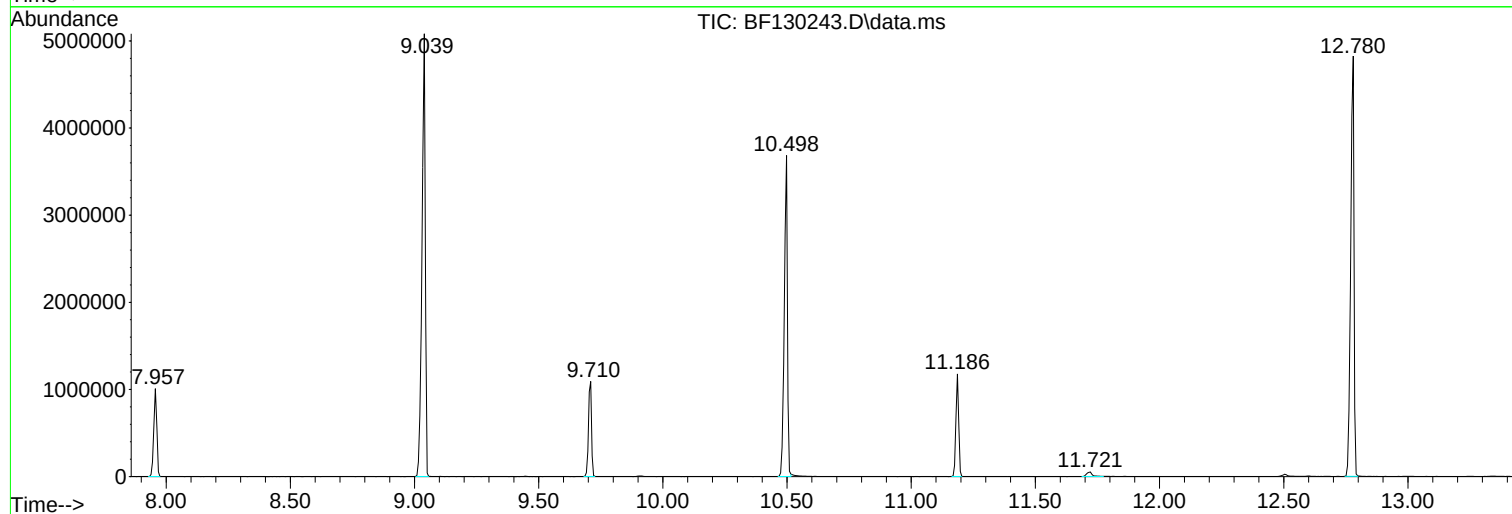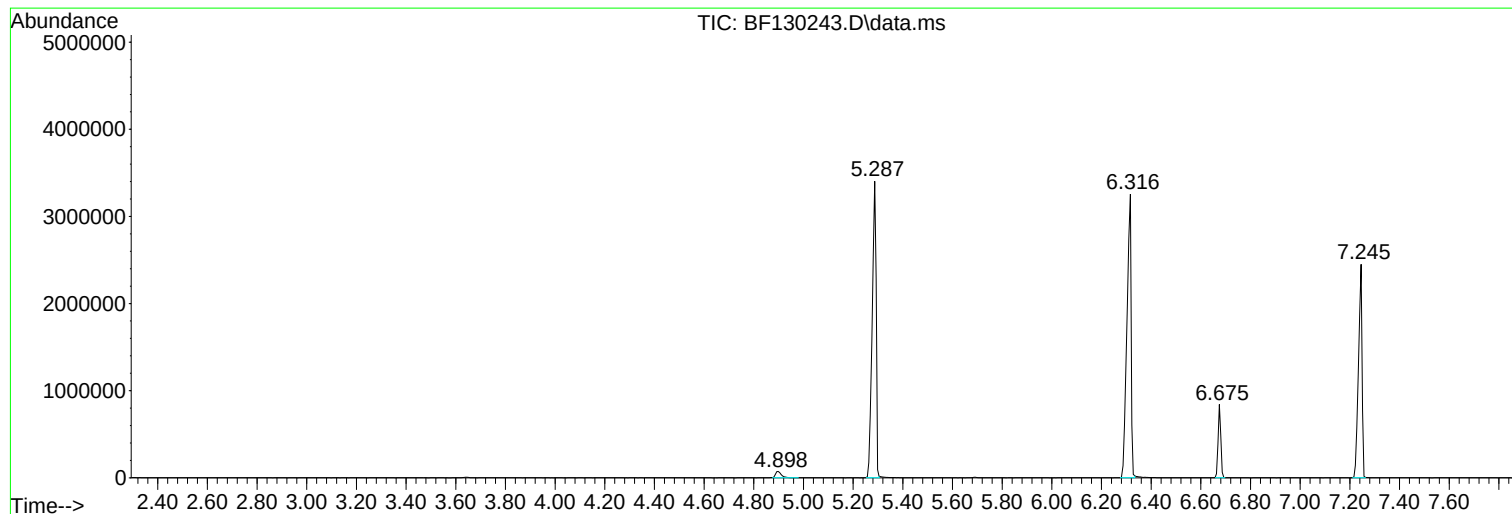

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130243.D
Acq On : 14 Sep 2022 16:58
Operator : CG\JU
Sample : PB147629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB147629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
4.898	3.69 ng	118264	1,4-Dichlorobenzene-d4	6.675	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	17
5	4-Pentene-2-ol, 2-methyl	100	C6H12O	000624-97-5	12

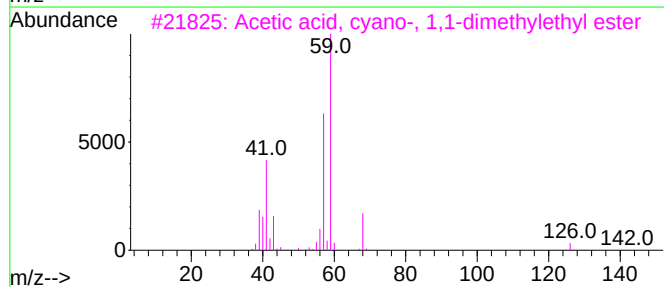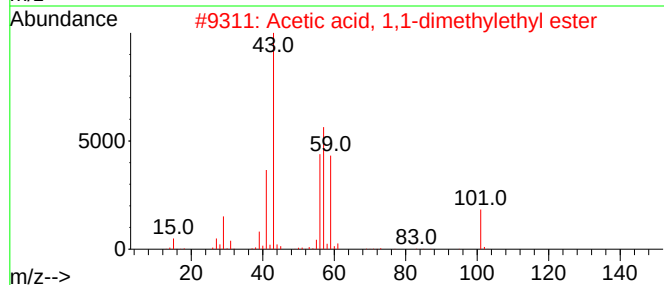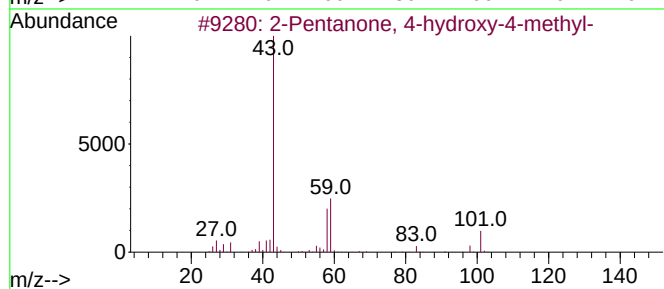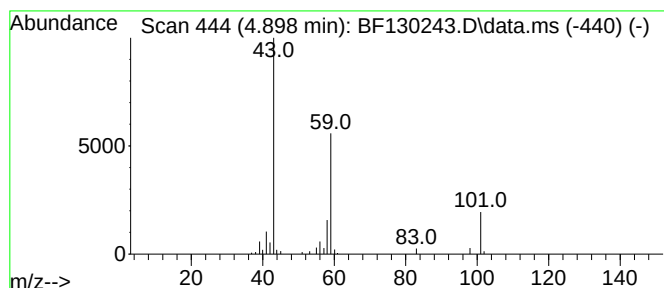

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130243.D
Acq On : 14 Sep 2022 16:58
Operator : CG\JU
Sample : PB147629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.898	3.7	ng	118264	1	6.675	640829	20.0