

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
 Data File : BF130261.D
 Acq On : 15 Sep 2022 02:36
 Operator : CG\JU
 Sample : N4551-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 2

Instrument :
 BNA_F
 ClientSampleId :
 251032-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.569	213	218	222	rBV	44505	71311	1.28%	0.267%
2	3.616	222	226	233	rVB	42012	60974	1.09%	0.228%
3	4.857	434	437	446	rVB	69277	82922	1.49%	0.310%
4	5.275	503	508	511	rBV	1609931	1614213	28.96%	6.041%
5	6.298	678	682	702	rVB	1141583	1077010	19.32%	4.031%
6	6.675	742	746	749	rBV	1673642	1325199	23.77%	4.959%
7	7.245	837	843	845	rBV	1887519	2000090	35.88%	7.485%
8	7.957	959	964	967	rBV	2139545	1743364	31.27%	6.524%
9	9.034	1142	1147	1150	rBV	4078038	3677615	65.97%	13.763%
10	9.710	1257	1262	1265	rBV	2174418	1922058	34.48%	7.193%
11	10.492	1390	1395	1398	rBV	2968455	2404199	43.13%	8.998%
12	11.186	1509	1513	1516	rBV	2264924	1829523	32.82%	6.847%
13	11.722	1600	1604	1607	rBV	151784	139489	2.50%	0.522%
14	12.604	1750	1754	1757	rBV	224395	189446	3.40%	0.709%
15	12.775	1778	1783	1786	rBV	6111418	5574718	100.00%	20.863%
16	13.304	1870	1873	1876	rBV	121275	102301	1.84%	0.383%
17	13.816	1955	1960	1963	rBV	2145708	2054277	36.85%	7.688%
18	15.204	2191	2196	2202	rBV	759099	851905	15.28%	3.188%




Sum of corrected areas: 26720614

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130261.D
Acq On : 15 Sep 2022 02:36
Operator : CG\JU
Sample : N4551-01
Misc :
ALS Vial : 21 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
251032-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

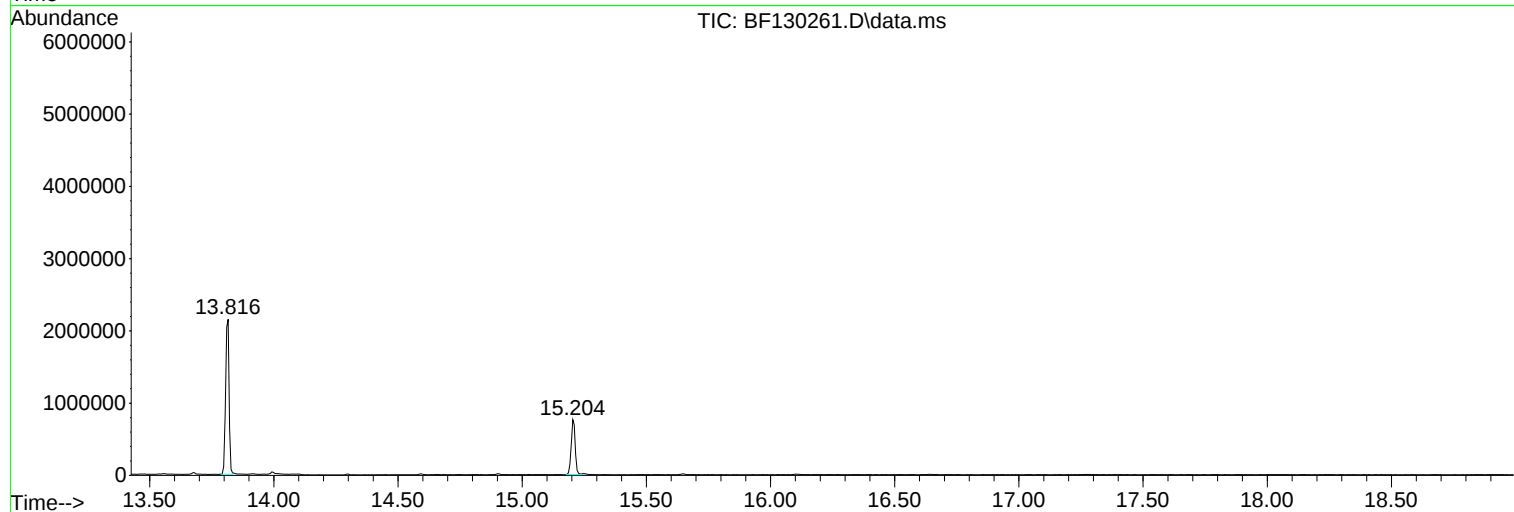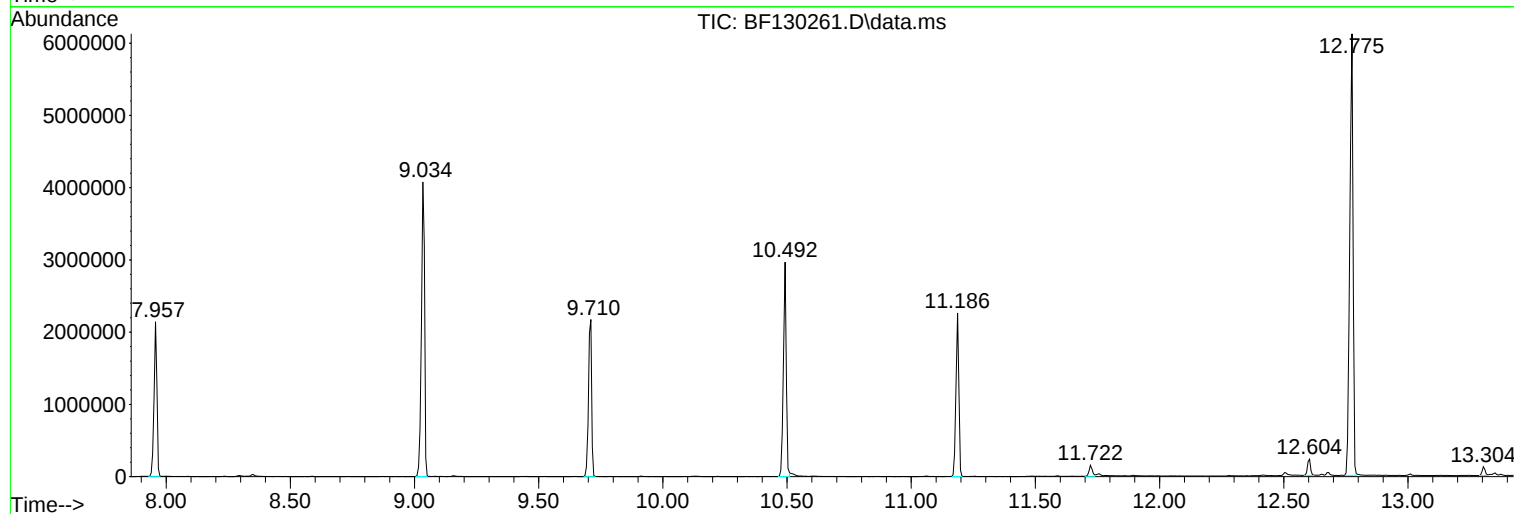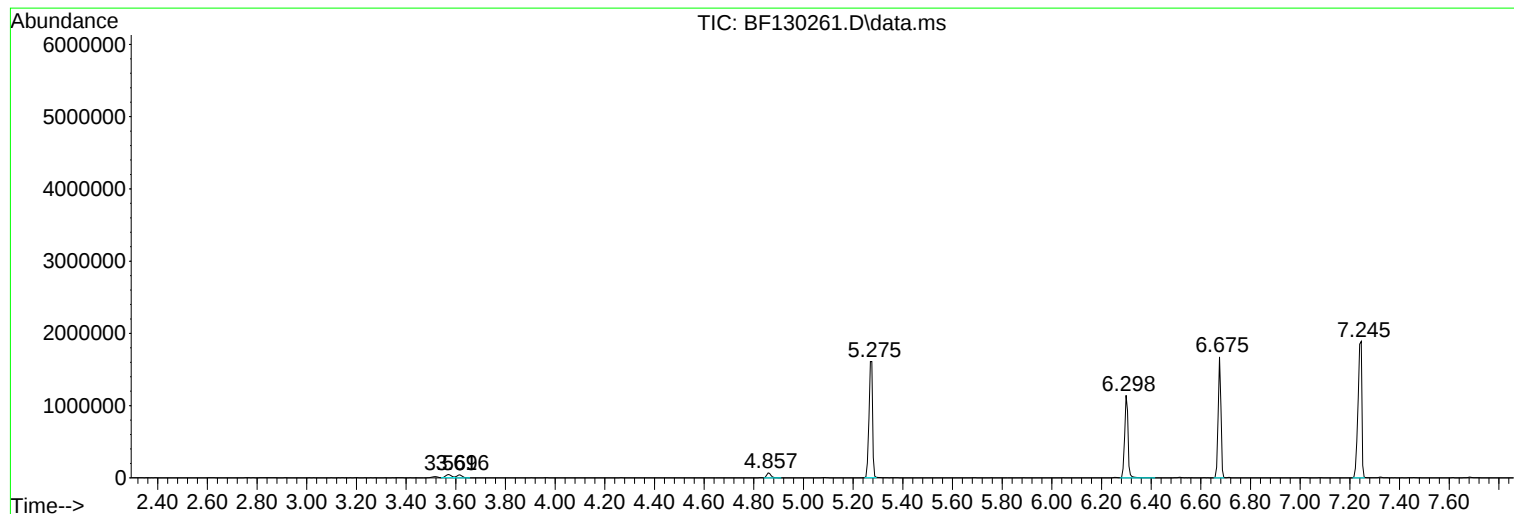

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130261.D
Acq On : 15 Sep 2022 02:36
Operator : CG\JU
Sample : N4551-01
Misc :
ALS Vial : 21 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
251032-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130261.D
Acq On : 15 Sep 2022 02:36
Operator : CG\JU
Sample : N4551-01
Misc :
ALS Vial : 21 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
251032-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------