


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
 Data File : BF130231.D
 Acq On : 14 Sep 2022 10:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 14:55:51 2022

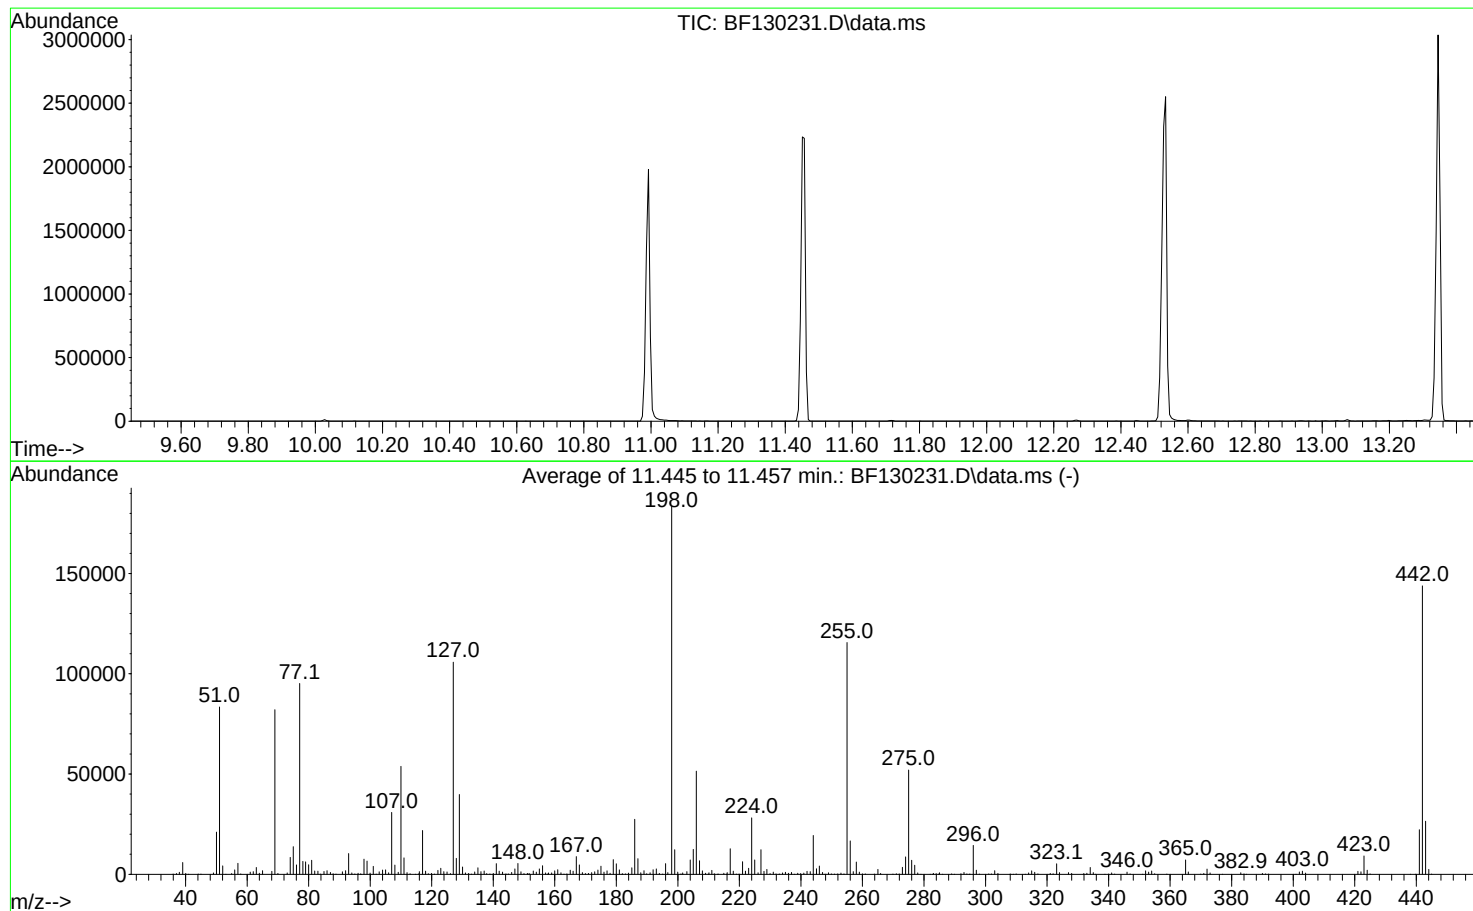




AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	83400	PASS
68	69	0.00	2	1.8	1460	PASS
69	198	0.00	100	44.7	82069	PASS
70	69	0.00	2	0.6	461	PASS
127	198	10	80	57.7	105792	PASS
197	198	0.00	2	0.5	851	PASS
198	198	100	100	100.0	183459	PASS
199	198	5	9	6.7	12219	PASS
275	198	10	60	28.3	51984	PASS
365	198	1	100	3.9	7165	PASS
441	198	0.01	100	12.1	22208	PASS
442	442	50	100	100.0	143875	PASS
443	442	15	24	18.4	26492	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130231.D
Acq On : 14 Sep 2022 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 14 13:59:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 13:52:44 2022
Response via : Initial Calibration

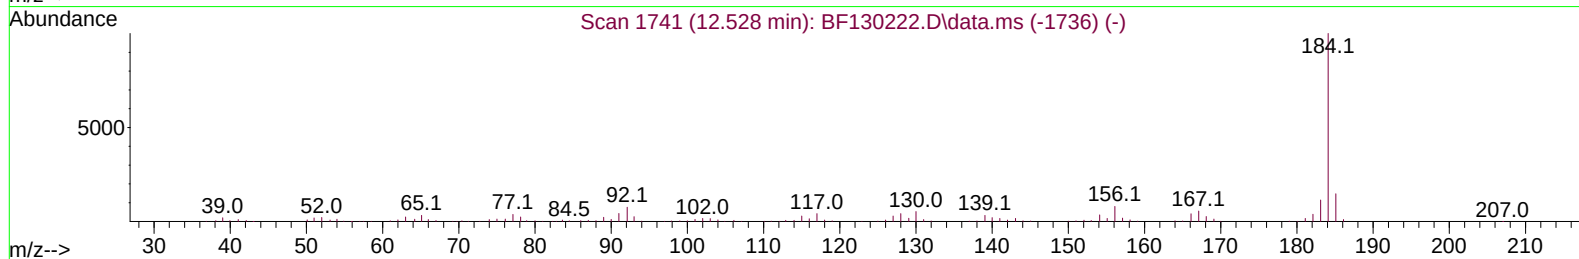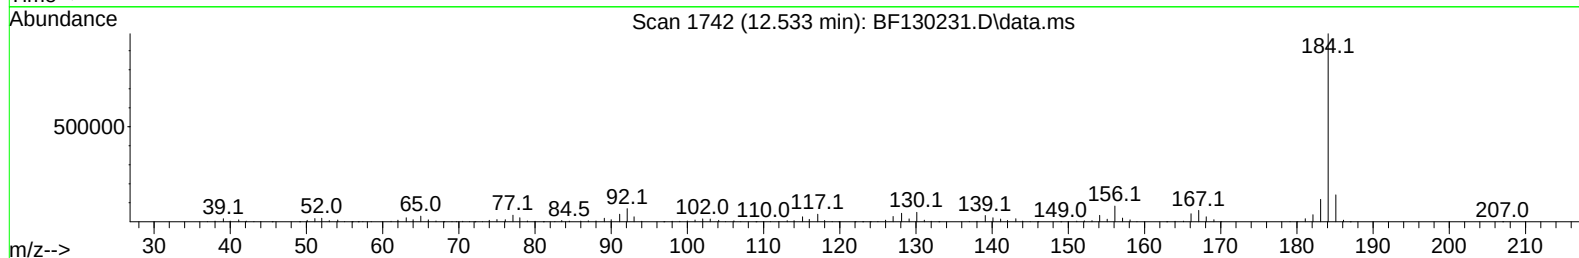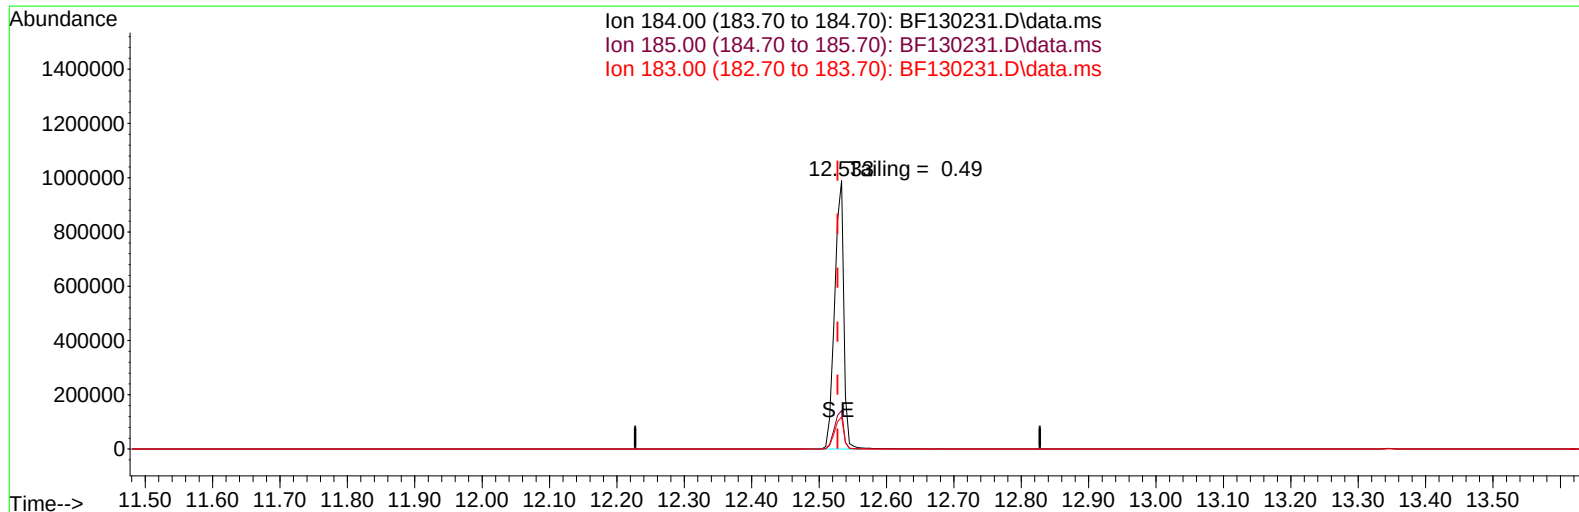

TIC: BF130231.D\data.ms

(77) Benzidine

12.533min (+ 0.006) 0.00 ng

response 932976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.32
183.00	11.40	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2022	BNA_F	<u>BF130231.D</u>
Compound Name	Response	Retention Time
DDT	418551	13.34
DDD	746	13.04
DDE	0	12.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
746	419297	0.18

Instrument :
BNA_F
ClientSampleId :
DFTPP