
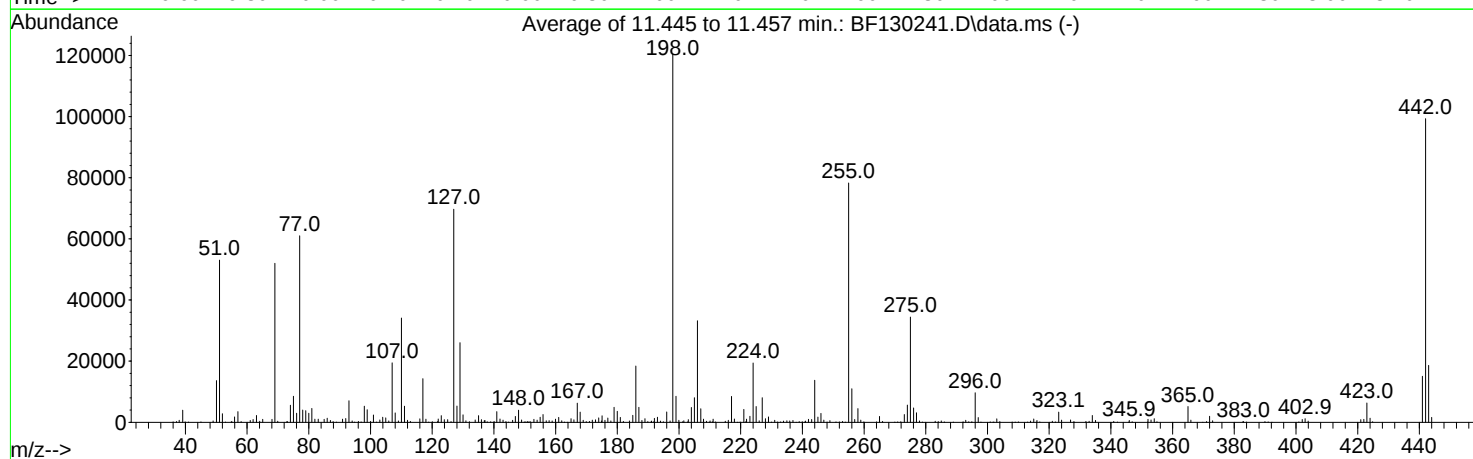


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
 Data File : BF130241.D
 Acq On : 14 Sep 2022 15:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 14:55:51 2022

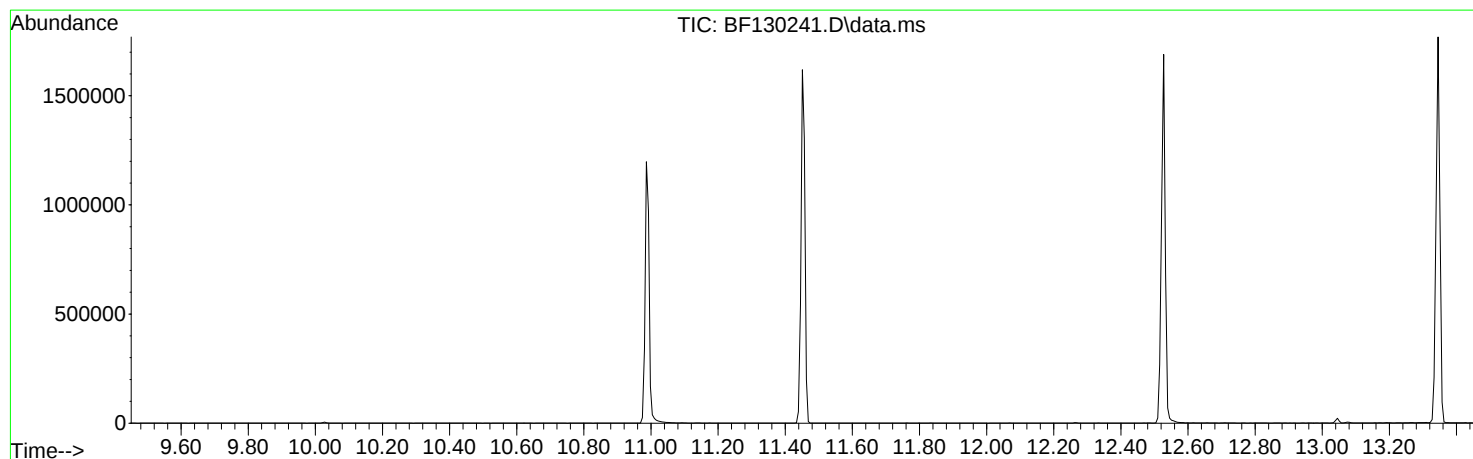




AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	53040	PASS
68	69	0.00	2	1.9	990	PASS
69	198	0.00	100	43.2	51981	PASS
70	69	0.00	2	0.6	318	PASS
127	198	10	80	57.9	69699	PASS
197	198	0.00	2	0.4	434	PASS
198	198	100	100	100.0	120341	PASS
199	198	5	9	7.1	8497	PASS
275	198	10	60	28.6	34420	PASS
365	198	1	100	4.3	5177	PASS
441	198	0.01	100	12.5	15048	PASS
442	442	50	100	100.0	99312	PASS
443	442	15	24	18.7	18602	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
 Data File : BF130241.D
 Acq On : 14 Sep 2022 15:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 05:55:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 14:55:51 2022
 Response via : Initial Calibration

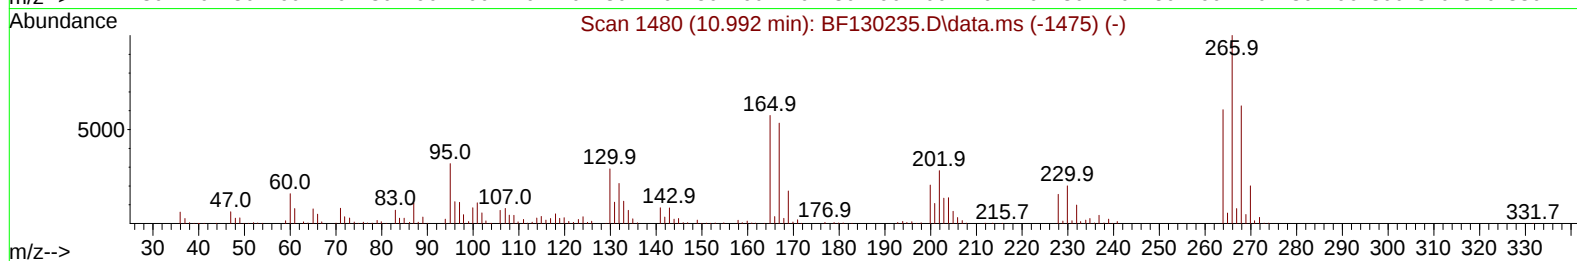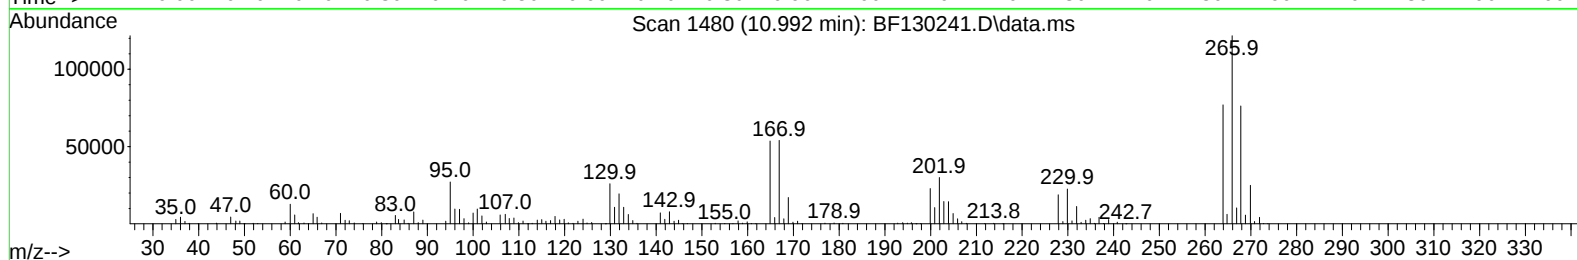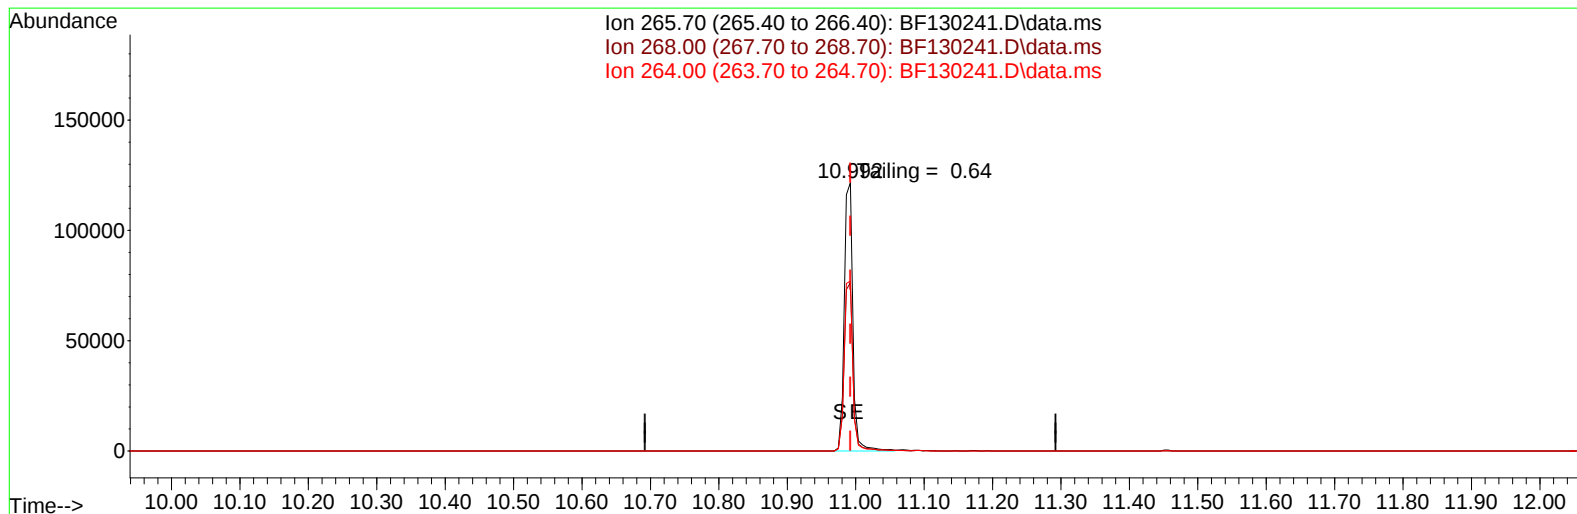

TIC: BF130241.D\data.ms

(70) Pentachlorophenol (C)

10.992min (+ 0.000) 25401.93 ng




response 106721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.71
264.00	63.10	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091422\
Data File : BF130241.D
Acq On : 14 Sep 2022 15:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 05:55:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 14:55:51 2022
Response via : Initial Calibration

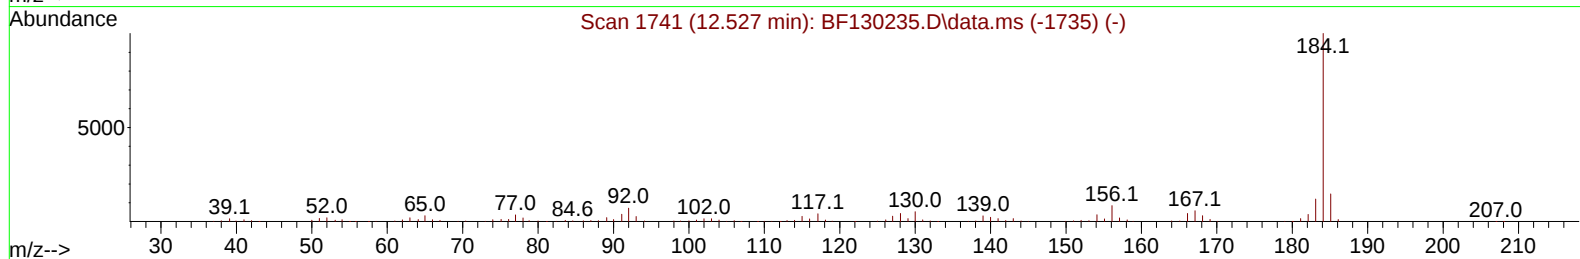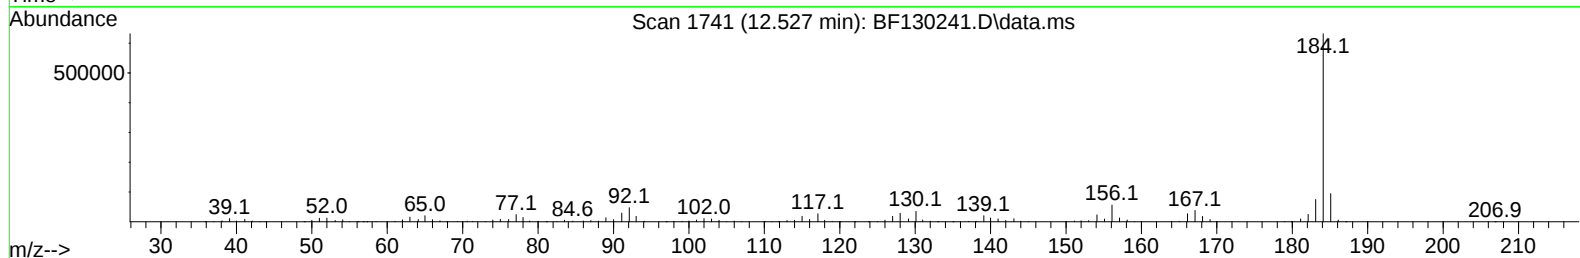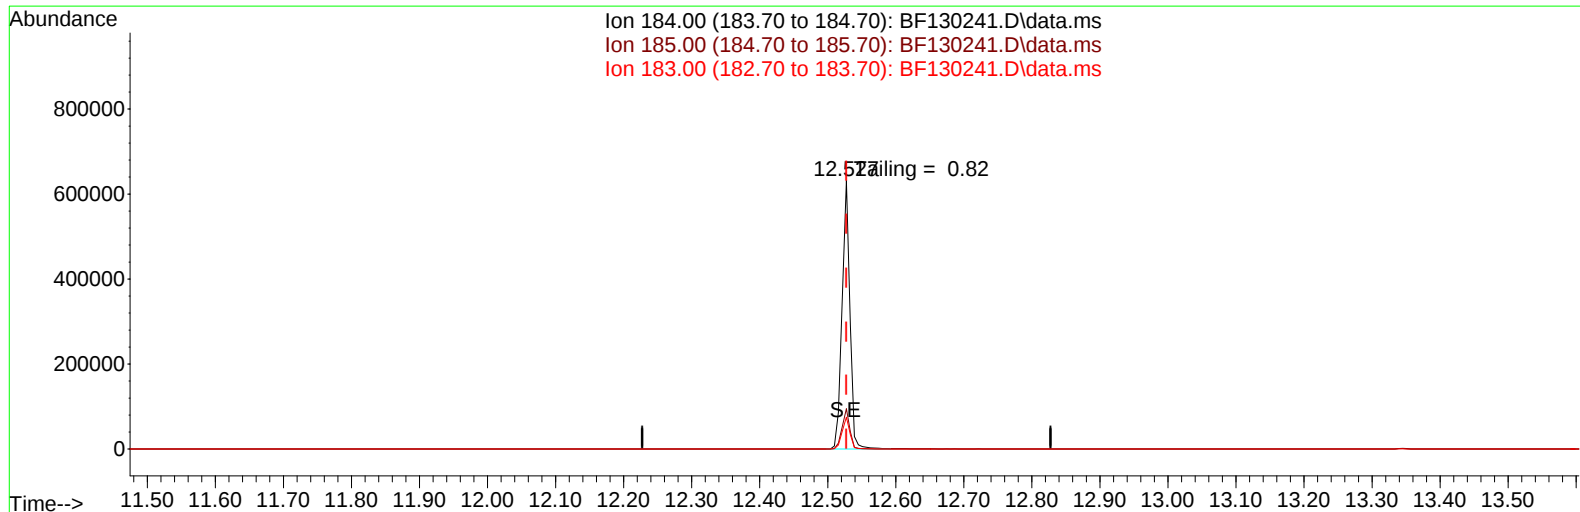

TIC: BF130241.D\data.ms

(77) Benzidine

12.527min (+ 0.000) 0.00 ng

response 507471

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.02
183.00	11.40	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2022	BNA_F	<u>BF130241.D</u>
Compound Name	Response	Retention Time
DDT	252437	13.345
DDD	4332	13.045
DDE	193	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4525	256962	1.76

Instrument :
BNA_F
ClientSampleId :
DFTPP