
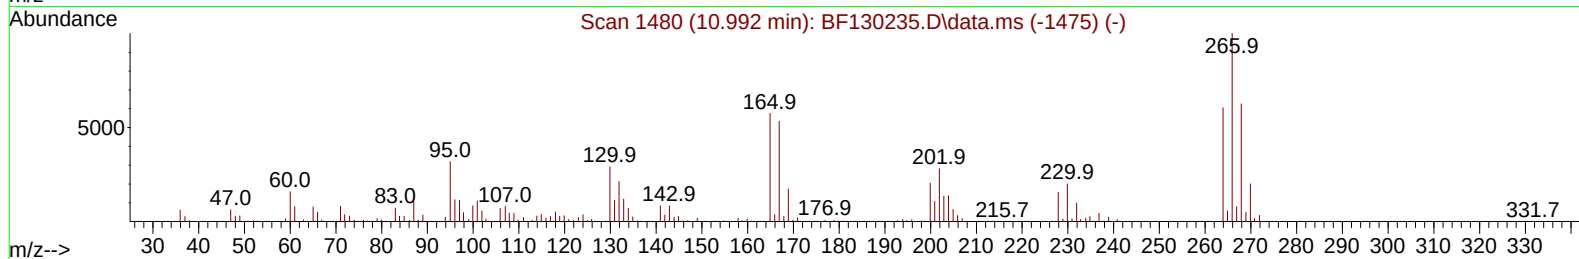
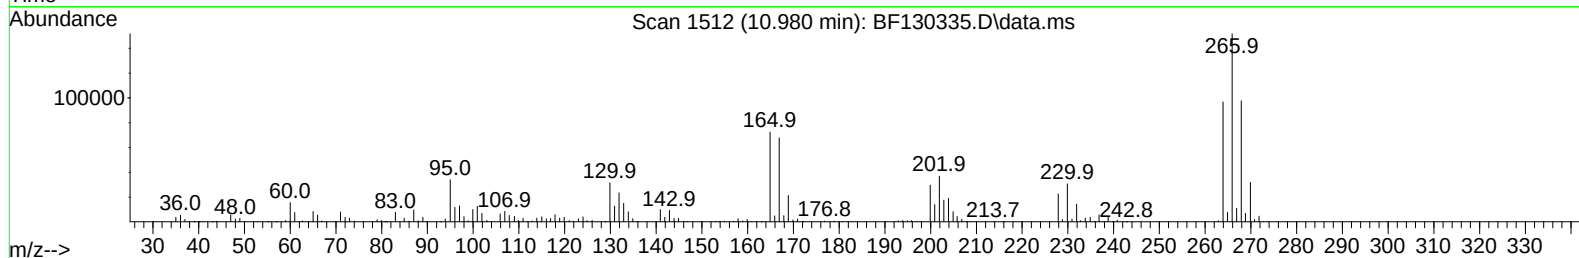


Quant Time: Sep 21 05:31:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

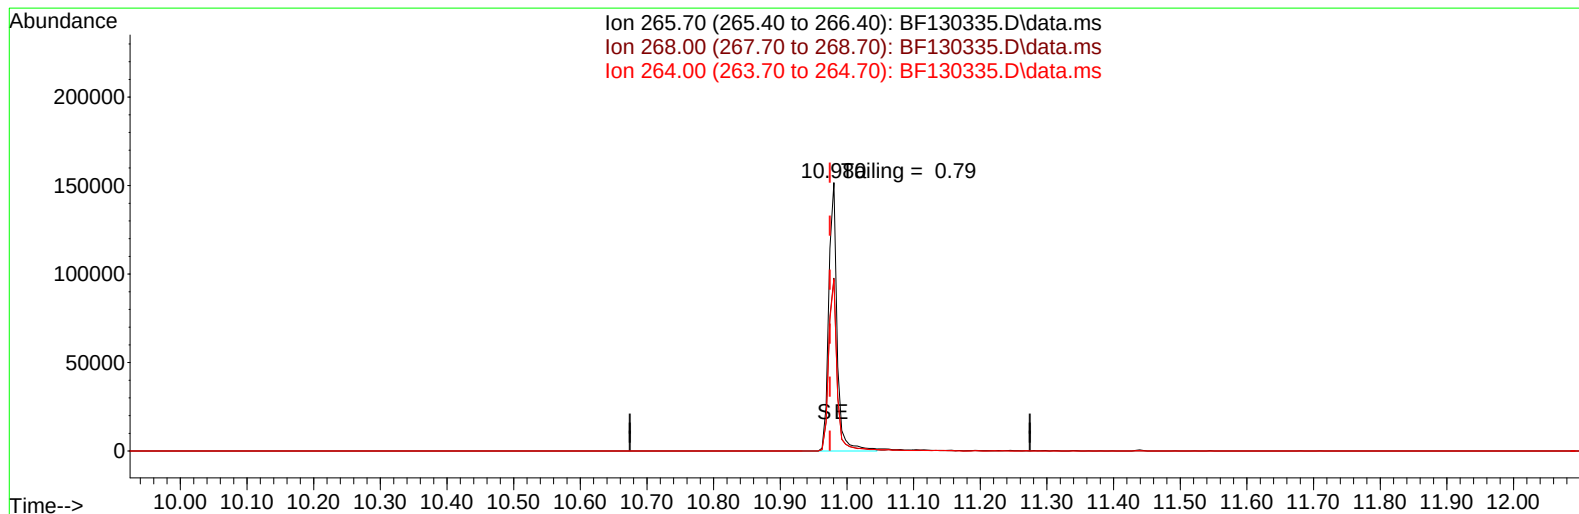

TIC: BF130335.D\data.ms

(70) Pentachlorophenol (C)




10.980min (+ 0.006) 0.00 ng

response **135278**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.41
264.00	63.10	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
Data File : BF130335.D
Acq On : 20 Sep 2022 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 05:31:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

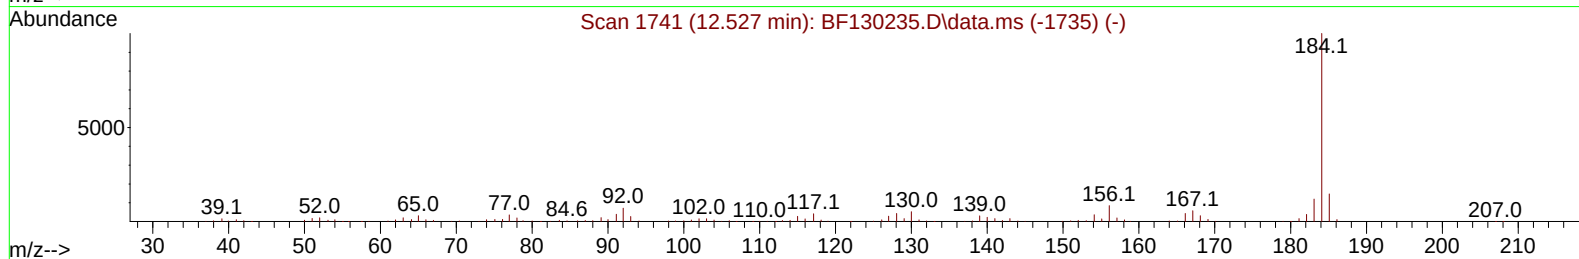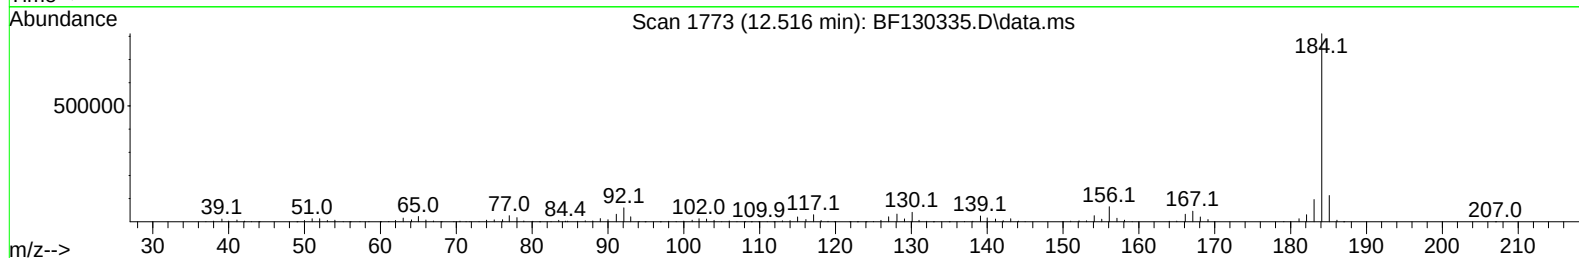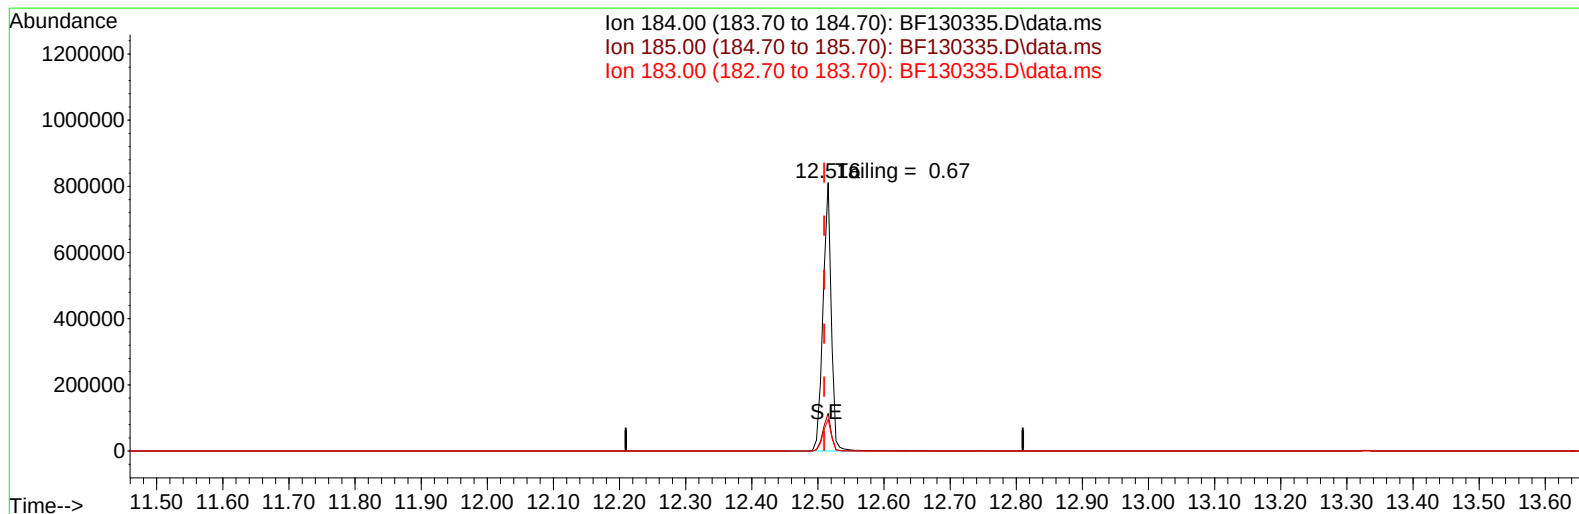

TIC: BF130335.D\data.ms

(77) Benzidine

12.516min (+ 0.006) 82914.18 ng

response 702822

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.02
183.00	11.40	11.85
0.00	0.00	0.00