

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
 Data File : BF130352.D
 Acq On : 20 Sep 2022 19:30
 Operator : CG\JU
 Sample : N4714-01 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-01-091922

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.569	247	252	258	rVB	8251	12754	1.53%	0.189%
2	5.263	536	540	552	rBV	484778	487276	58.58%	7.238%
3	6.304	713	717	729	rBV	419712	466697	56.10%	6.932%
4	6.663	774	778	781	rBV	868295	707823	85.09%	10.514%
5	7.222	869	873	883	rBV	348360	293974	35.34%	4.367%
6	7.945	991	996	999	rBV	1054243	831837	100.00%	12.356%
7	9.022	1173	1179	1182	rBV	615239	541080	65.05%	8.037%
8	9.557	1266	1270	1275	rBV	20527	18199	2.19%	0.270%
9	9.692	1290	1293	1297	rVB	912551	780279	93.80%	11.590%
10	10.481	1423	1427	1434	rBV	321822	267035	32.10%	3.967%
11	10.610	1445	1449	1454	rVB7	13878	19467	2.34%	0.289%
12	11.175	1541	1545	1548	rBV	831592	674576	81.09%	10.020%
13	11.198	1548	1549	1554	rVV	31756	22752	2.74%	0.338%
14	11.245	1555	1557	1561	rVB2	12252	12174	1.46%	0.181%
15	11.675	1628	1630	1632	rBV	19253	18568	2.23%	0.276%
16	11.704	1633	1635	1637	rVV	22624	18861	2.27%	0.280%
17	11.786	1646	1649	1651	rBV	22880	22795	2.74%	0.339%
18	12.222	1721	1723	1727	rBV	39713	38920	4.68%	0.578%
19	12.380	1748	1750	1754	rBV	48281	48304	5.81%	0.718%
20	12.610	1786	1789	1793	rBV	81648	71922	8.65%	1.068%
21	12.757	1811	1814	1822	rVB	514718	436469	52.47%	6.483%
22	13.810	1989	1993	1995	rBV	583087	576272	69.28%	8.560%
23	15.204	2227	2230	2233	rVB	345072	364135	43.77%	5.409%




Sum of corrected areas: 6732169

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
Data File : BF130352.D
Acq On : 20 Sep 2022 19:30
Operator : CG\JU
Sample : N4714-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-091922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

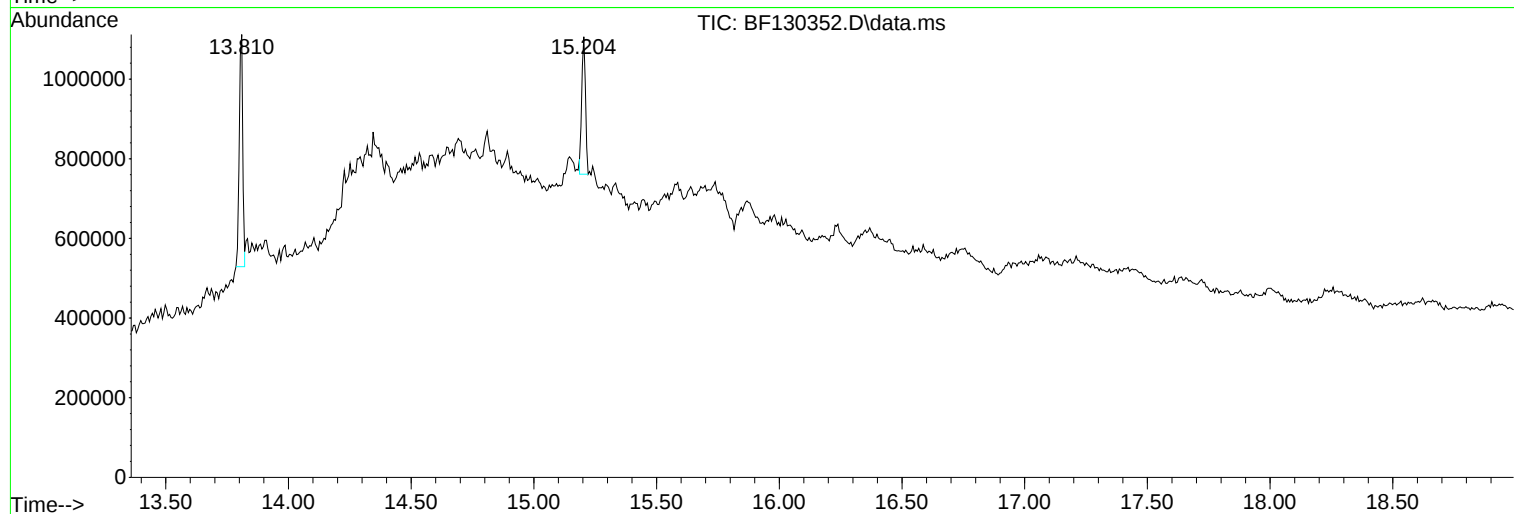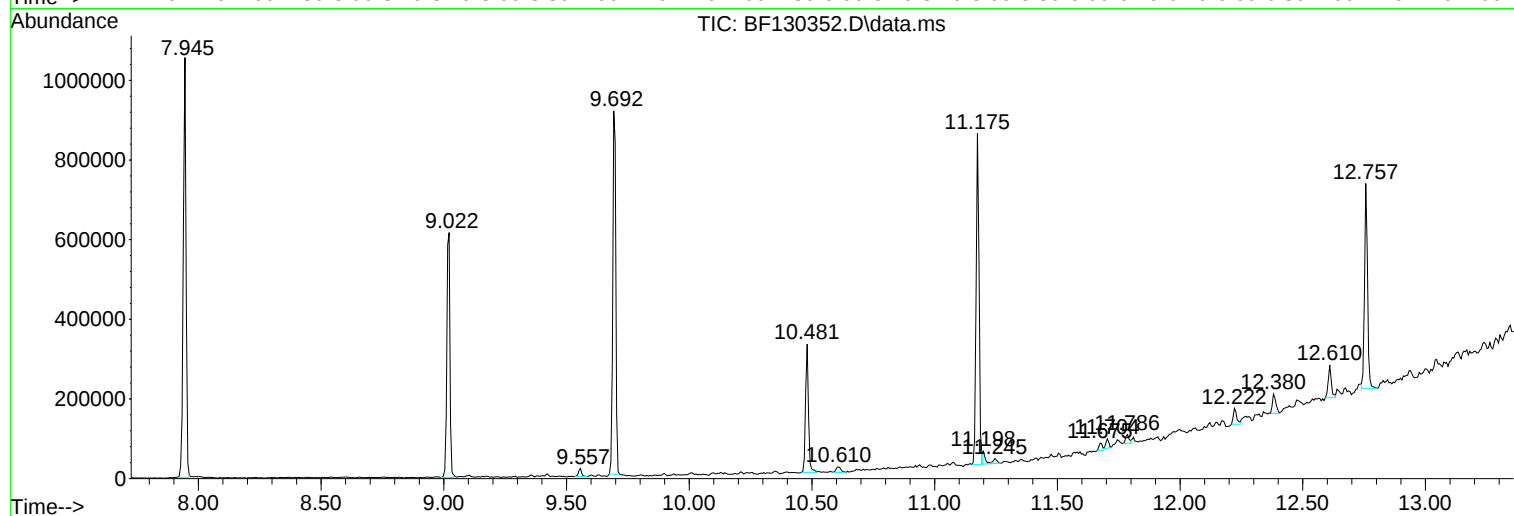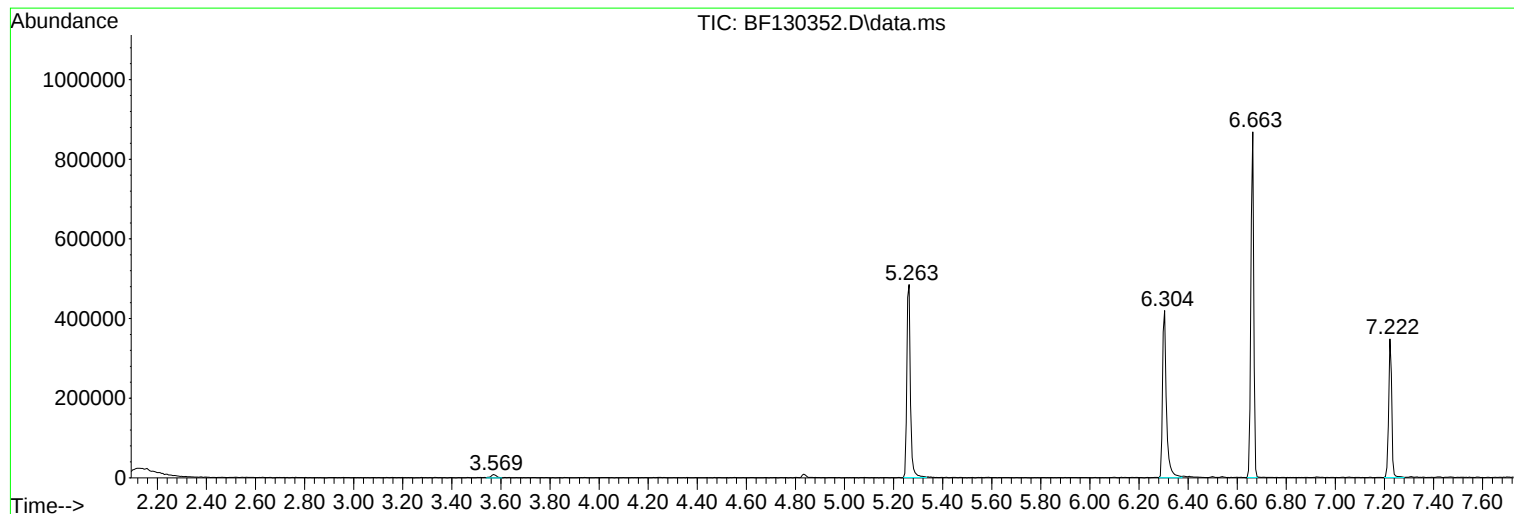

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
Data File : BF130352.D
Acq On : 20 Sep 2022 19:30
Operator : CG\JU
Sample : N4714-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-091922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
Data File : BF130352.D
Acq On : 20 Sep 2022 19:30
Operator : CG\JU
Sample : N4714-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-091922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------