


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
 Data File : BF130335.D
 Acq On : 20 Sep 2022 10:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 15:06:14 2022

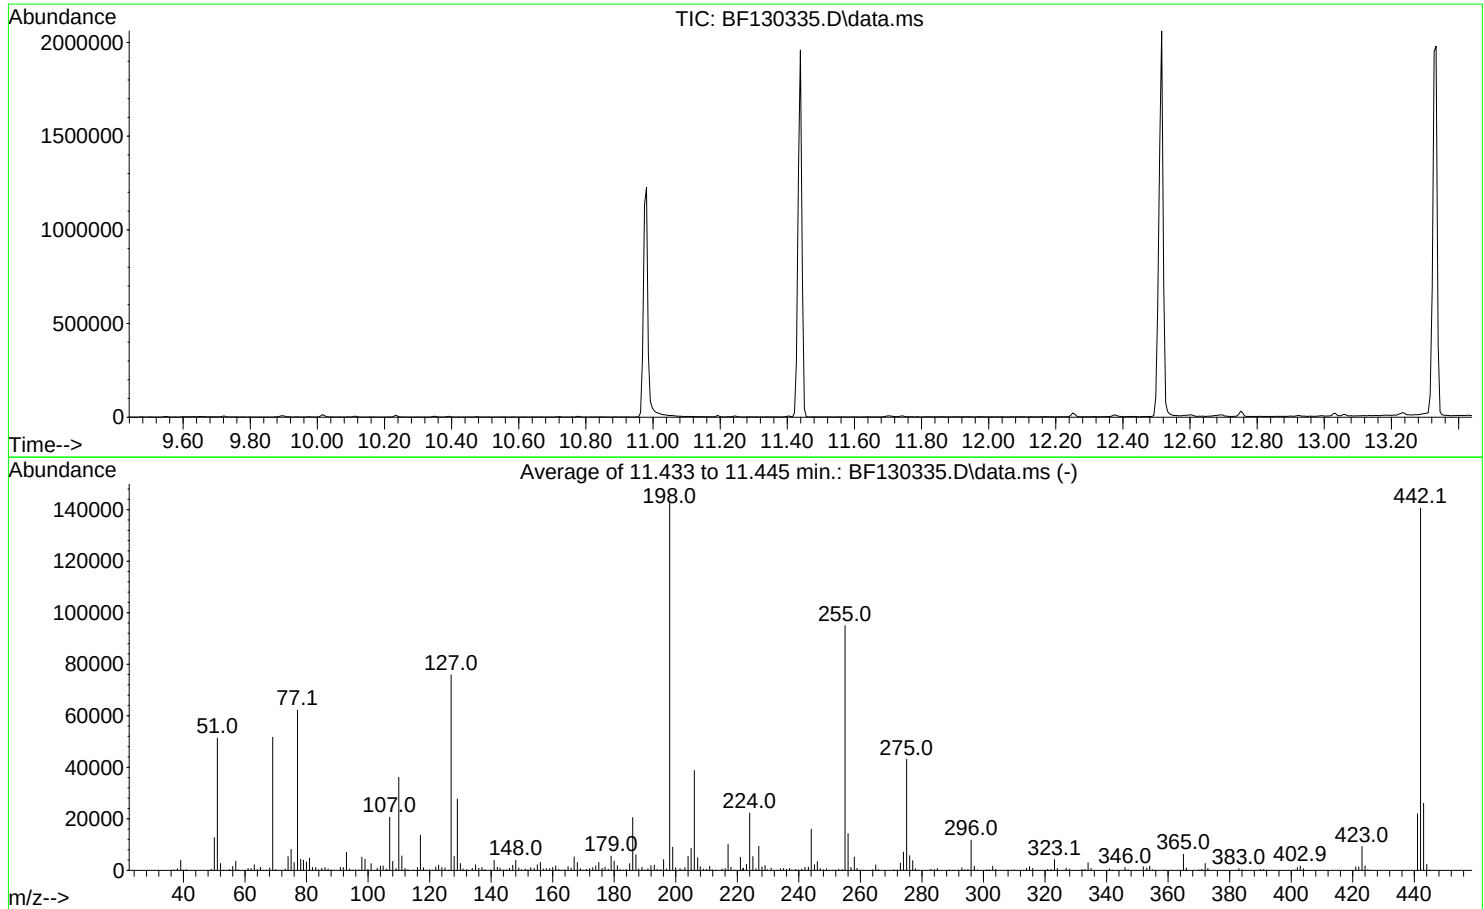




AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	51260	PASS
68	69	0.00	2	1.7	895	PASS
69	198	0.00	100	36.2	51672	PASS
70	69	0.00	2	0.5	268	PASS
127	198	10	80	53.1	75877	PASS
197	198	0.00	2	0.4	546	PASS
198	198	100	100	100.0	142813	PASS
199	198	5	9	6.3	8989	PASS
275	198	10	60	30.2	43093	PASS
365	198	1	100	4.4	6257	PASS
441	198	0.01	100	15.4	21928	PASS
442	442	50	100	100.0	140611	PASS
443	442	15	24	18.5	25988	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
Data File : BF130335.D
Acq On : 20 Sep 2022 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 21 05:31:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

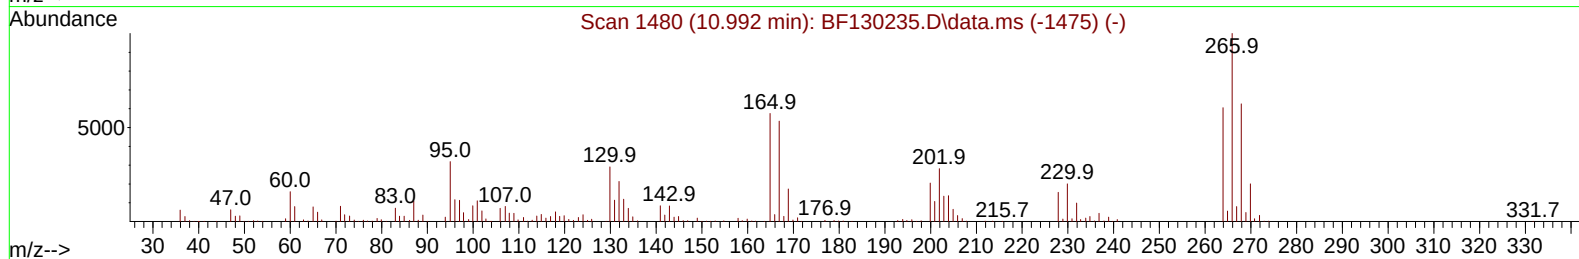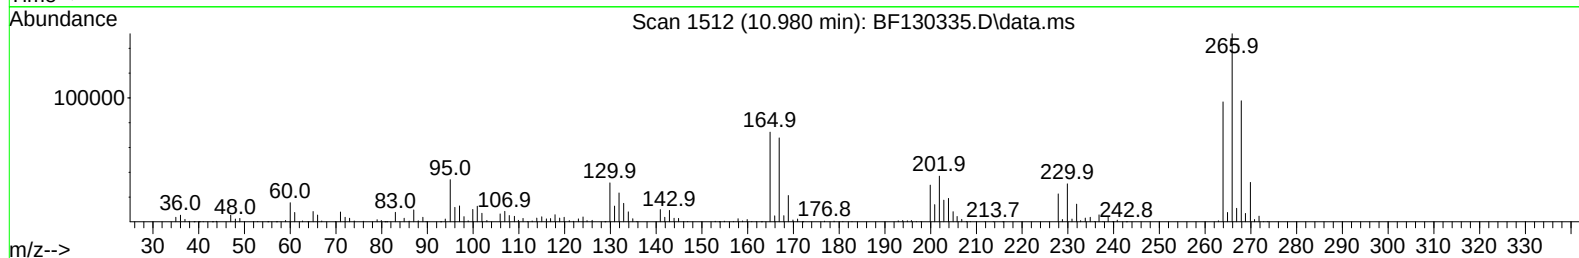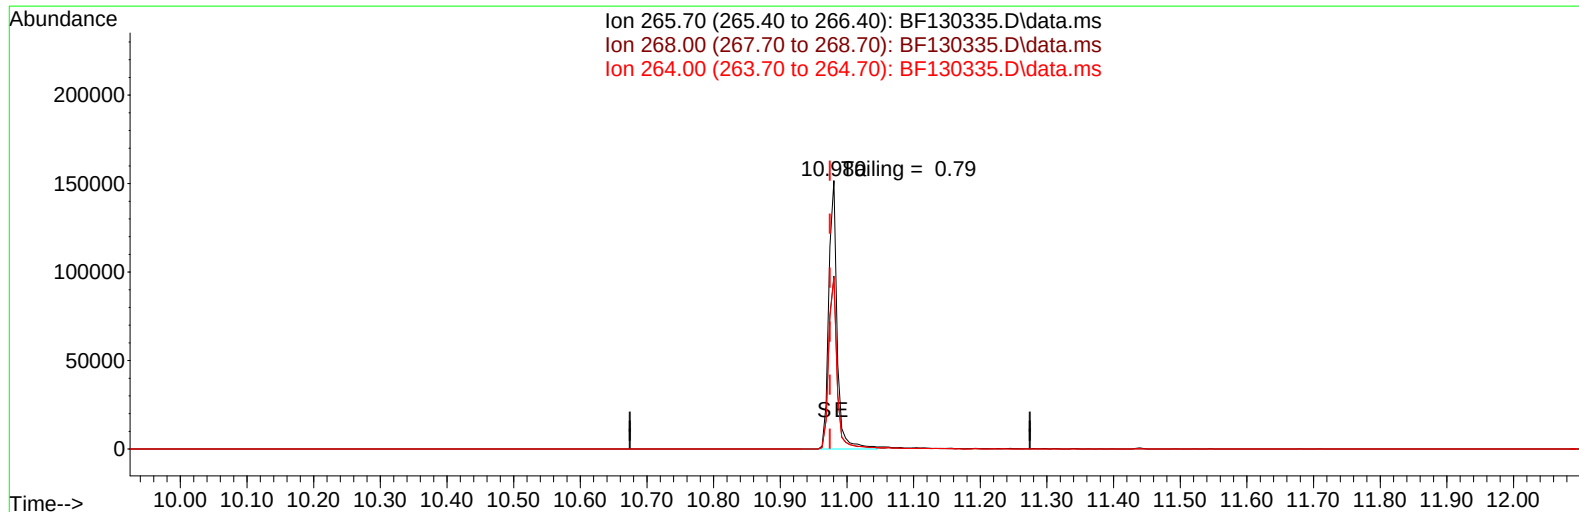

TIC: BF130335.D\data.ms

(70) Pentachlorophenol (C)

10.980min (+ 0.006) 0.00 ng




response 135278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.41
264.00	63.10	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092022\
Data File : BF130335.D
Acq On : 20 Sep 2022 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 21 05:31:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

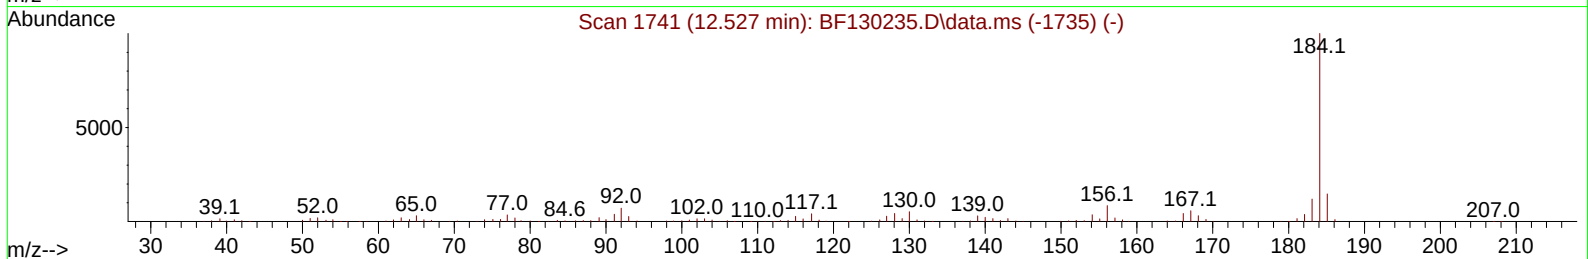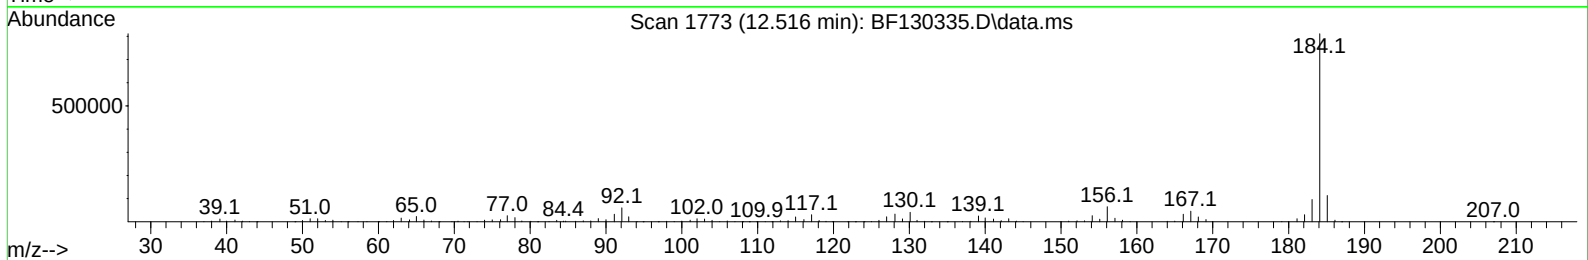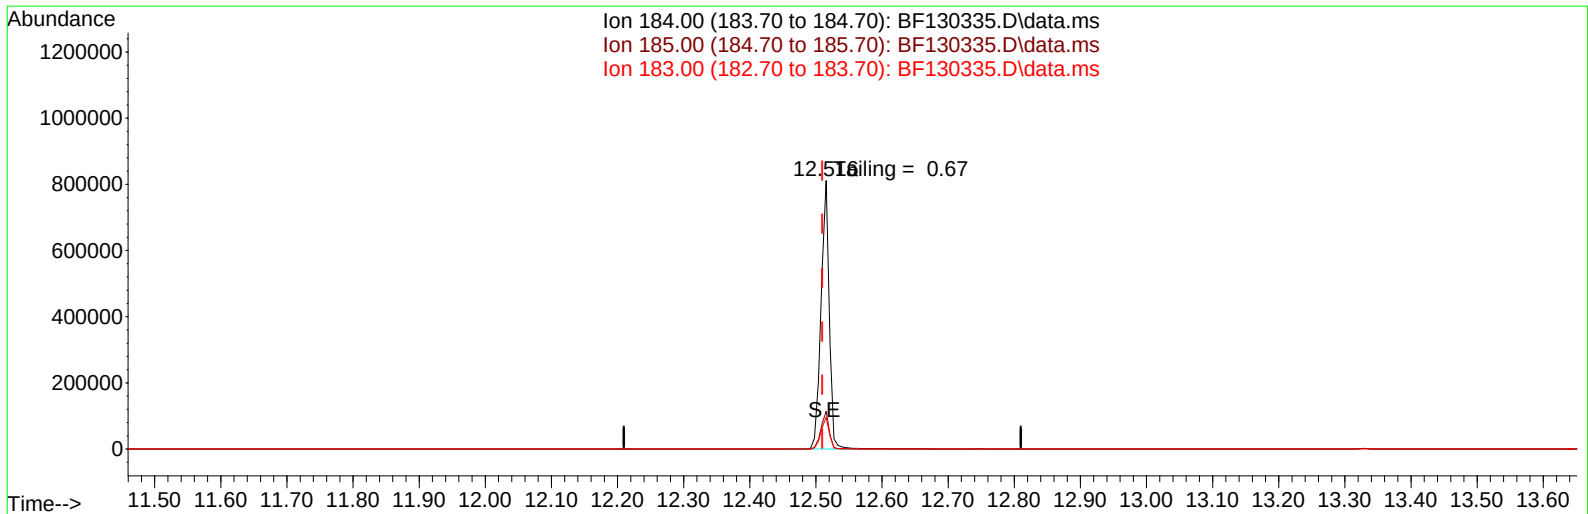

TIC: BF130335.D\data.ms

(77) Benzidine

12.516min (+ 0.006) 82914.18 ng

response 702822

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.02
183.00	11.40	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2022	BNA_F	<u>BF130335.D</u>
Compound Name	Response	Retention Time
DDT	337791	13.33
DDD	2791	13.03
DDE	1035	12.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3826	341617	1.12

Instrument :
BNA_F
ClientSampleId :
DFTPP