
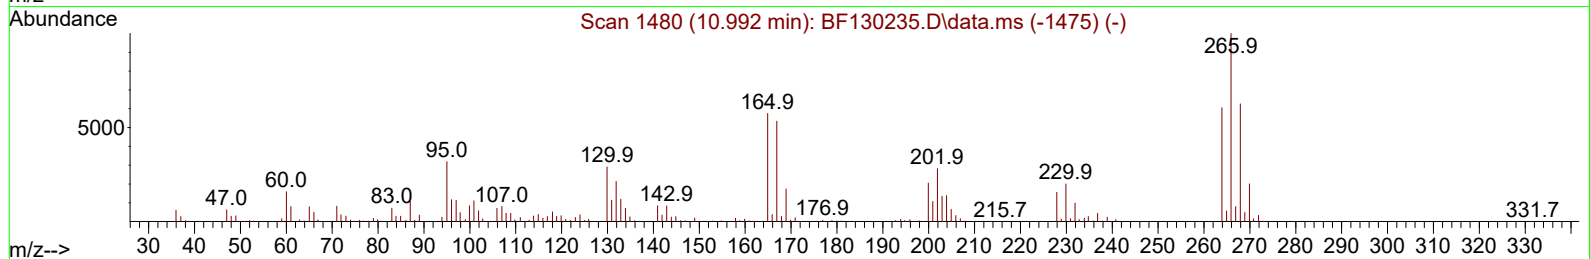
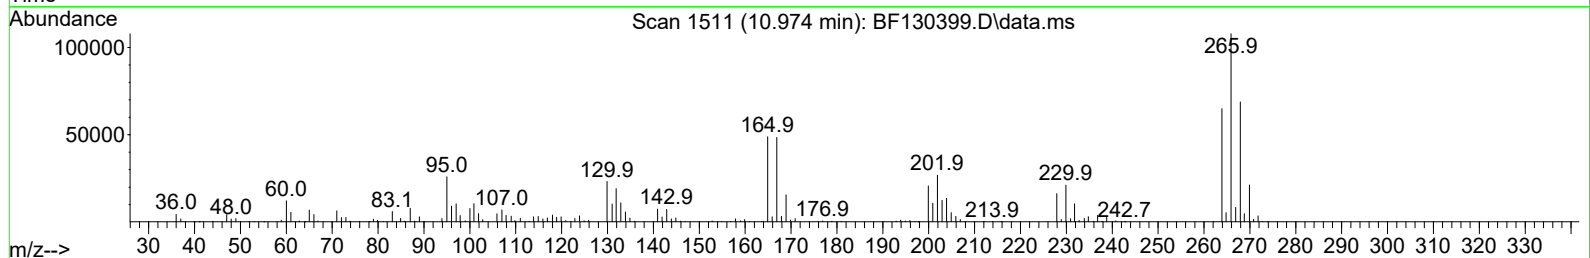


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130399.D
Acq On : 26 Sep 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 06:55:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration

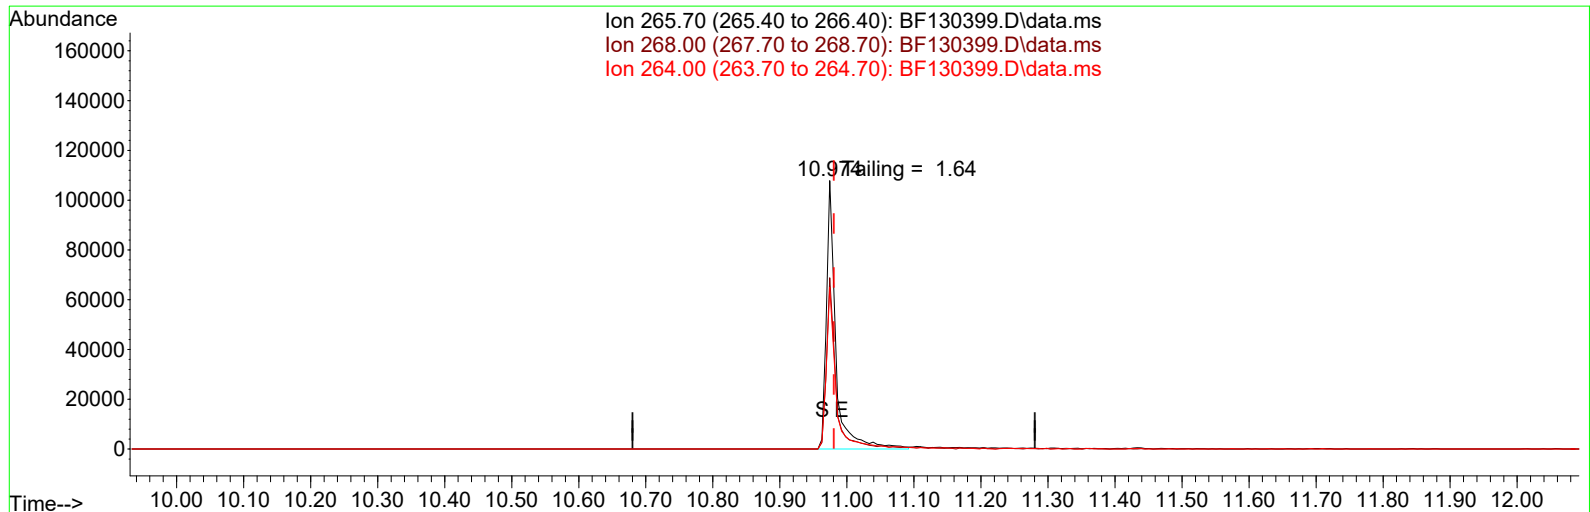

TIC: BF130399.D\data.ms

(70) Pentachlorophenol (C)




10.974min (-0.006) 27636.81 ng

response 105909

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.80
264.00	63.10	60.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130399.D
Acq On : 26 Sep 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 06:55:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration

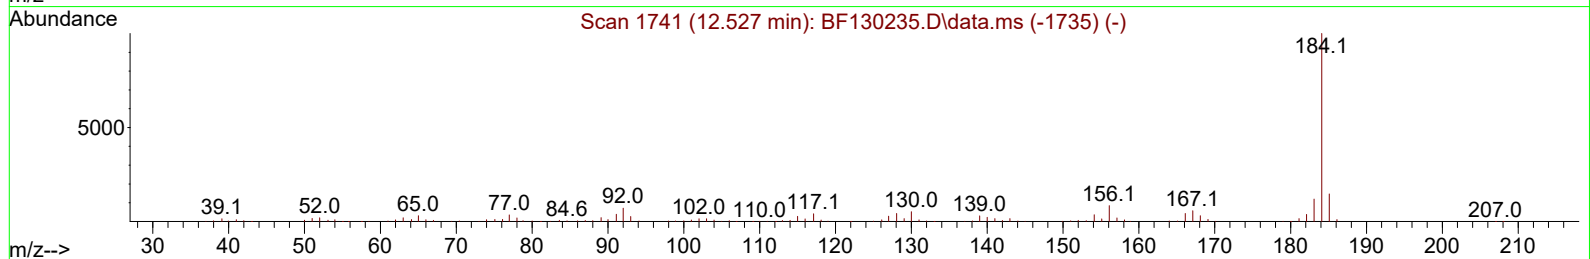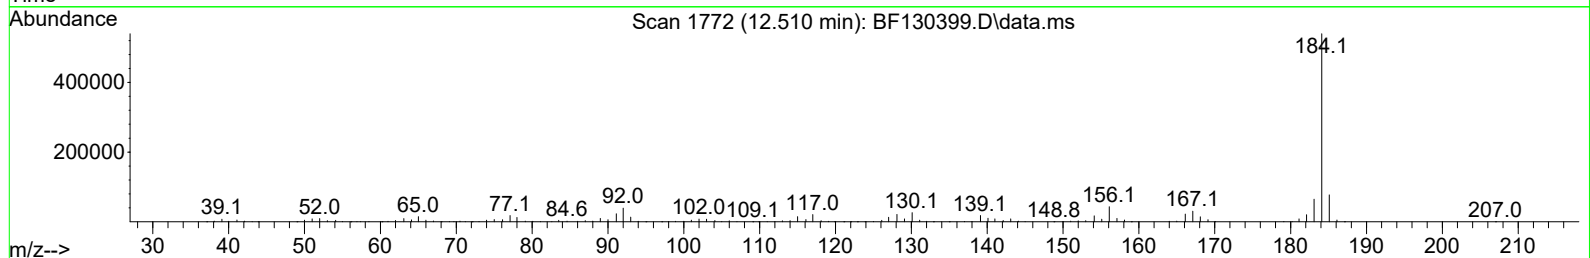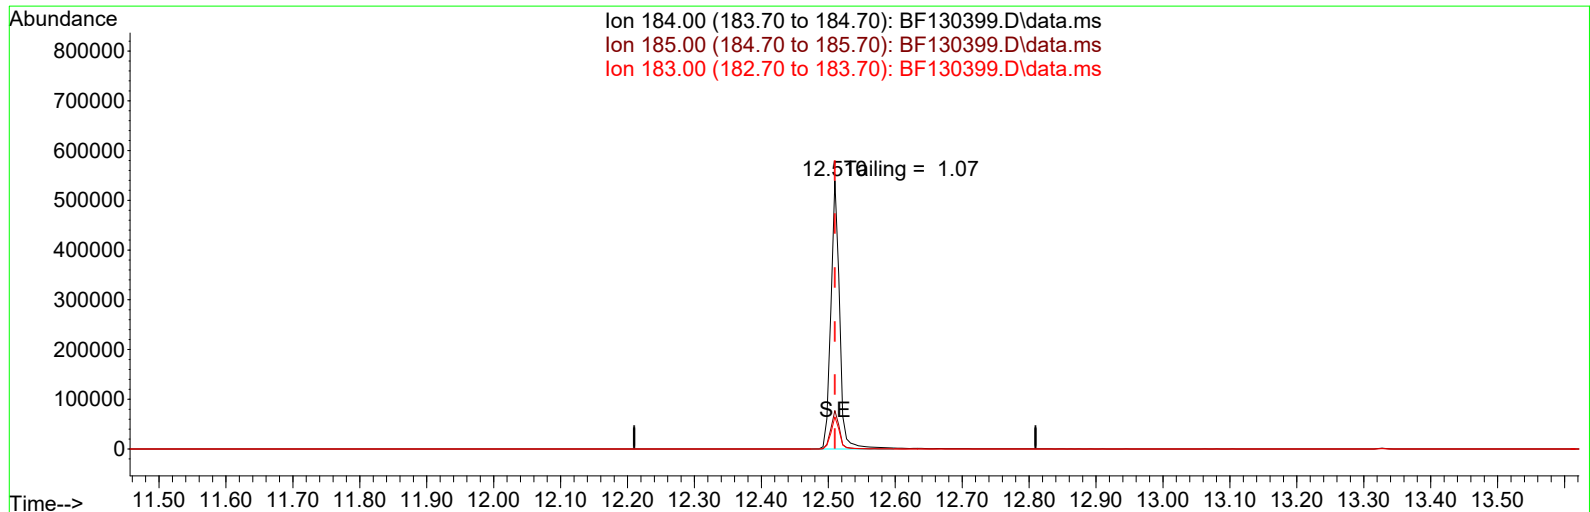

TIC: BF130399.D\data.ms

(77) Benzidine

12.510min (-0.000) 0.00 ng

response 490341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.34
183.00	11.40	12.03
0.00	0.00	0.00