

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
 Data File : BF130401.D
 Acq On : 26 Sep 2022 10:38
 Operator : CG\JU
 Sample : PB147858BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147858BL

Quant Time: Sep 27 01:03:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 27 01:00:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.651	152	106046	20.000	ng	0.00
21) Naphthalene-d8	7.934	136	431324	20.000	ng	# 0.00
39) Acenaphthene-d10	9.687	164	233705	20.000	ng	0.00
64) Phenanthrene-d10	11.169	188	419572	20.000	ng	0.00
76) Chrysene-d12	13.798	240	296294	20.000	ng	0.00
86) Perylene-d12	15.192	264	225847	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.263	112	606631	99.219	ng	0.02
7) Phenol-d6	6.293	99	746340	97.560	ng	0.00
23) Nitrobenzene-d5	7.222	82	711984	84.331	ng	0.00
42) 2,4,6-Tribromophenol	10.475	330	248510	110.975	ng	0.00
45) 2-Fluorobiphenyl	9.016	172	1415207	88.180	ng	0.00
79) Terphenyl-d14	12.763	244	1677145	93.764	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130401.D
Acq On : 26 Sep 2022 10:38
Operator : CG\JU
Sample : PB147858BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147858BL

Quant Time: Sep 27 01:03:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration




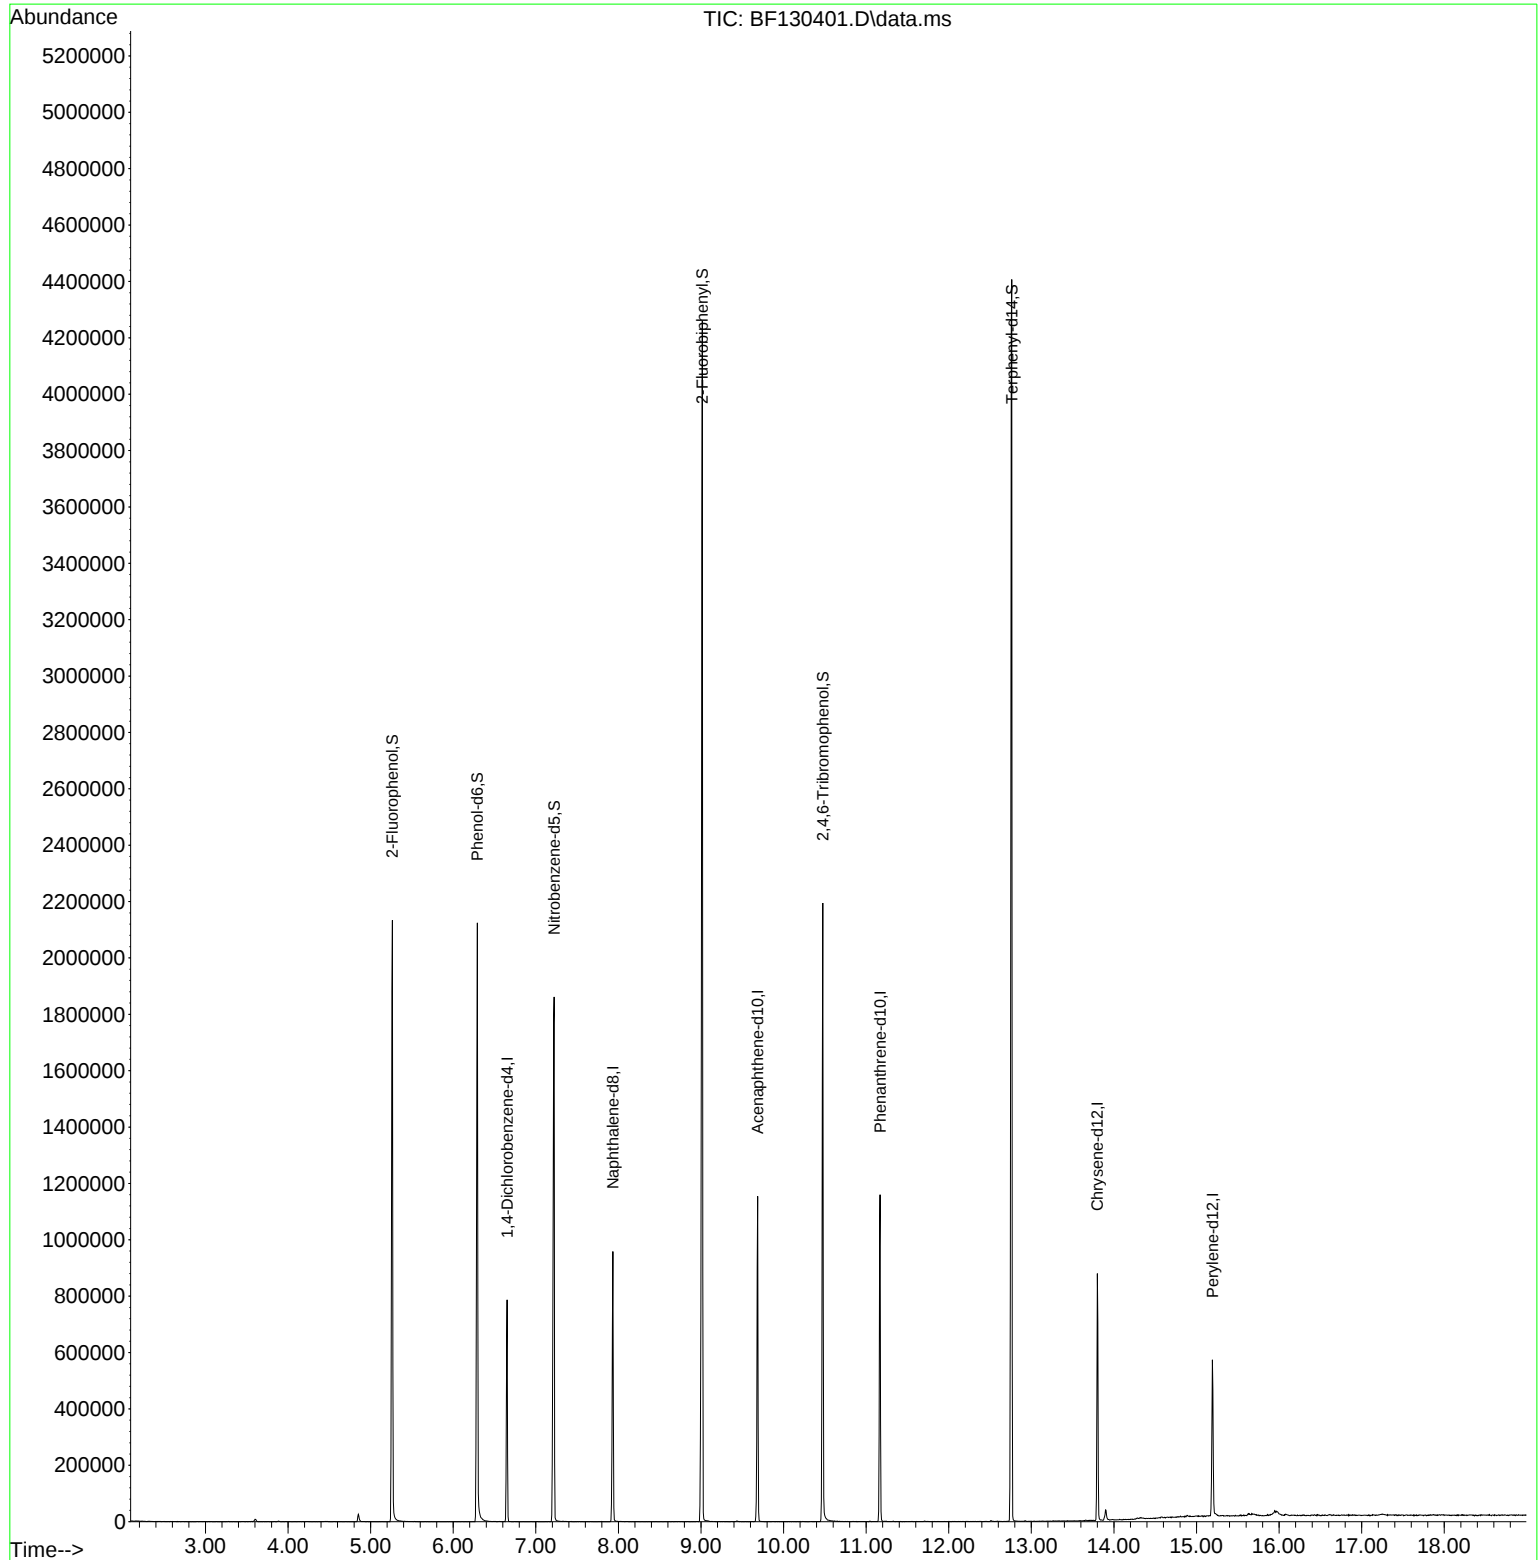




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.651 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38




Instrument :
BNA_F
ClientSampleId :
PB147858BL


Tgt Ion:152 Resp: 106046
Ion Ratio Lower Upper
152 100
150 157.7 122.8 184.2
115 62.8 53.8 80.8

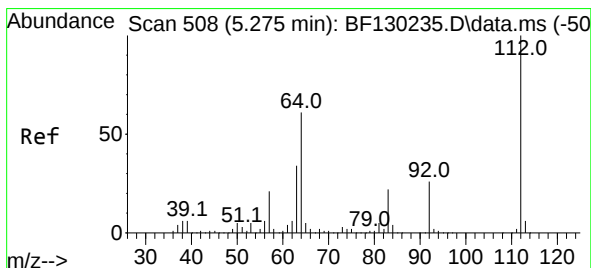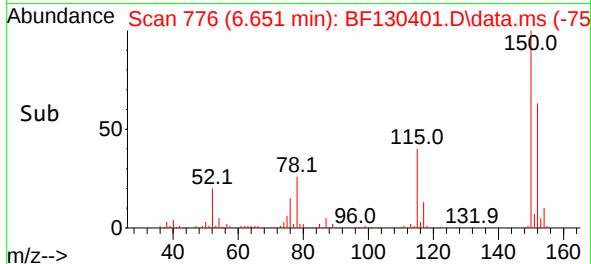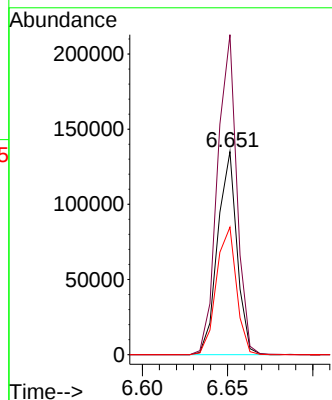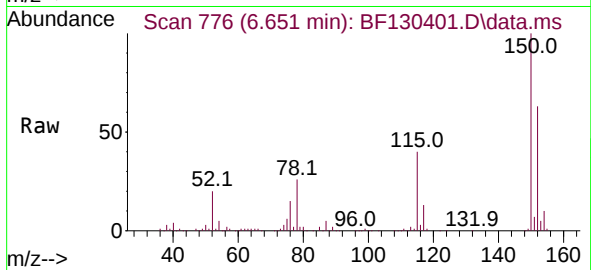

#5
2-Fluorophenol
Concen: 99.219 ng
RT: 5.263 min Scan# 540
Delta R.T. 0.018 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38

Tgt Ion:112 Resp: 606631
Ion Ratio Lower Upper
112 100
64 55.0 51.4 77.0
63 30.2 28.8 43.2


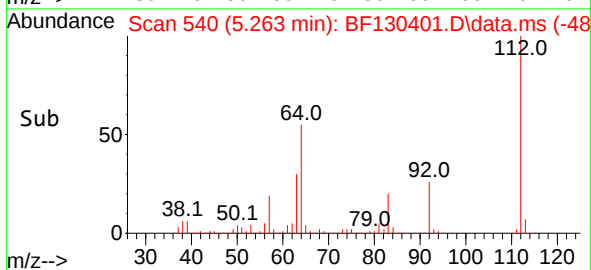
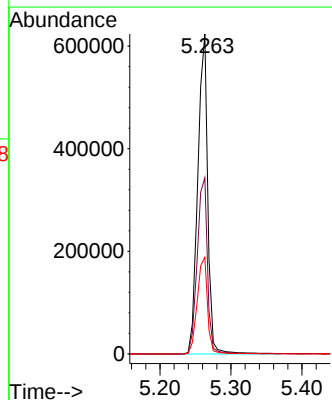
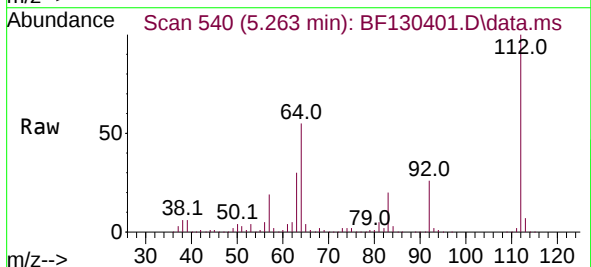


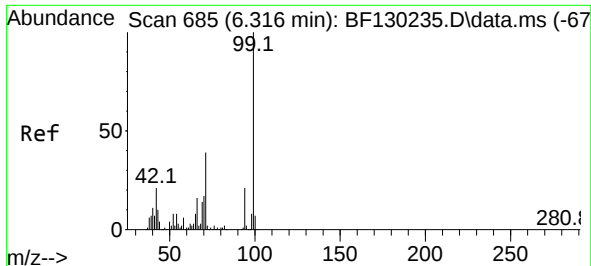

#7
Phenol-d6
Concen: 97.560 ng
RT: 6.293 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38




Instrument :
BNA_F
ClientSampleId :
PB147858BL

Tgt Ion: 99 Resp: 746340
Ion Ratio Lower Upper
99 100
42 18.3 17.0 25.6
71 38.0 32.3 48.5

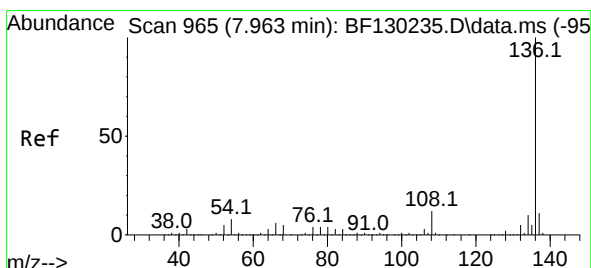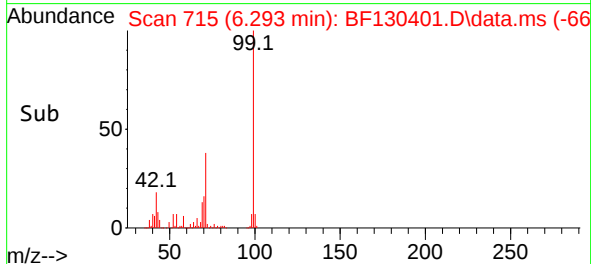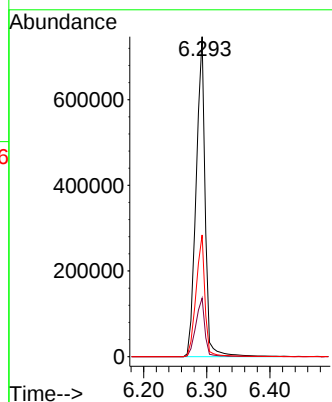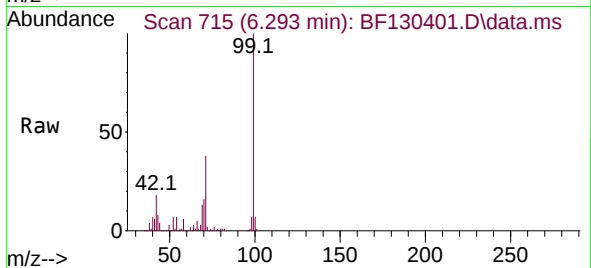

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.934 min Scan# 994
Delta R.T. -0.006 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38

Tgt Ion: 136 Resp: 431324
Ion Ratio Lower Upper
136 100
137 10.5 9.1 13.7
54 6.7 7.1 10.7#
68 4.6 4.5 6.7


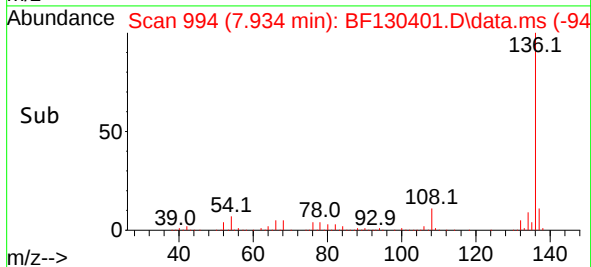
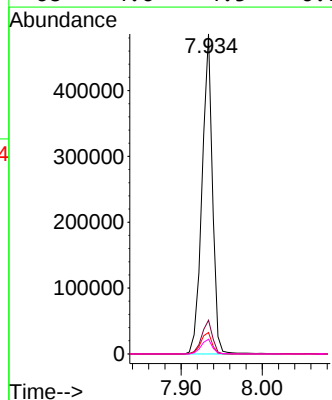
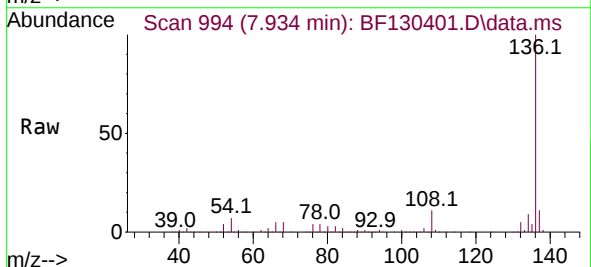




#23
Nitrobenzene-d5
Concen: 84.331 ng
RT: 7.222 min Scan# 81
Delta R.T. 0.000 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38




Instrument :
BNA_F
ClientSampleId :
PB147858BL


Tgt Ion: 82 Resp: 711984
Ion Ratio Lower Upper
82 100
128 46.5 32.6 49.0
54 48.3 43.8 65.6

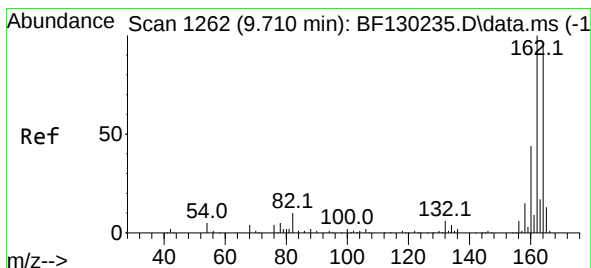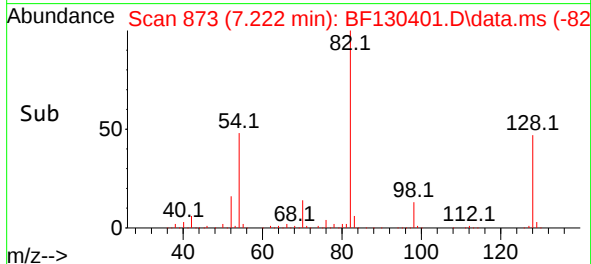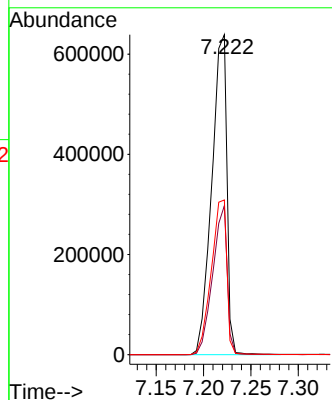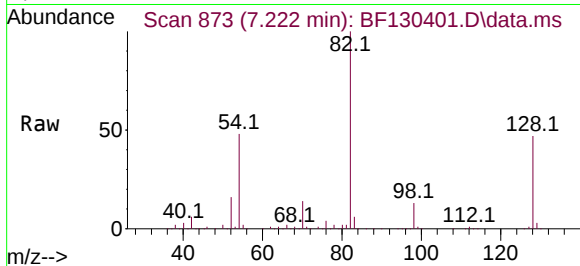

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.687 min Scan# 1292
Delta R.T. 0.000 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38


Tgt Ion:164 Resp: 233705
Ion Ratio Lower Upper
164 100
162 102.6 81.4 122.0
160 44.5 36.2 54.4

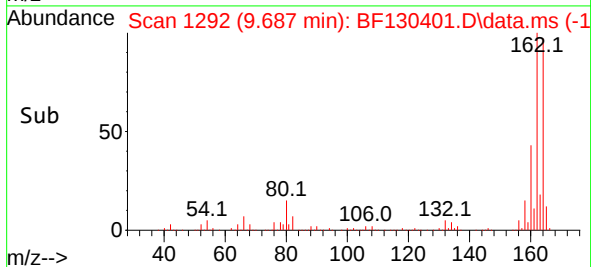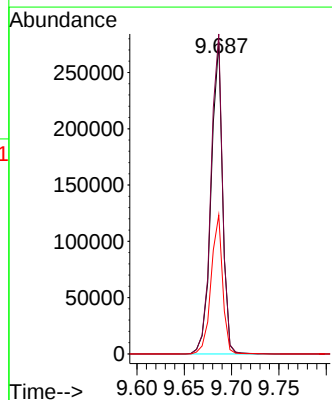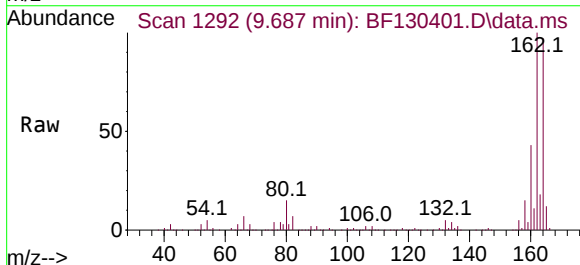



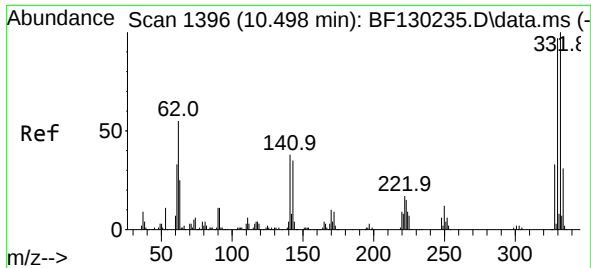


#42
2,4,6-Tribromophenol
Concen: 110.975 ng
RT: 10.475 min Scan# 14
Delta R.T. -0.006 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38

Instrument :
BNA_F
ClientSampleId :
PB147858BL



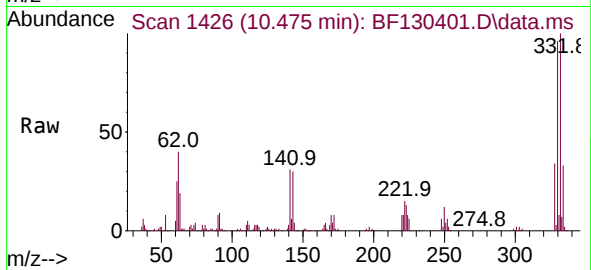



Tgt Ion:330 Resp: 248510
Ion Ratio Lower Upper
330 100
332 103.1 83.4 125.2
141 33.8 34.0 51.0#

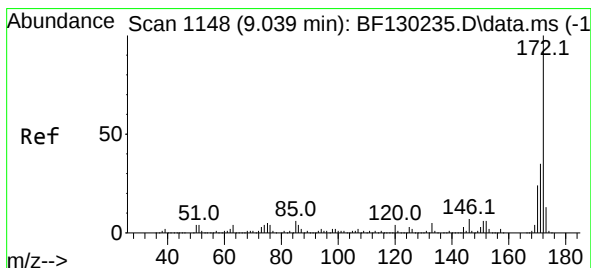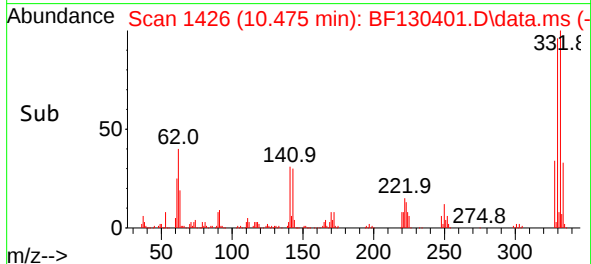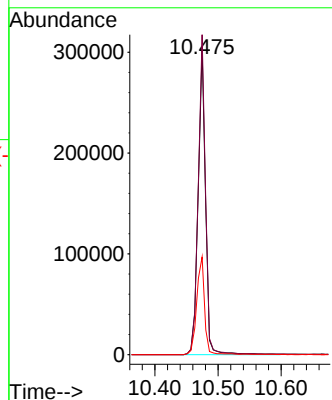

#45
2-Fluorobiphenyl
Concen: 88.180 ng
RT: 9.016 min Scan# 1178
Delta R.T. 0.000 min
Lab File: BF130401.D
Acq: 26 Sep 2022 10:38

Tgt Ion:172 Resp: 1415207
Ion Ratio Lower Upper
172 100
171 34.9 28.3 42.5
170 23.4 18.7 28.1

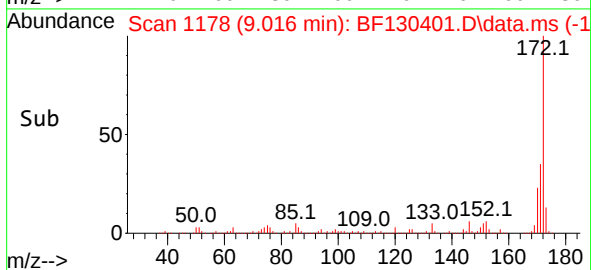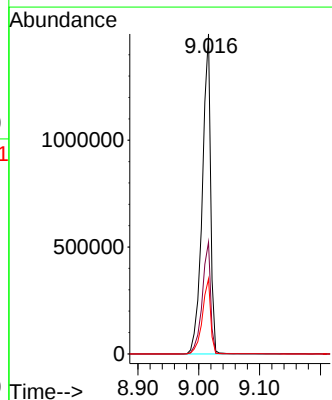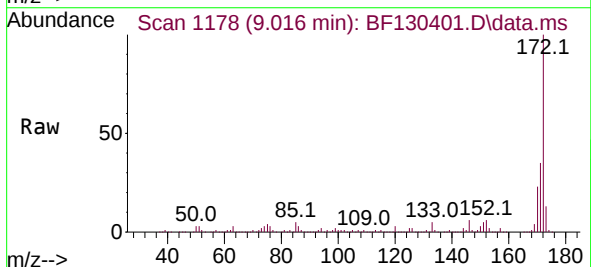

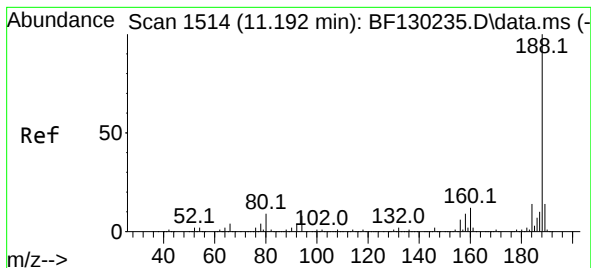

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.169 min Scan# 11

Delta R.T. 0.000 min

Lab File: BF130401.D

Acq: 26 Sep 2022 10:38

Instrument :

BNA_F

ClientSampleId :

PB147858BL





Tgt Ion:188 Resp: 419572

Ion Ratio Lower Upper

188 100

94 7.7 7.4 11.2

80 8.1 7.9 11.9

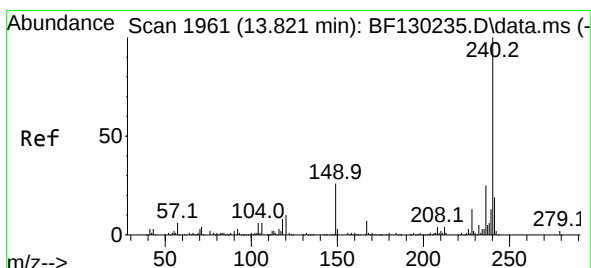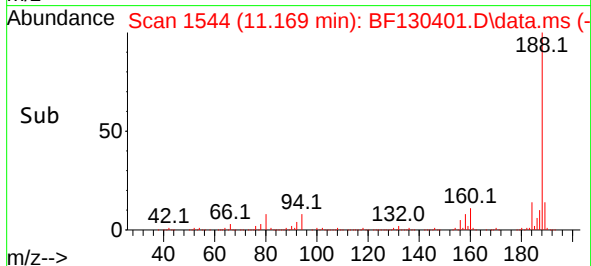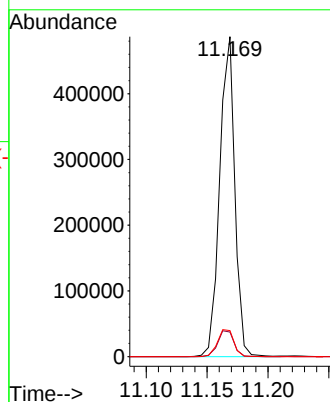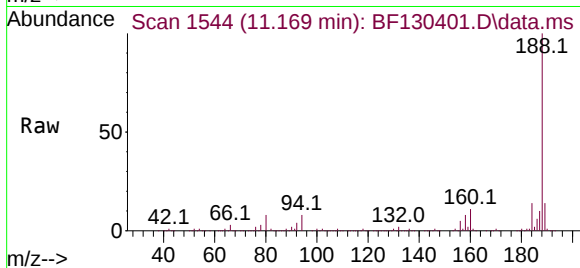

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.798 min Scan# 1991

Delta R.T. -0.006 min

Lab File: BF130401.D

Acq: 26 Sep 2022 10:38




Tgt Ion:240 Resp: 296294


Ion Ratio Lower Upper

240 100

120 10.9 8.7 13.1

236 25.2 20.9 31.3


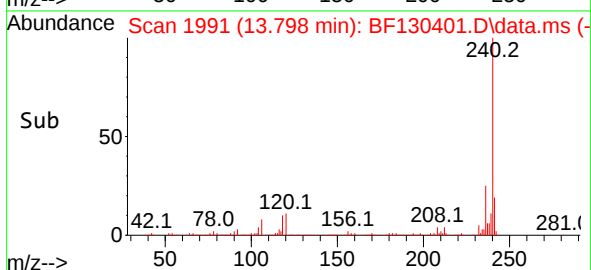
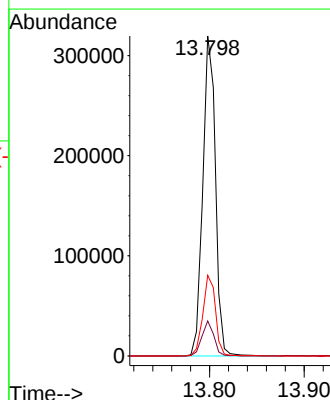
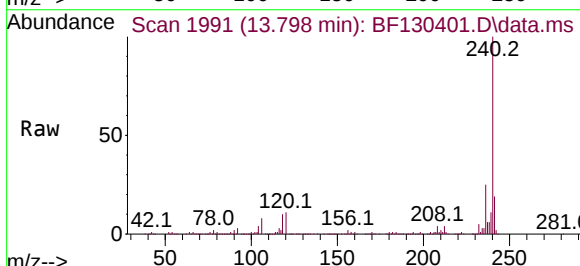


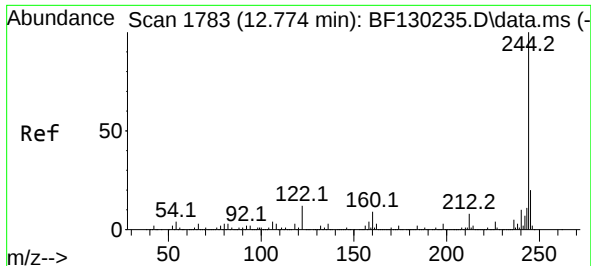

#79
 Terphenyl-d14
 Concen: 93.764 ng
 RT: 12.763 min Scan# 1815
 Delta R.T. 0.006 min
 Lab File: BF130401.D
 Acq: 26 Sep 2022 10:38

Instrument :
 BNA_F
 ClientSampleId :
 PB147858BL

Tgt Ion:244 Resp: 1677145
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.9 8.9
 122 9.4 8.5 12.7

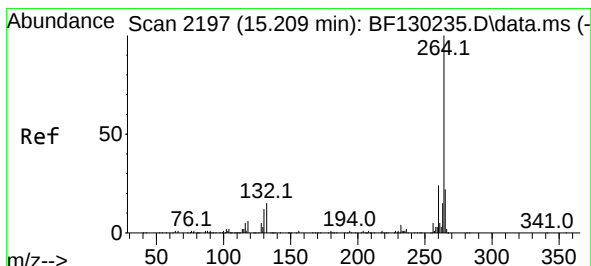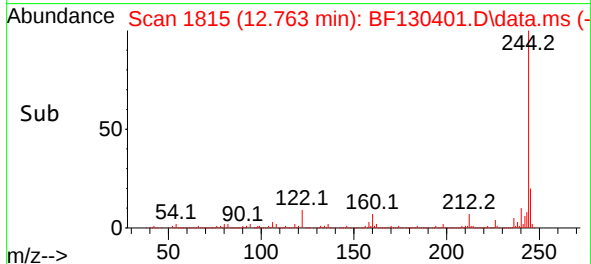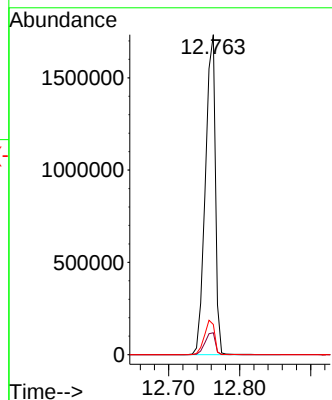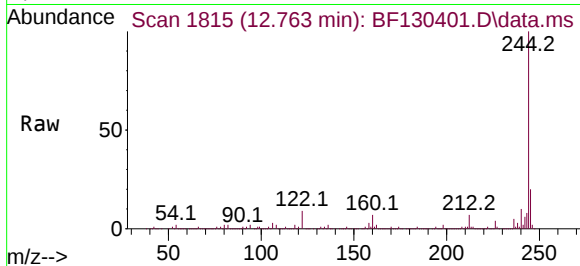

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.192 min Scan# 2228
 Delta R.T. 0.000 min
 Lab File: BF130401.D
 Acq: 26 Sep 2022 10:38

Tgt Ion:264 Resp: 225847
 Ion Ratio Lower Upper
 264 100
 260 23.1 19.3 28.9
 265 21.1 17.0 25.4

