

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
 Data File : BF130403.D
 Acq On : 26 Sep 2022 11:48
 Operator : CG\JU
 Sample : N4609-04RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSN002RE

Quant Time: Sep 27 01:03:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 27 01:00:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.651	152	88863	20.000	ng	0.00
21) Naphthalene-d8	7.934	136	329617	20.000	ng	# 0.00
39) Acenaphthene-d10	9.686	164	160973	20.000	ng	0.00
64) Phenanthrene-d10	11.169	188	231135	20.000	ng	# 0.00
76) Chrysene-d12	13.798	240	185232	20.000	ng	0.00
86) Perylene-d12	15.198	264	220456	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.251	112	335245	65.434	ng	0.00
7) Phenol-d6	6.293	99	254107	39.639	ng	0.00
23) Nitrobenzene-d5	7.222	82	537476	83.305	ng	0.00
42) 2,4,6-Tribromophenol	10.475	330	199269	129.192	ng	0.00
45) 2-Fluorobiphenyl	9.016	172	967458	87.518	ng	0.00
79) Terphenyl-d14	12.757	244	749377	67.015	ng	0.00


Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130403.D
Acq On : 26 Sep 2022 11:48
Operator : CG\JU
Sample : N4609-04RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN002RE

Quant Time: Sep 27 01:03:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration




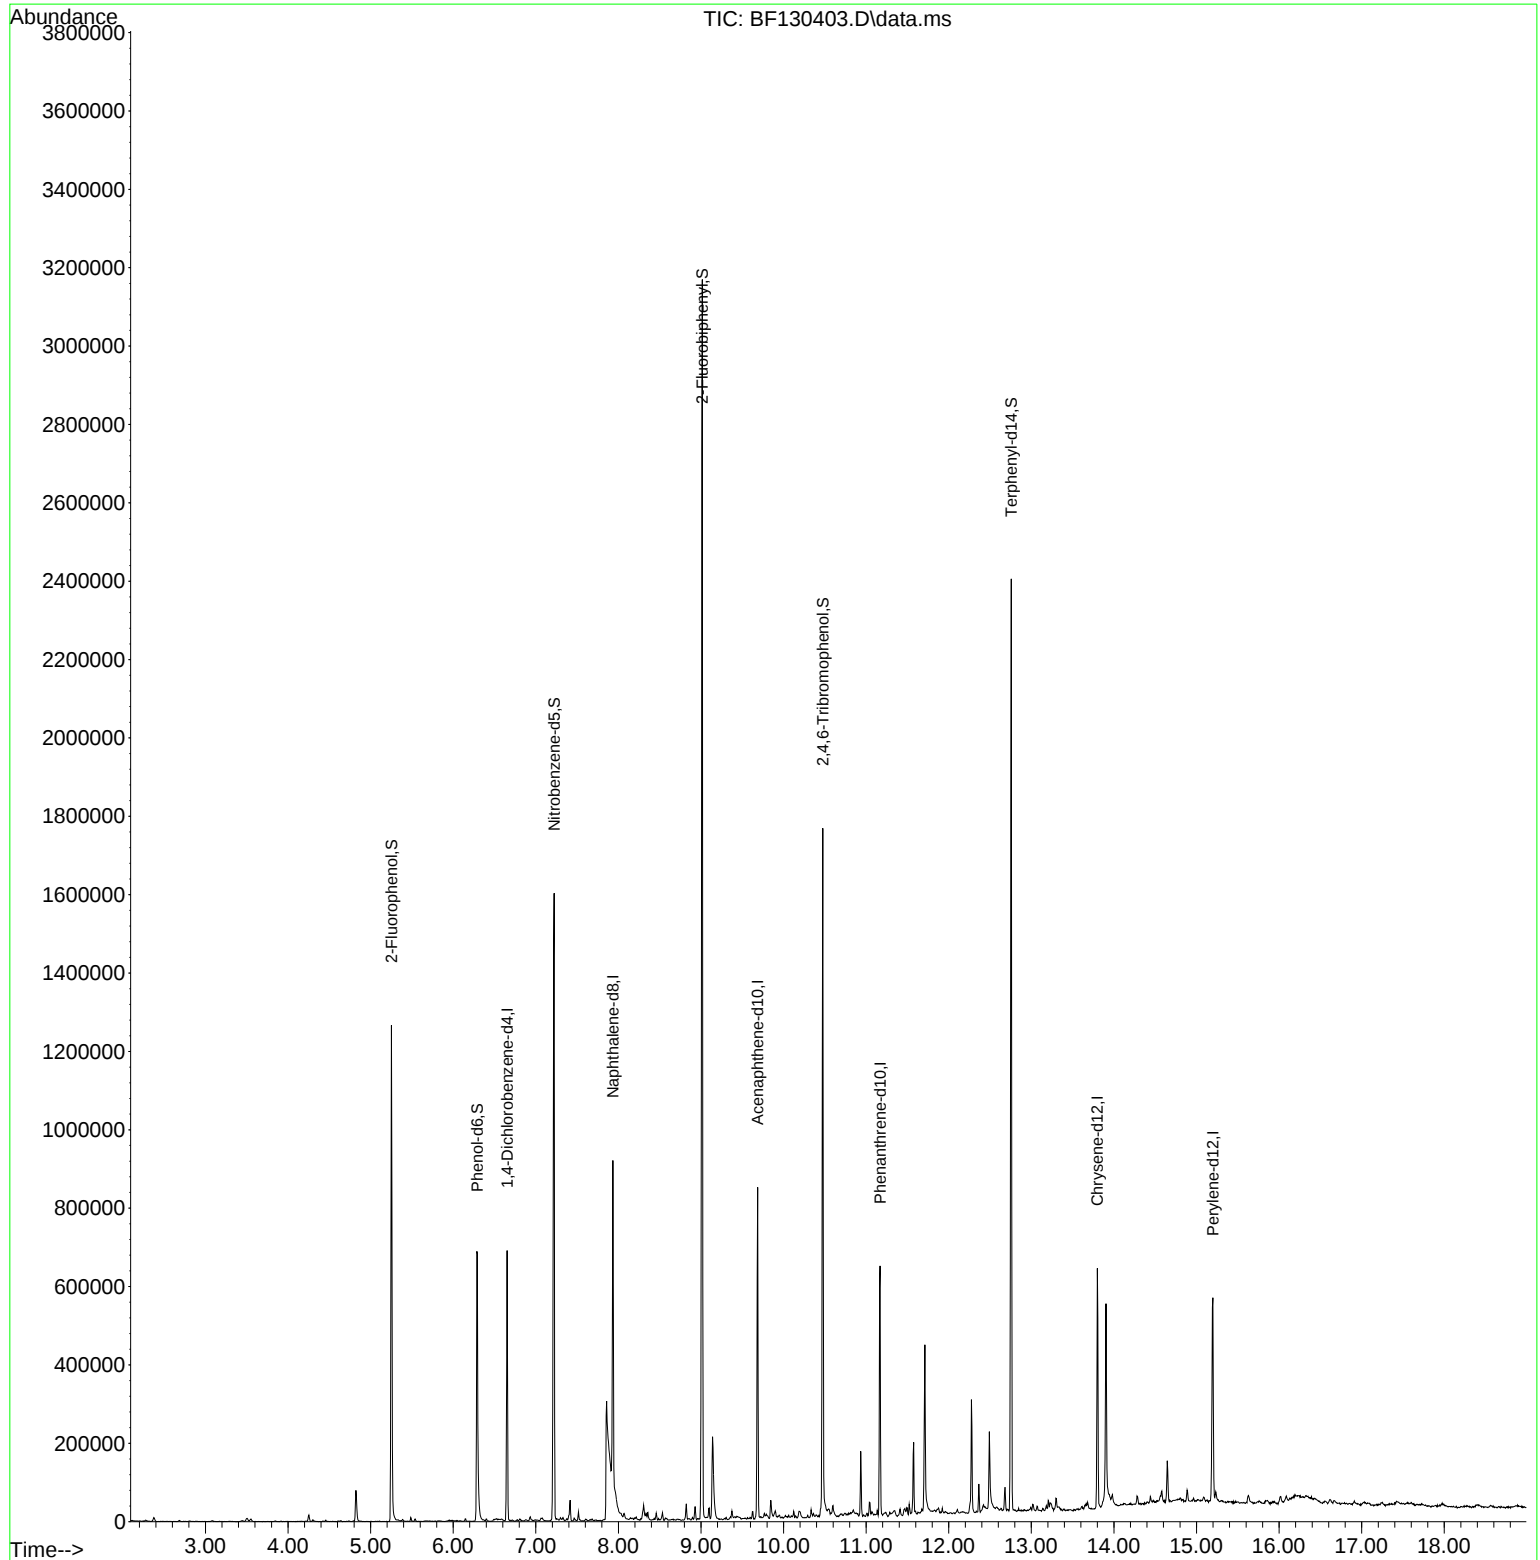




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.651 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF130403.D
Acq: 26 Sep 2022 11:48




Instrument :
BNA_F
ClientSampleId :
DSN002RE


Tgt Ion:152 Resp: 88863
Ion Ratio Lower Upper
152 100
150 157.3 122.8 184.2
115 66.1 53.8 80.8

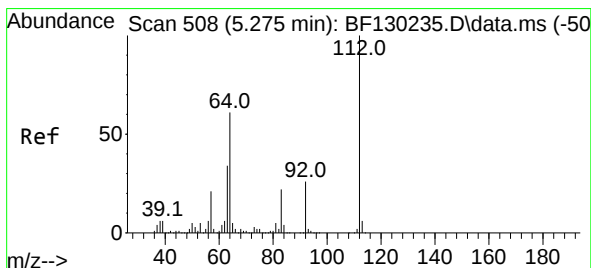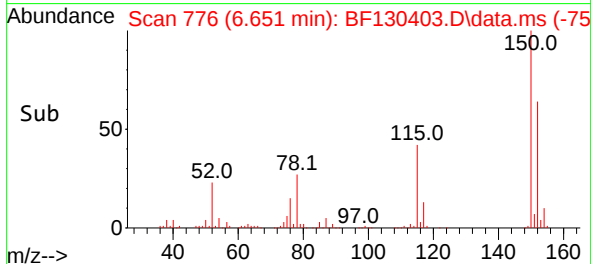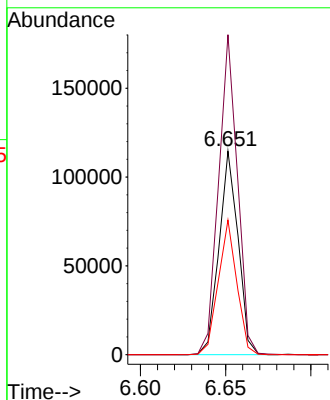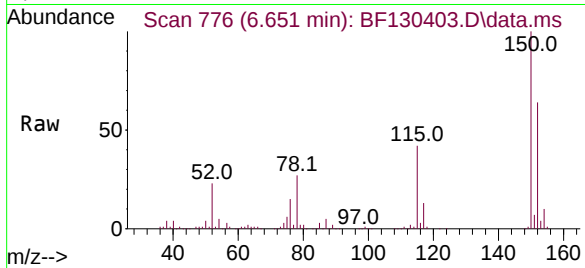

#5
2-Fluorophenol
Concen: 65.434 ng
RT: 5.251 min Scan# 538
Delta R.T. 0.006 min
Lab File: BF130403.D
Acq: 26 Sep 2022 11:48

Tgt Ion:112 Resp: 335245
Ion Ratio Lower Upper
112 100
64 59.0 51.4 77.0
63 32.5 28.8 43.2


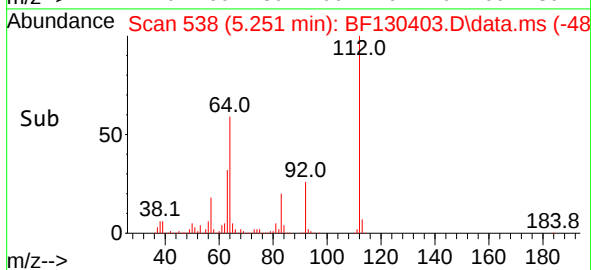
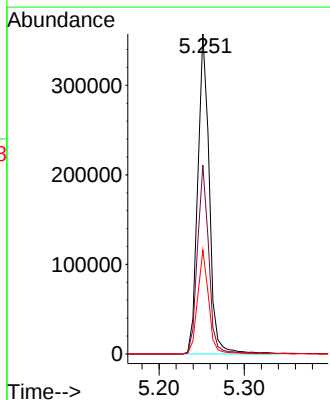
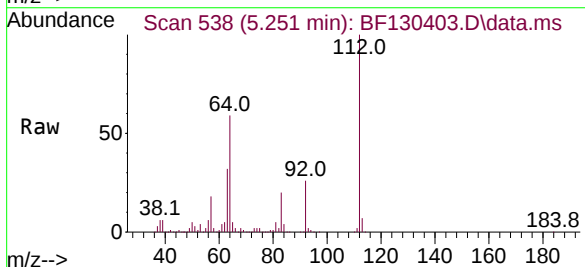


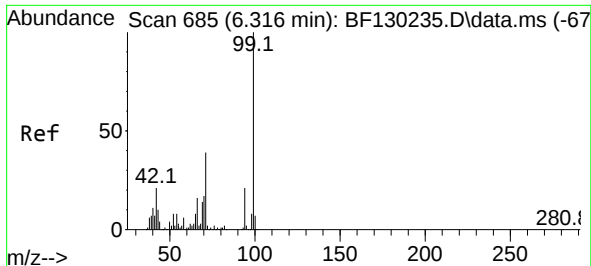

#7
Phenol-d6
Concen: 39.639 ng
RT: 6.293 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF130403.D
Acq: 26 Sep 2022 11:48




Instrument :
BNA_F
ClientSampleId :
DSN002RE


Tgt Ion: 99 Resp: 254107
Ion Ratio Lower Upper
99 100
42 17.4 17.0 25.6
71 35.8 32.3 48.5

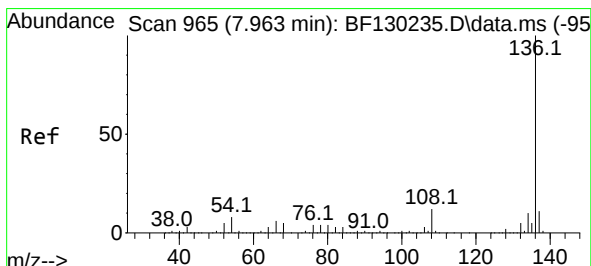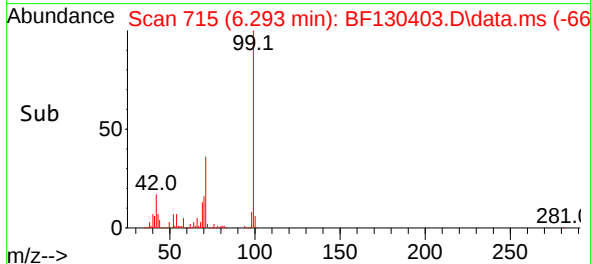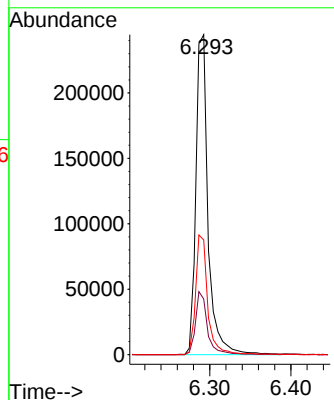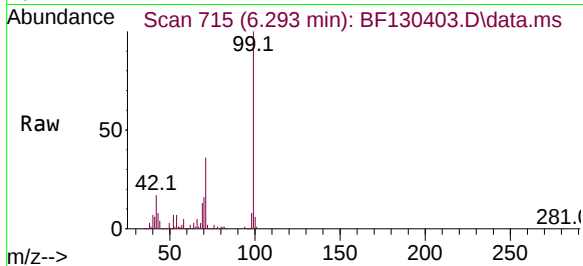

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.934 min Scan# 994
Delta R.T. -0.006 min
Lab File: BF130403.D
Acq: 26 Sep 2022 11:48

Tgt Ion: 136 Resp: 329617
Ion Ratio Lower Upper
136 100
137 10.6 9.1 13.7
54 7.0 7.1 10.7#
68 4.8 4.5 6.7

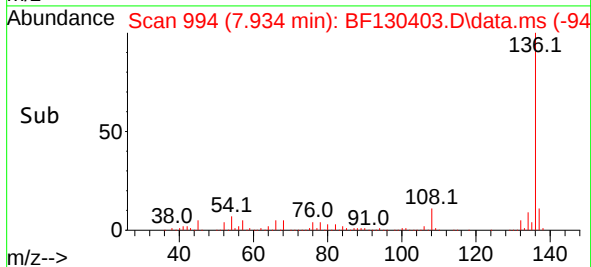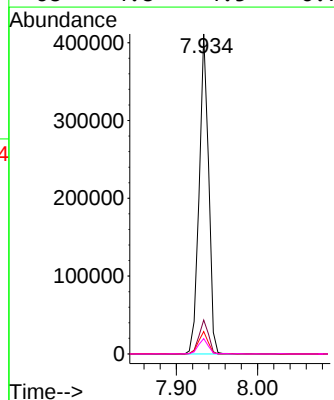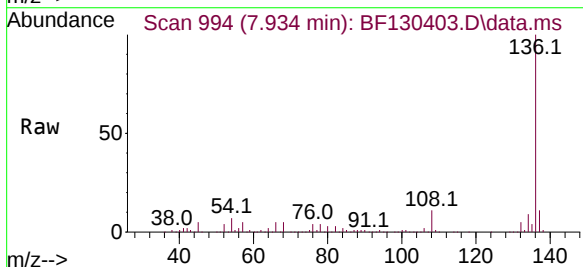

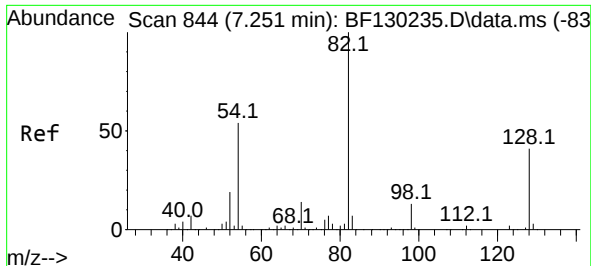

#23

Nitrobenzene-d5

Concen: 83.305 ng

RT: 7.222 min Scan# 81

Delta R.T. -0.000 min

Lab File: BF130403.D

Acq: 26 Sep 2022 11:48

Instrument :

BNA_F

ClientSampleId :

DSN002RE





Tgt Ion: 82 Resp: 537476

Ion Ratio Lower Upper

82 100

128 46.9 32.6 49.0

54 49.1 43.8 65.6

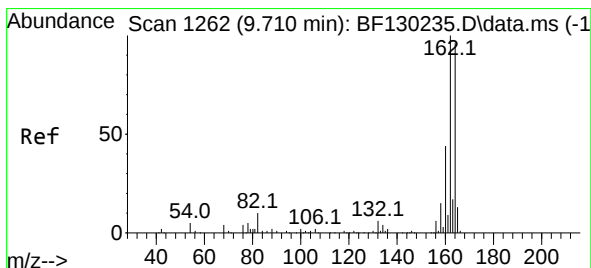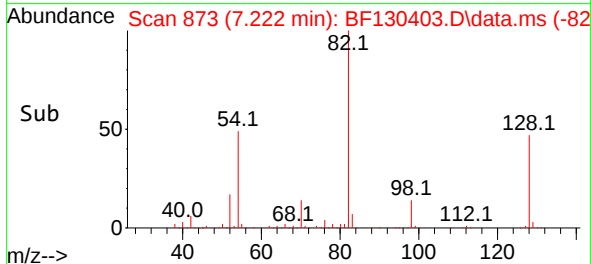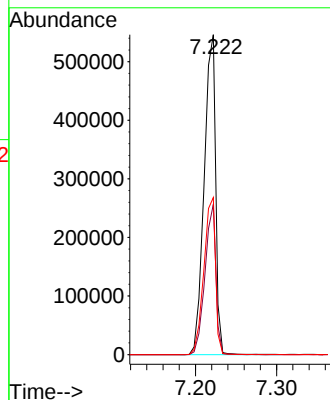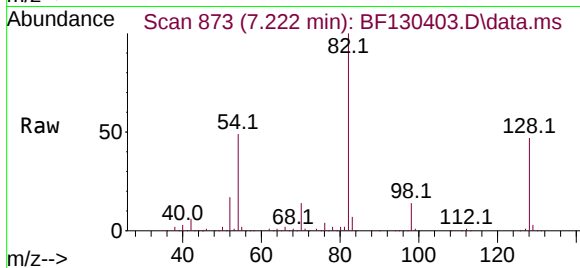

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.686 min Scan# 1292

Delta R.T. -0.000 min

Lab File: BF130403.D

Acq: 26 Sep 2022 11:48




Tgt Ion:164 Resp: 160973

Ion Ratio Lower Upper

164 100

162 101.3 81.4 122.0

160 43.6 36.2 54.4

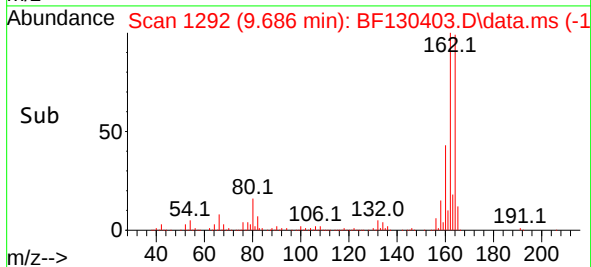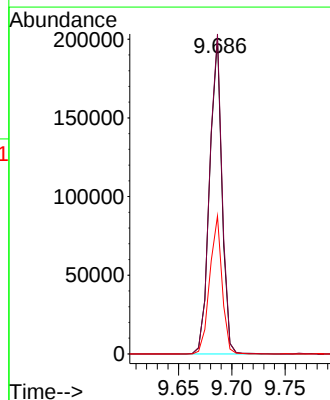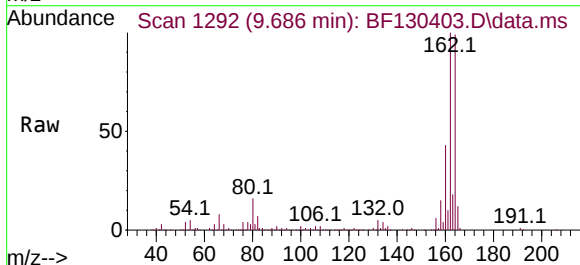



#42

2,4,6-Tribromophenol

Concen: 129.192 ng

RT: 10.475 min Scan# 1426

Delta R.T. -0.006 min

Lab File: BF130403.D

Acq: 26 Sep 2022 11:48

Instrument :

BNA_F

ClientSampleId :

DSN002RE





Tgt Ion:330 Resp: 199269

Ion Ratio Lower Upper

330 100

332 105.6 83.4 125.2

141 35.5 34.0 51.0

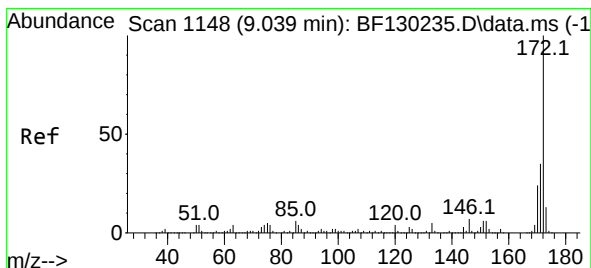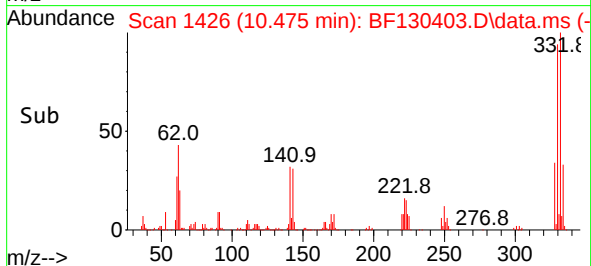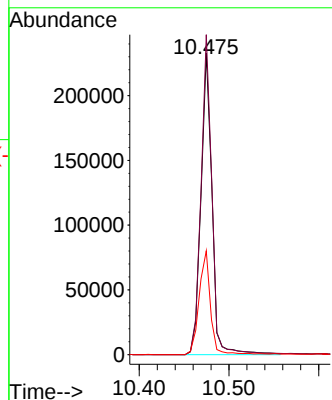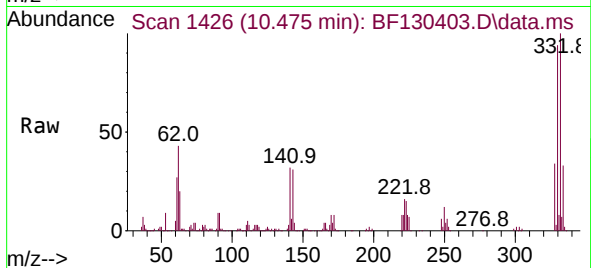

#45

2-Fluorobiphenyl

Concen: 87.518 ng

RT: 9.016 min Scan# 1178

Delta R.T. -0.000 min

Lab File: BF130403.D

Acq: 26 Sep 2022 11:48




Tgt Ion:172 Resp: 967458


Ion Ratio Lower Upper

172 100

171 35.4 28.3 42.5

170 23.3 18.7 28.1


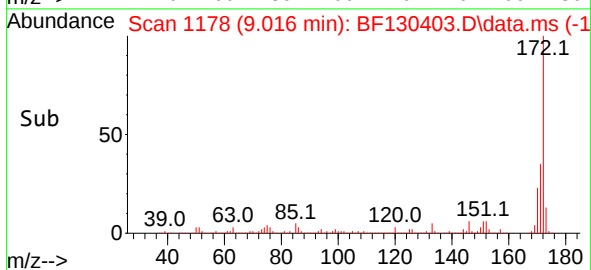
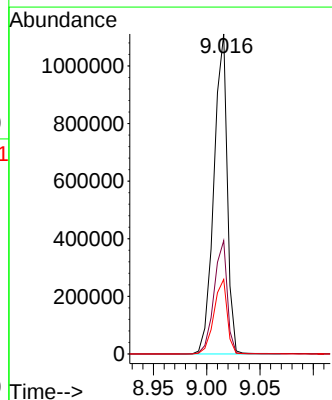
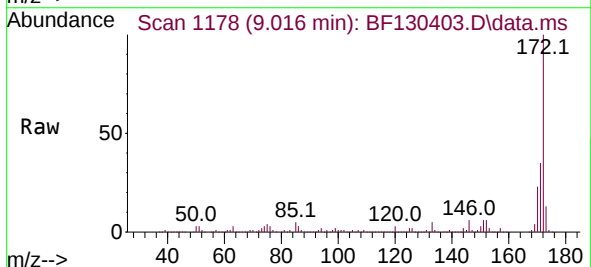


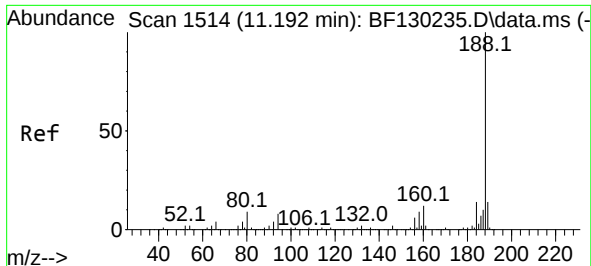

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.169 min Scan# 111
Delta R.T. -0.000 min
Lab File: BF130403.D
Acq: 26 Sep 2022 11:48




Instrument :
BNA_F
ClientSampleId :
DSN002RE


Tgt Ion:188 Resp: 231135
Ion Ratio Lower Upper
188 100
94 8.1 7.4 11.2
80 7.7 7.9 11.9#

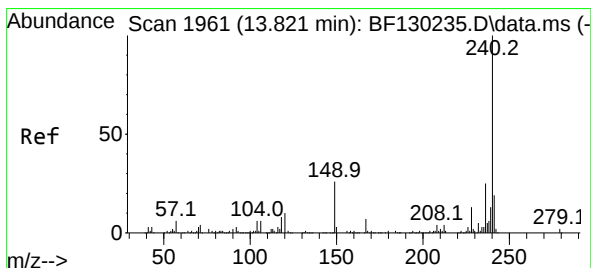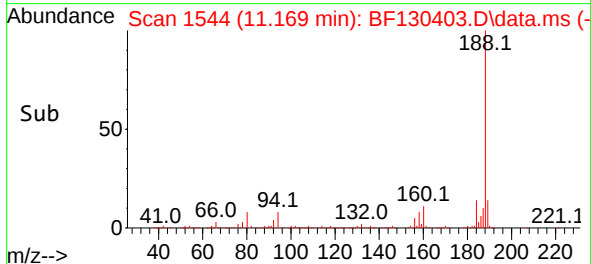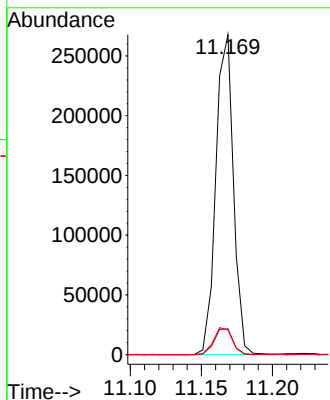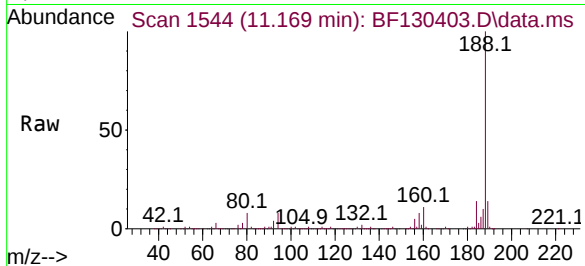

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.798 min Scan# 1991
Delta R.T. -0.006 min
Lab File: BF130403.D
Acq: 26 Sep 2022 11:48

Tgt Ion:240 Resp: 185232
Ion Ratio Lower Upper
240 100
120 11.0 8.7 13.1
236 25.5 20.9 31.3


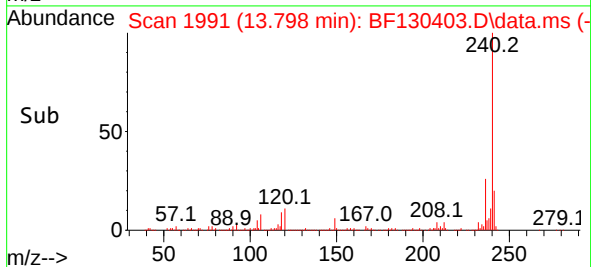
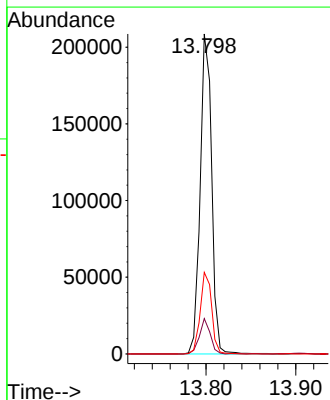
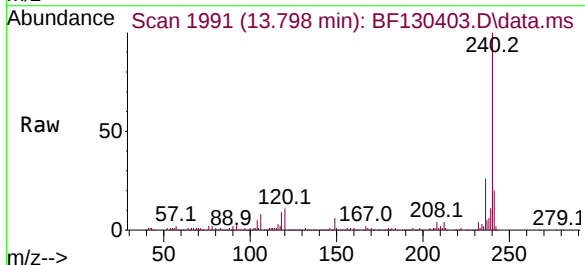


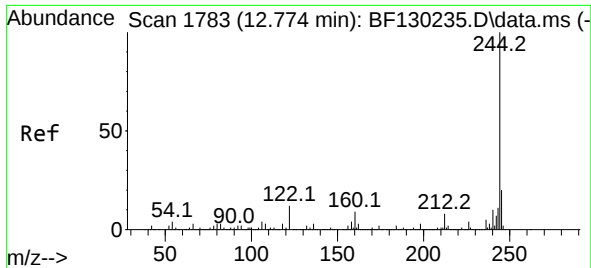

#79
 Terphenyl-d14
 Concen: 67.015 ng
 RT: 12.757 min Scan# 1814
 Delta R.T. -0.000 min
 Lab File: BF130403.D
 Acq: 26 Sep 2022 11:48

Instrument :
 BNA_F
 ClientSampleId :
 DSN002RE

Tgt Ion:244 Resp: 749377
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.9 8.9
 122 10.3 8.5 12.7

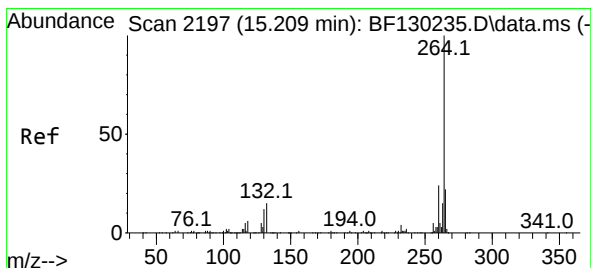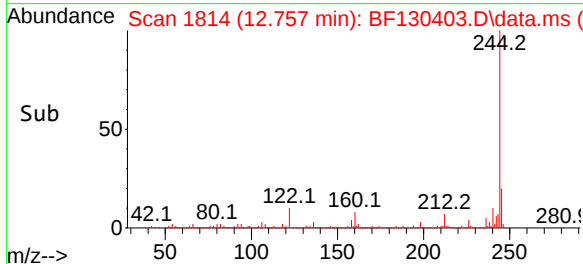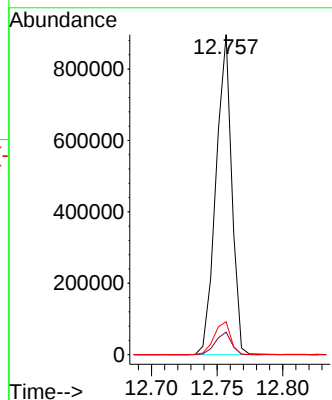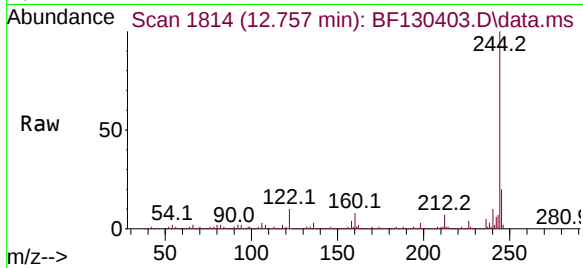

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.198 min Scan# 2229
 Delta R.T. 0.006 min
 Lab File: BF130403.D
 Acq: 26 Sep 2022 11:48

Tgt Ion:264 Resp: 220456
 Ion Ratio Lower Upper
 264 100
 260 23.1 19.3 28.9
 265 21.6 17.0 25.4

