

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
 Data File : BF130401.D
 Acq On : 26 Sep 2022 10:38
 Operator : CG\JU
 Sample : PB147858BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147858BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	535	540	543	rBV	2133875	2075803	46.63%	9.634%
2	6.293	710	715	718	rBV	2124581	2061152	46.30%	9.566%
3	6.651	772	776	779	rBV	787014	637120	14.31%	2.957%
4	7.222	867	873	875	rBV	1860862	2057303	46.22%	9.548%
5	7.934	989	994	997	rBV	958372	859039	19.30%	3.987%
6	9.016	1171	1178	1181	rBV	4260597	4102813	92.17%	19.041%
7	9.687	1286	1292	1295	rBV	1154199	994684	22.35%	4.616%
8	10.475	1421	1426	1429	rBV	2194180	1833346	41.19%	8.508%
9	11.169	1540	1544	1547	rBV	1156037	1006808	22.62%	4.673%
10	12.763	1809	1815	1818	rBV	4406261	4451409	100.00%	20.659%
11	13.798	1987	1991	1995	rBV	876127	804848	18.08%	3.735%
12	13.898	2003	2008	2013	rBV	36957	53357	1.20%	0.248%
13	15.192	2223	2228	2233	rBV	554409	609719	13.70%	2.830%




Sum of corrected areas: 21547401

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130401.D
Acq On : 26 Sep 2022 10:38
Operator : CG\JU
Sample : PB147858BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147858BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

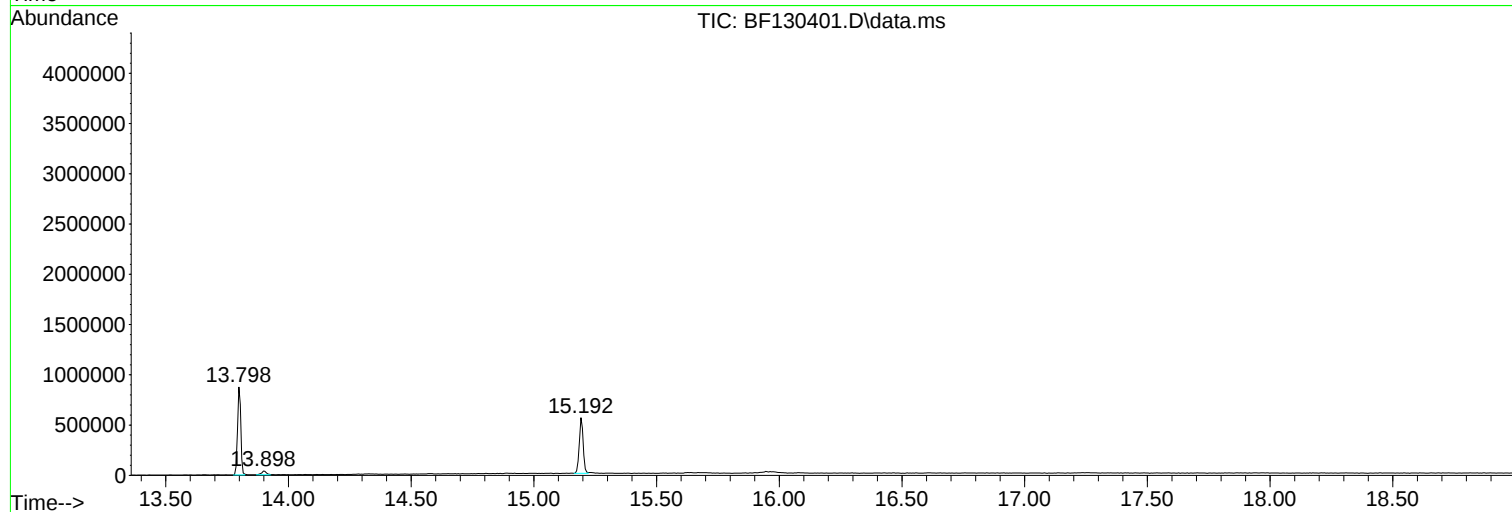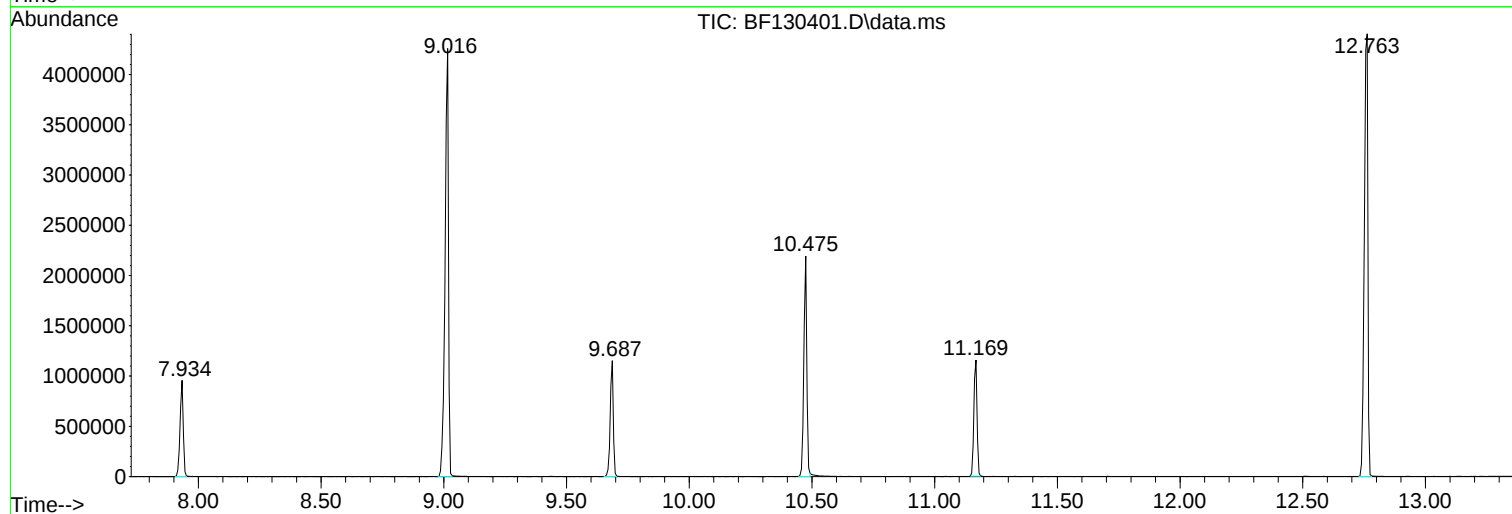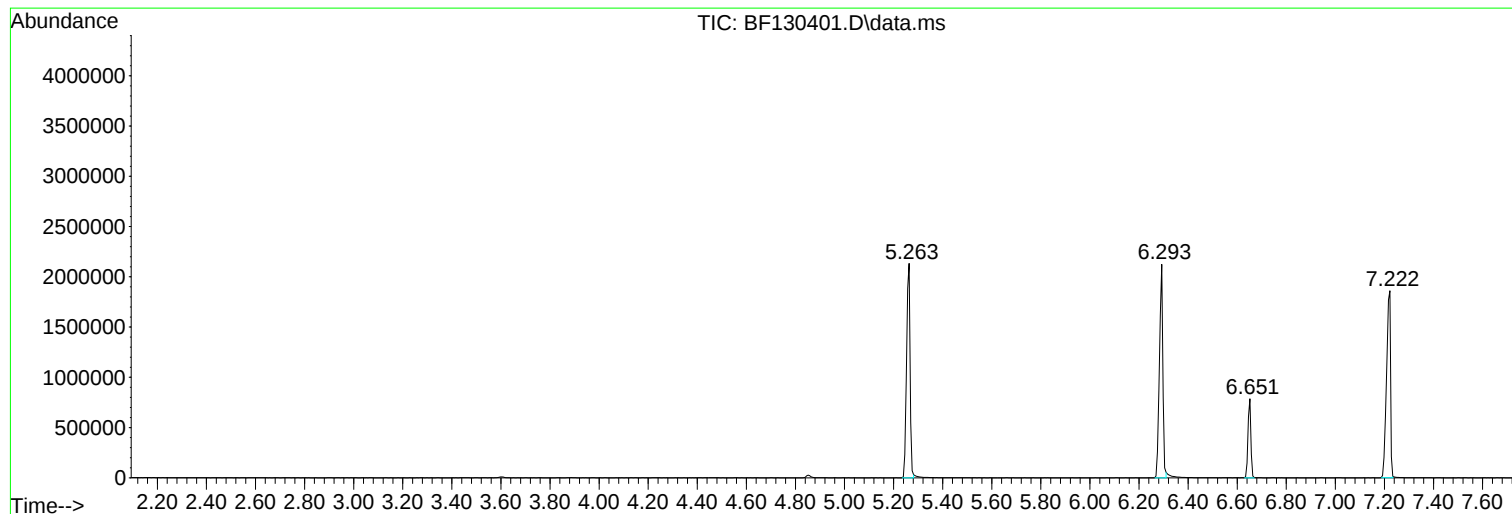

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130401.D
Acq On : 26 Sep 2022 10:38
Operator : CG\JU
Sample : PB147858BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147858BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130401.D
Acq On : 26 Sep 2022 10:38
Operator : CG\JU
Sample : PB147858BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147858BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------