

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
 Data File : BF130405.D
 Acq On : 26 Sep 2022 13:15
 Operator : CG\JU
 Sample : PB147850BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147850BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.869	467	473	483	rVB	33604	50428	1.32%	0.215%
2	5.263	535	540	543	rBV	2690518	2853388	74.94%	12.171%
3	6.293	710	715	718	rBV	2473184	2851759	74.90%	12.164%
4	6.651	772	776	779	rBV	845572	707710	18.59%	3.019%
5	7.216	866	872	875	rBV	1713385	1904639	50.03%	8.124%
6	7.934	989	994	997	rBV	1028435	947549	24.89%	4.042%
7	9.016	1171	1178	1181	rBV	3920281	3746931	98.41%	15.982%
8	9.687	1286	1292	1295	rBV	1294672	1101611	28.93%	4.699%
9	10.475	1420	1426	1429	rBV	2659524	2422203	63.62%	10.332%
10	11.169	1540	1544	1547	rBV	1355809	1087042	28.55%	4.637%
11	11.328	1568	1571	1575	rBV	54178	42082	1.11%	0.179%
12	11.704	1628	1635	1640	rBV2	29402	47846	1.26%	0.204%
13	12.757	1809	1814	1817	rBV	3873658	3807326	100.00%	16.240%
14	13.798	1987	1991	1995	rBV	870416	809118	21.25%	3.451%
15	13.904	2002	2009	2018	rBV	357463	460396	12.09%	1.964%
16	15.192	2223	2228	2233	rBV	522080	604639	15.88%	2.579%




Sum of corrected areas: 23444667

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130405.D
Acq On : 26 Sep 2022 13:15
Operator : CG\JU
Sample : PB147850BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

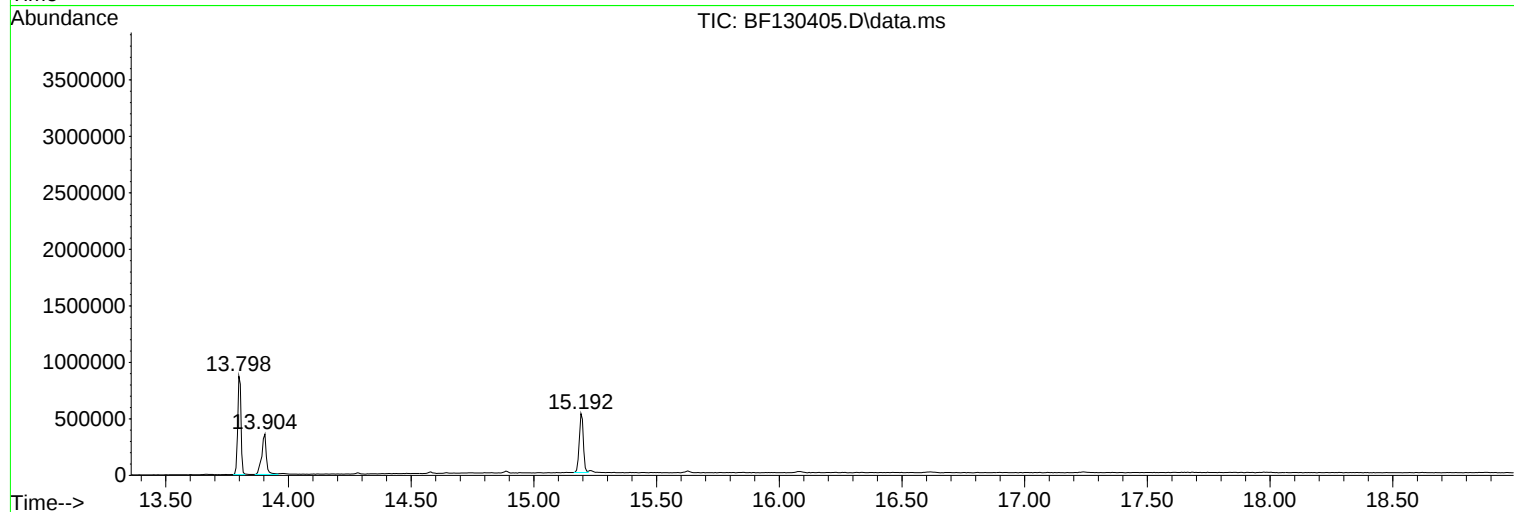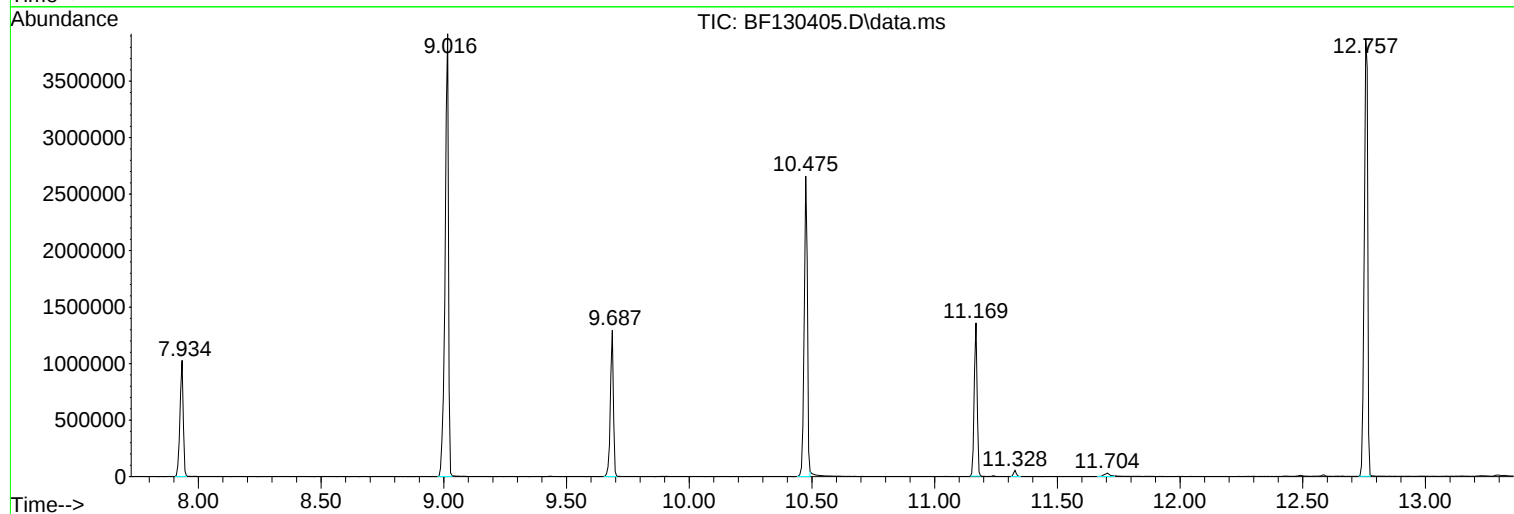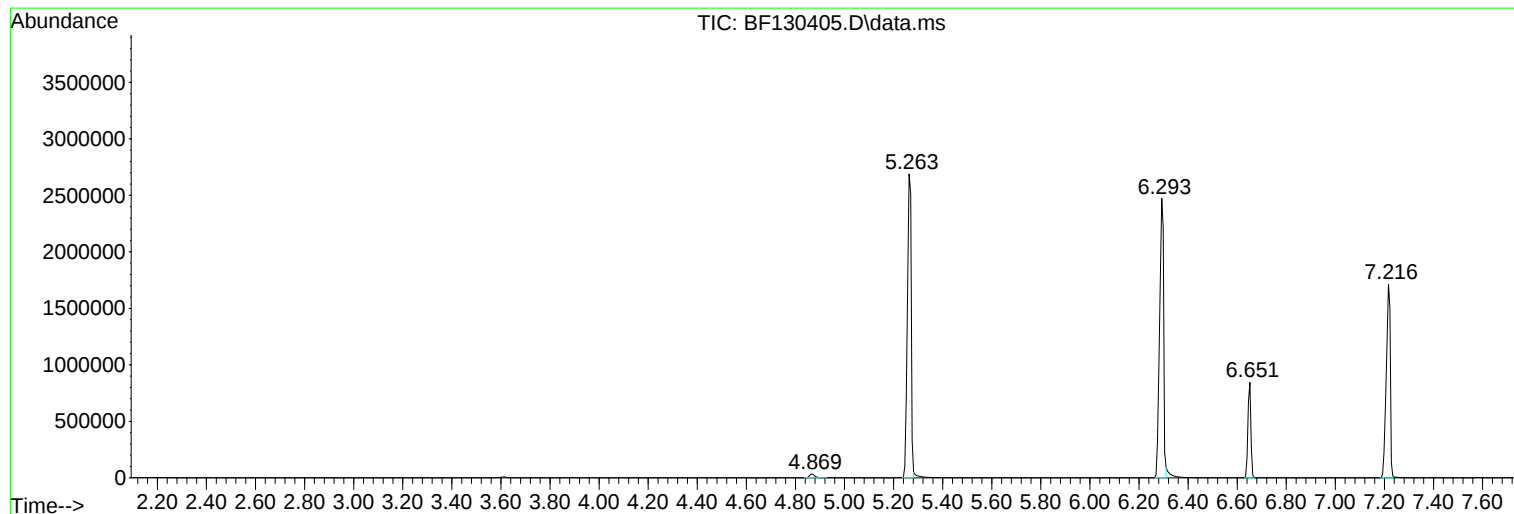

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130405.D
Acq On : 26 Sep 2022 13:15
Operator : CG\JU
Sample : PB147850BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147850BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.904	11.38 ng	460396	Chrysene-d12	13.798

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	45
4			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28
5			Yohimban, 16,17-didehydro-	278	C19H22N2	006874-77-7	10

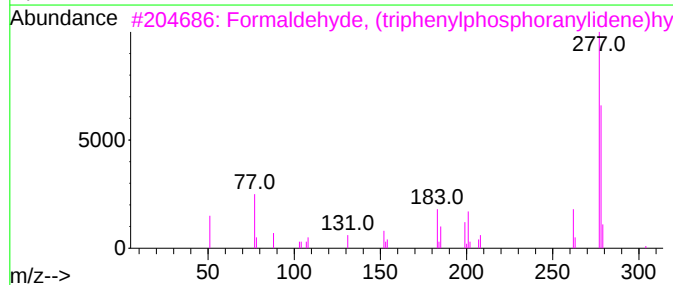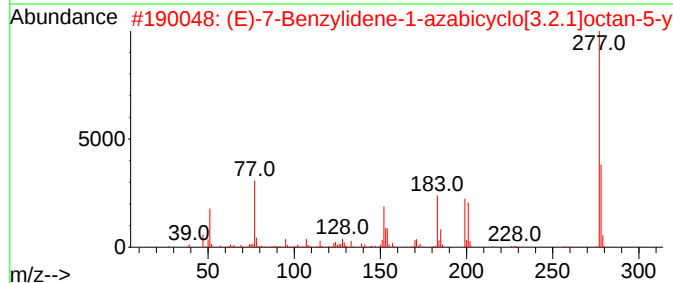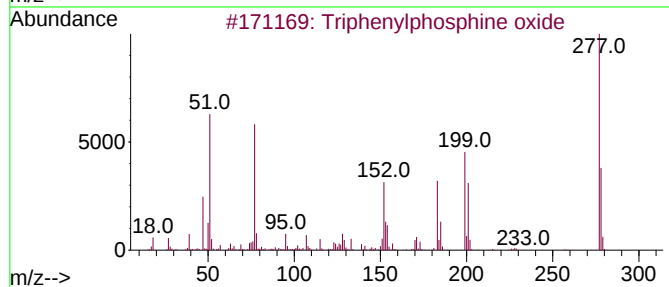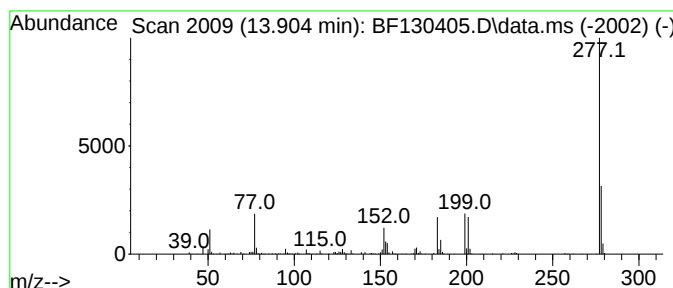

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130405.D
Acq On : 26 Sep 2022 13:15
Operator : CG\JU
Sample : PB147850BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147850BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.904	11.4	ng	460396	5	13.798	809118	20.0