

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
 Data File : BF130414.D
 Acq On : 26 Sep 2022 18:32
 Operator : CG\JU
 Sample : N4742-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP-14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.828	463	466	477	rVB	44763	51599	1.55%	0.353%
2	5.251	534	538	550	rBV	1050163	957391	28.75%	6.552%
3	6.287	710	714	726	rBV	667540	611766	18.37%	4.187%
4	6.651	772	776	779	rBV	733071	570826	17.14%	3.906%
5	7.216	867	872	875	rBV	1728098	1823349	54.76%	12.478%
6	7.934	990	994	997	rBV	874937	724491	21.76%	4.958%
7	9.010	1172	1177	1181	rBV	3356628	3329558	100.00%	22.785%
8	9.681	1287	1291	1295	rBV	797615	749476	22.51%	5.129%
9	10.469	1421	1425	1443	rBV	1361831	1240700	37.26%	8.491%
10	11.163	1539	1543	1547	rBV	727508	612763	18.40%	4.193%
11	11.704	1631	1635	1638	rBV	40773	40674	1.22%	0.278%
12	12.757	1809	1814	1817	rBV	2827789	2504502	75.22%	17.139%
13	13.798	1987	1991	1999	rBV	589641	508327	15.27%	3.479%
14	13.898	2003	2008	2014	rBV	294654	296286	8.90%	2.028%
15	15.192	2222	2228	2233	rBV	507947	590951	17.75%	4.044%




Sum of corrected areas: 14612659

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130414.D
Acq On : 26 Sep 2022 18:32
Operator : CG\JU
Sample : N4742-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

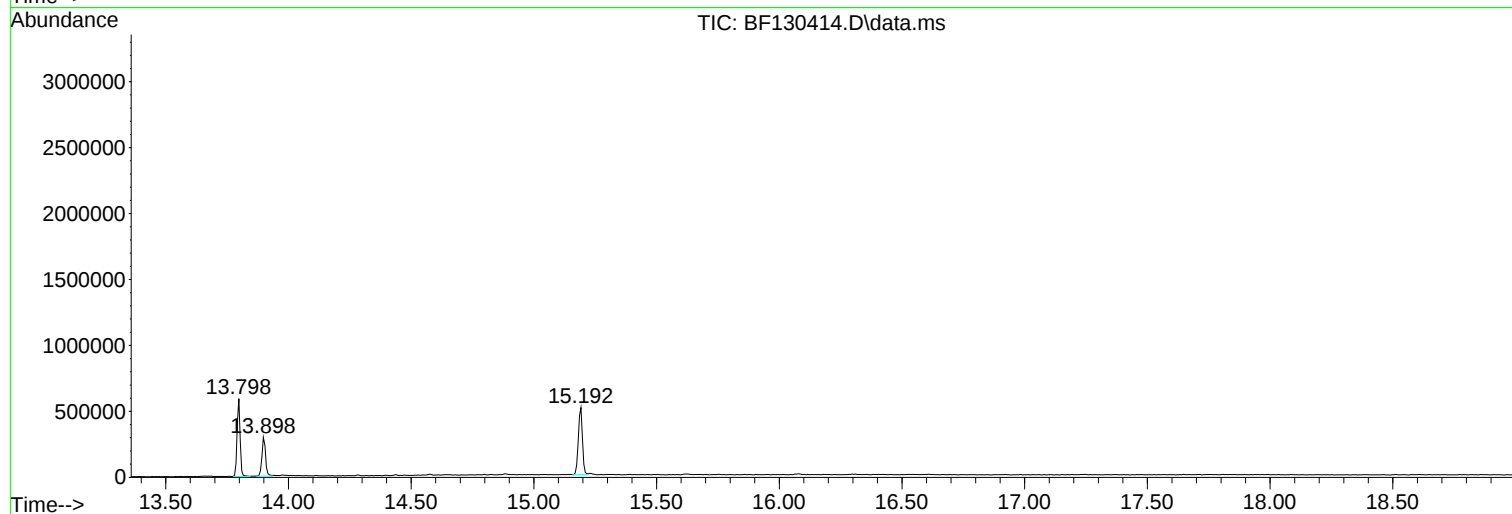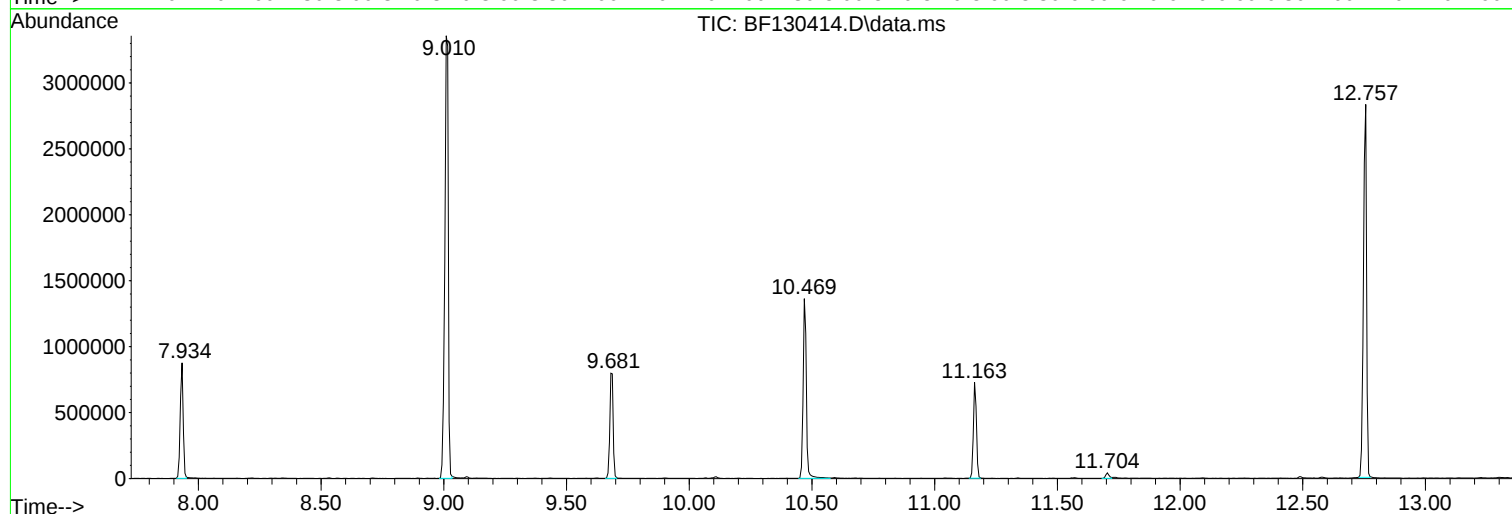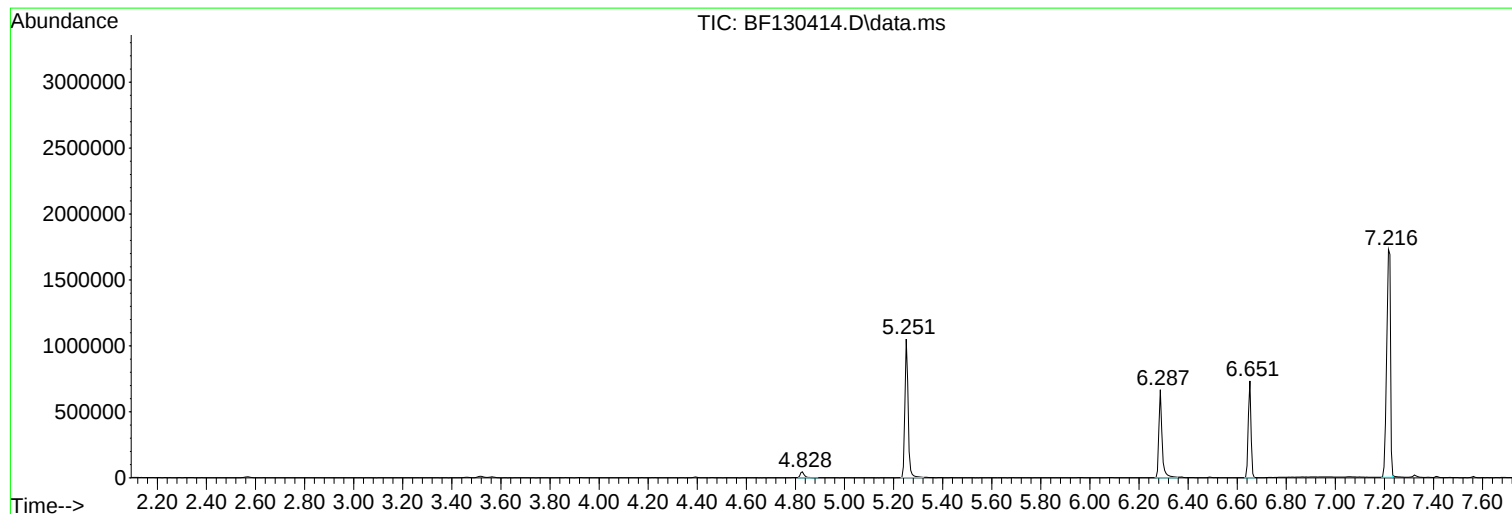

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130414.D
Acq On : 26 Sep 2022 18:32
Operator : CG\JU
Sample : N4742-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-14










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.898	11.66 ng	296286	Chrysene-d12	13.798

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	81
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	37
4			Vanadium, cycloheptatrienyl-(pen...]	277	C17H22V	1000155-20-5	25
5			1H-Indole-3-acetic acid, 5-[(tri...]	277	C14H19N03Si	072101-35-0	17

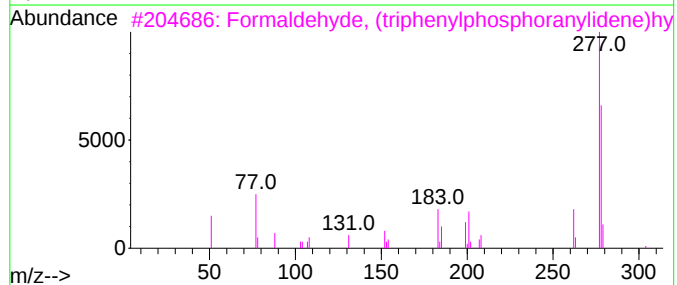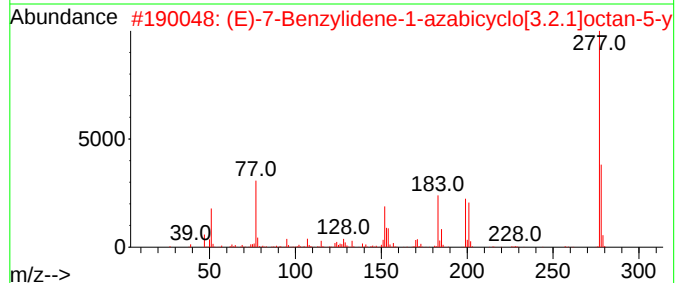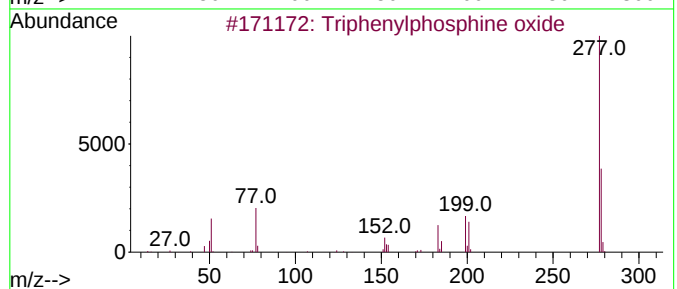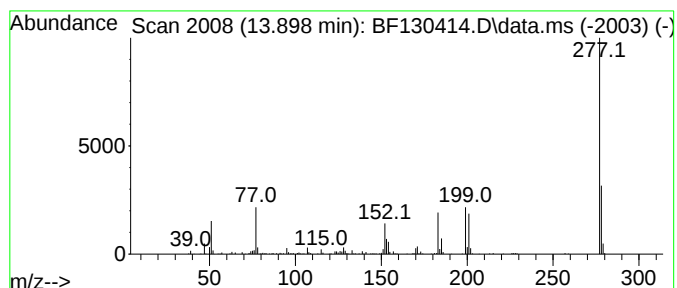

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130414.D
Acq On : 26 Sep 2022 18:32
Operator : CG\JU
Sample : N4742-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.898	11.7	ng	296286	5	13.798	508327	20.0