


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
 Data File : BF130399.D
 Acq On : 26 Sep 2022 09:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 27 01:00:47 2022

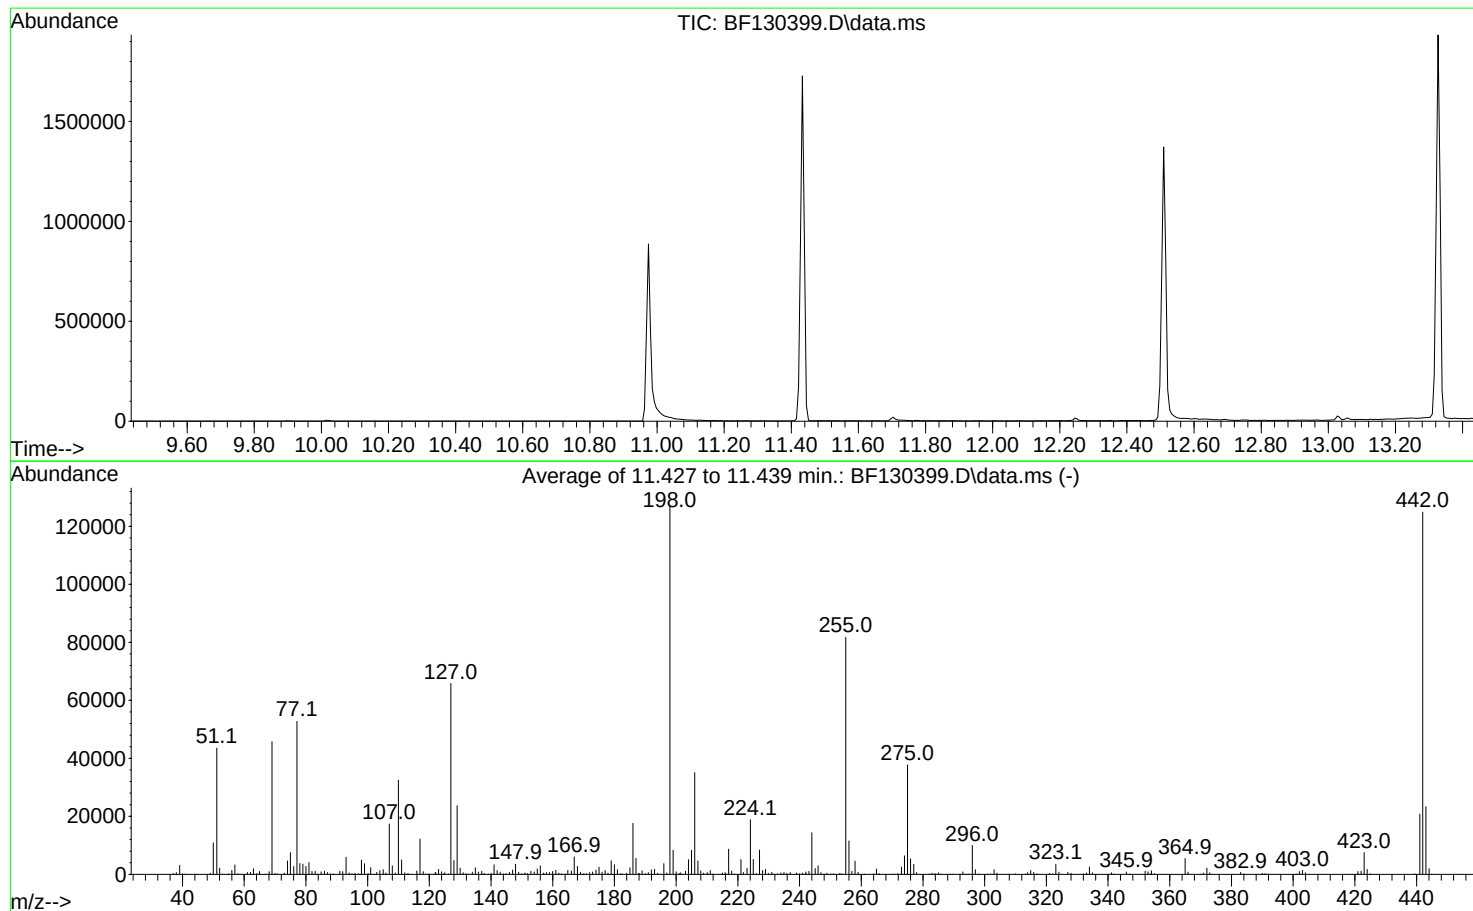




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	43499	PASS
68	69	0.00	2	2.0	892	PASS
69	198	0.00	100	36.0	45707	PASS
70	69	0.00	2	0.6	286	PASS
127	198	10	80	51.9	65813	PASS
197	198	0.00	2	0.4	496	PASS
198	198	100	100	100.0	126864	PASS
199	198	5	9	6.5	8292	PASS
275	198	10	60	29.7	37720	PASS
365	198	1	100	4.3	5427	PASS
441	198	0.01	100	16.4	20749	PASS
442	442	50	100	100.0	124896	PASS
443	442	15	24	18.6	23292	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
 Data File : BF130399.D
 Acq On : 26 Sep 2022 09:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 27 06:55:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 27 01:00:47 2022
 Response via : Initial Calibration

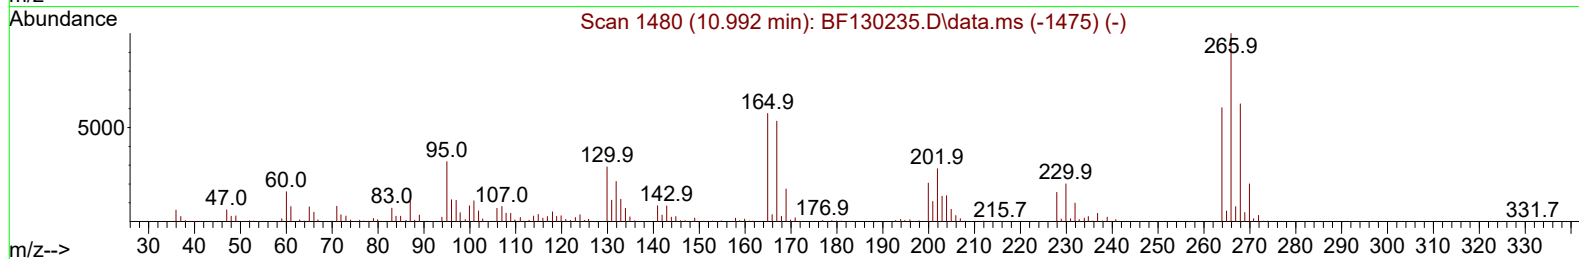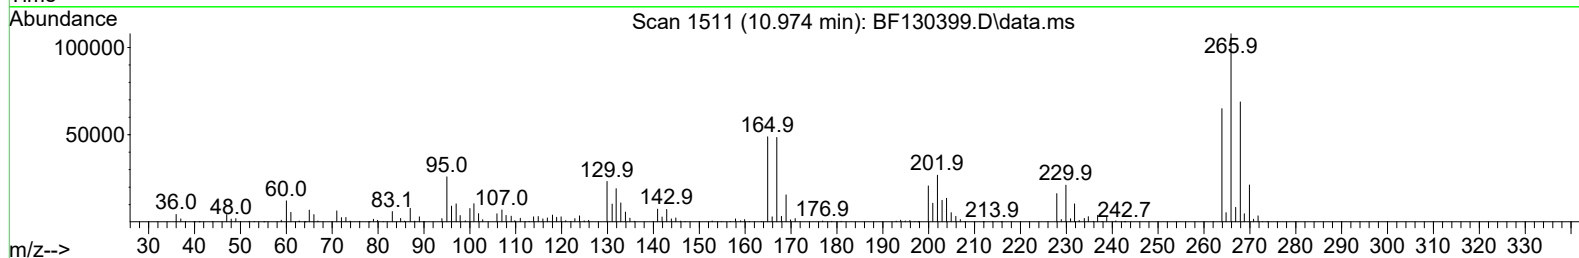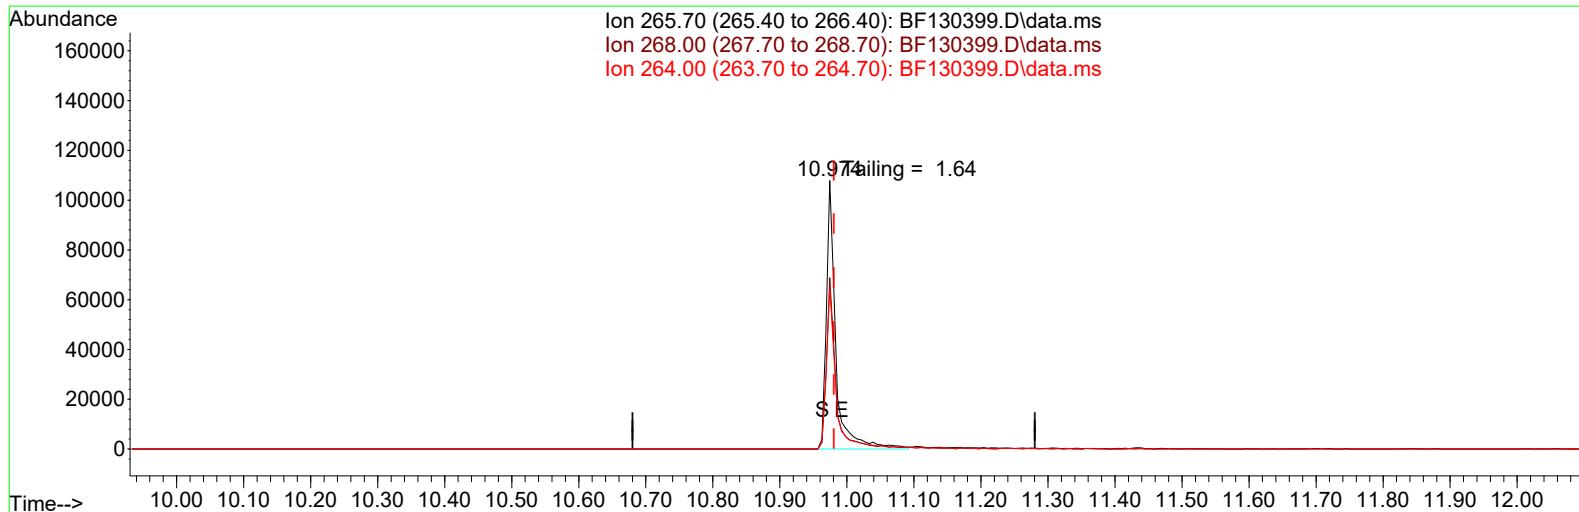

TIC: BF130399.D\data.ms

(70) Pentachlorophenol (C)

10.974min (-0.006) 27636.81 ng




response 105909

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.80
264.00	63.10	60.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092622\
Data File : BF130399.D
Acq On : 26 Sep 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 27 06:55:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration

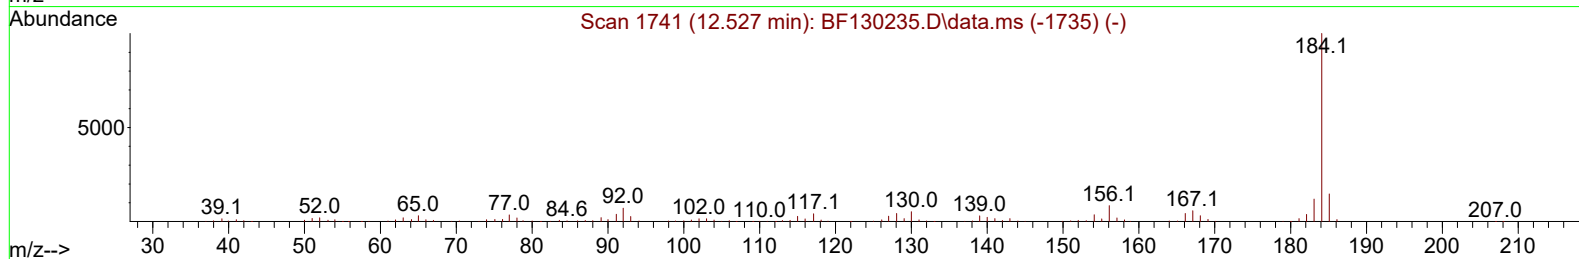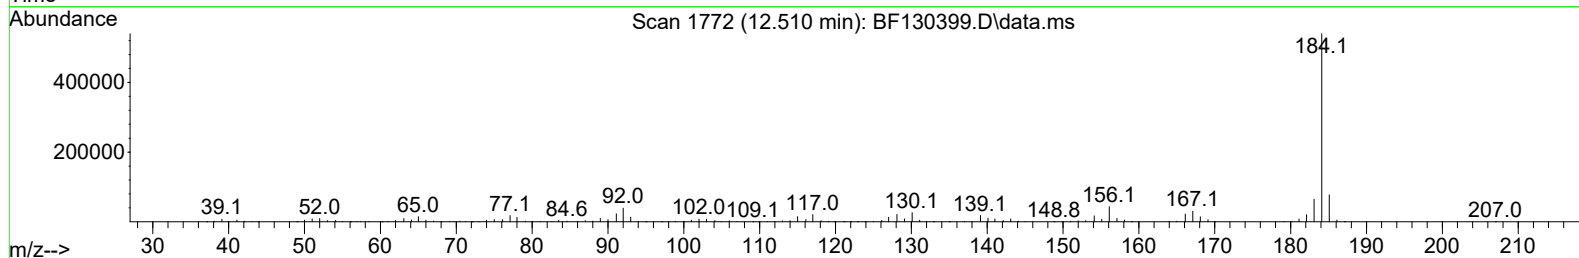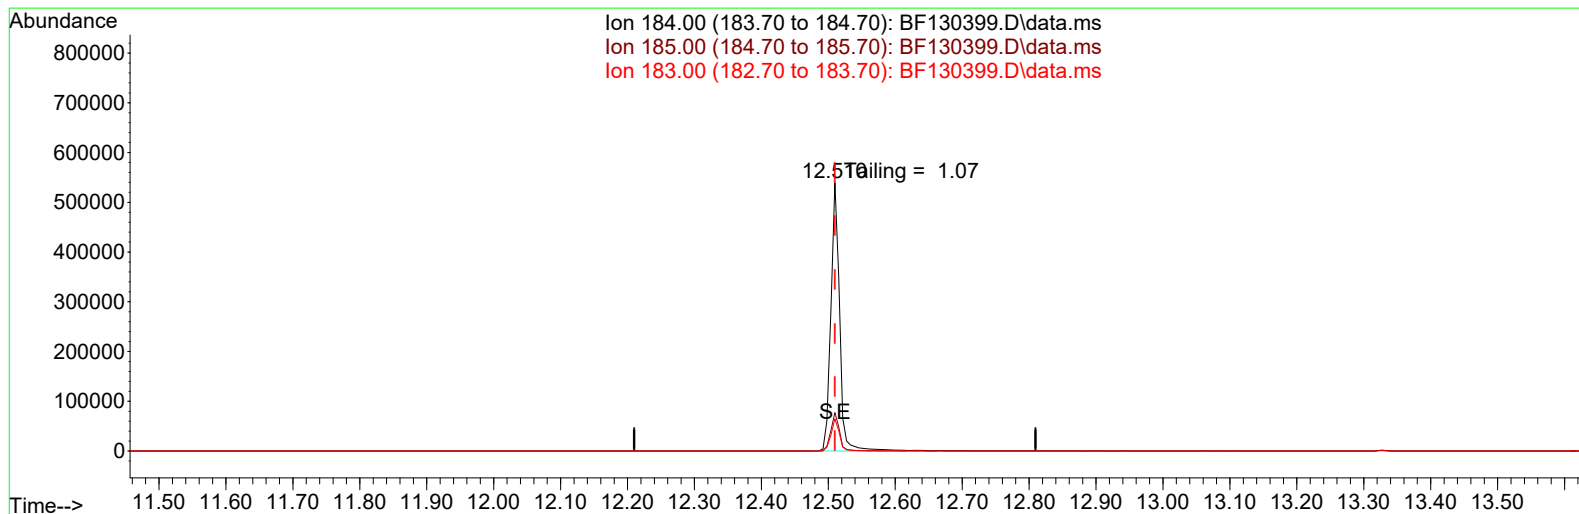

TIC: BF130399.D\data.ms

(77) Benzidine

12.510min (-0.000) 0.00 ng

response 490341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.34
183.00	11.40	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2022	BNA_F	<u>BF130399.D</u>
Compound Name	Response	Retention Time
DDT	298442	13.327
DDD	5188	13.027
DDE	641	12.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5829	304271	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP