

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
 Data File : BF125695.D
 Acq On : 28 Sep 2021 18:33
 Operator : JU/CG
 Sample : M3953-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-RR-01-(2.0)

Quant Time: Sep 29 02:20:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.886	152	201127	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	817753	20.000	ng	# 0.00
39) Acenaphthene-d10	9.922	164	413576	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	681482	20.000	ng	# 0.00
76) Chrysene-d12	14.039	240	403828	20.000	ng	0.00
86) Perylene-d12	15.515	264	409672	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	866538	70.984	ng	0.00
7) Phenol-d6	6.498	99	644120	39.247	ng	-0.01
23) Nitrobenzene-d5	7.445	82	1253700	106.934	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	541335	140.386	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	2261552	100.731	ng	0.00
79) Terphenyl-d14	12.992	244	2137379	91.659	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
Data File : BF125695.D
Acq On : 28 Sep 2021 18:33
Operator : JU/CG
Sample : M3953-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-RR-01-(2.0)

Quant Time: Sep 29 02:20:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration




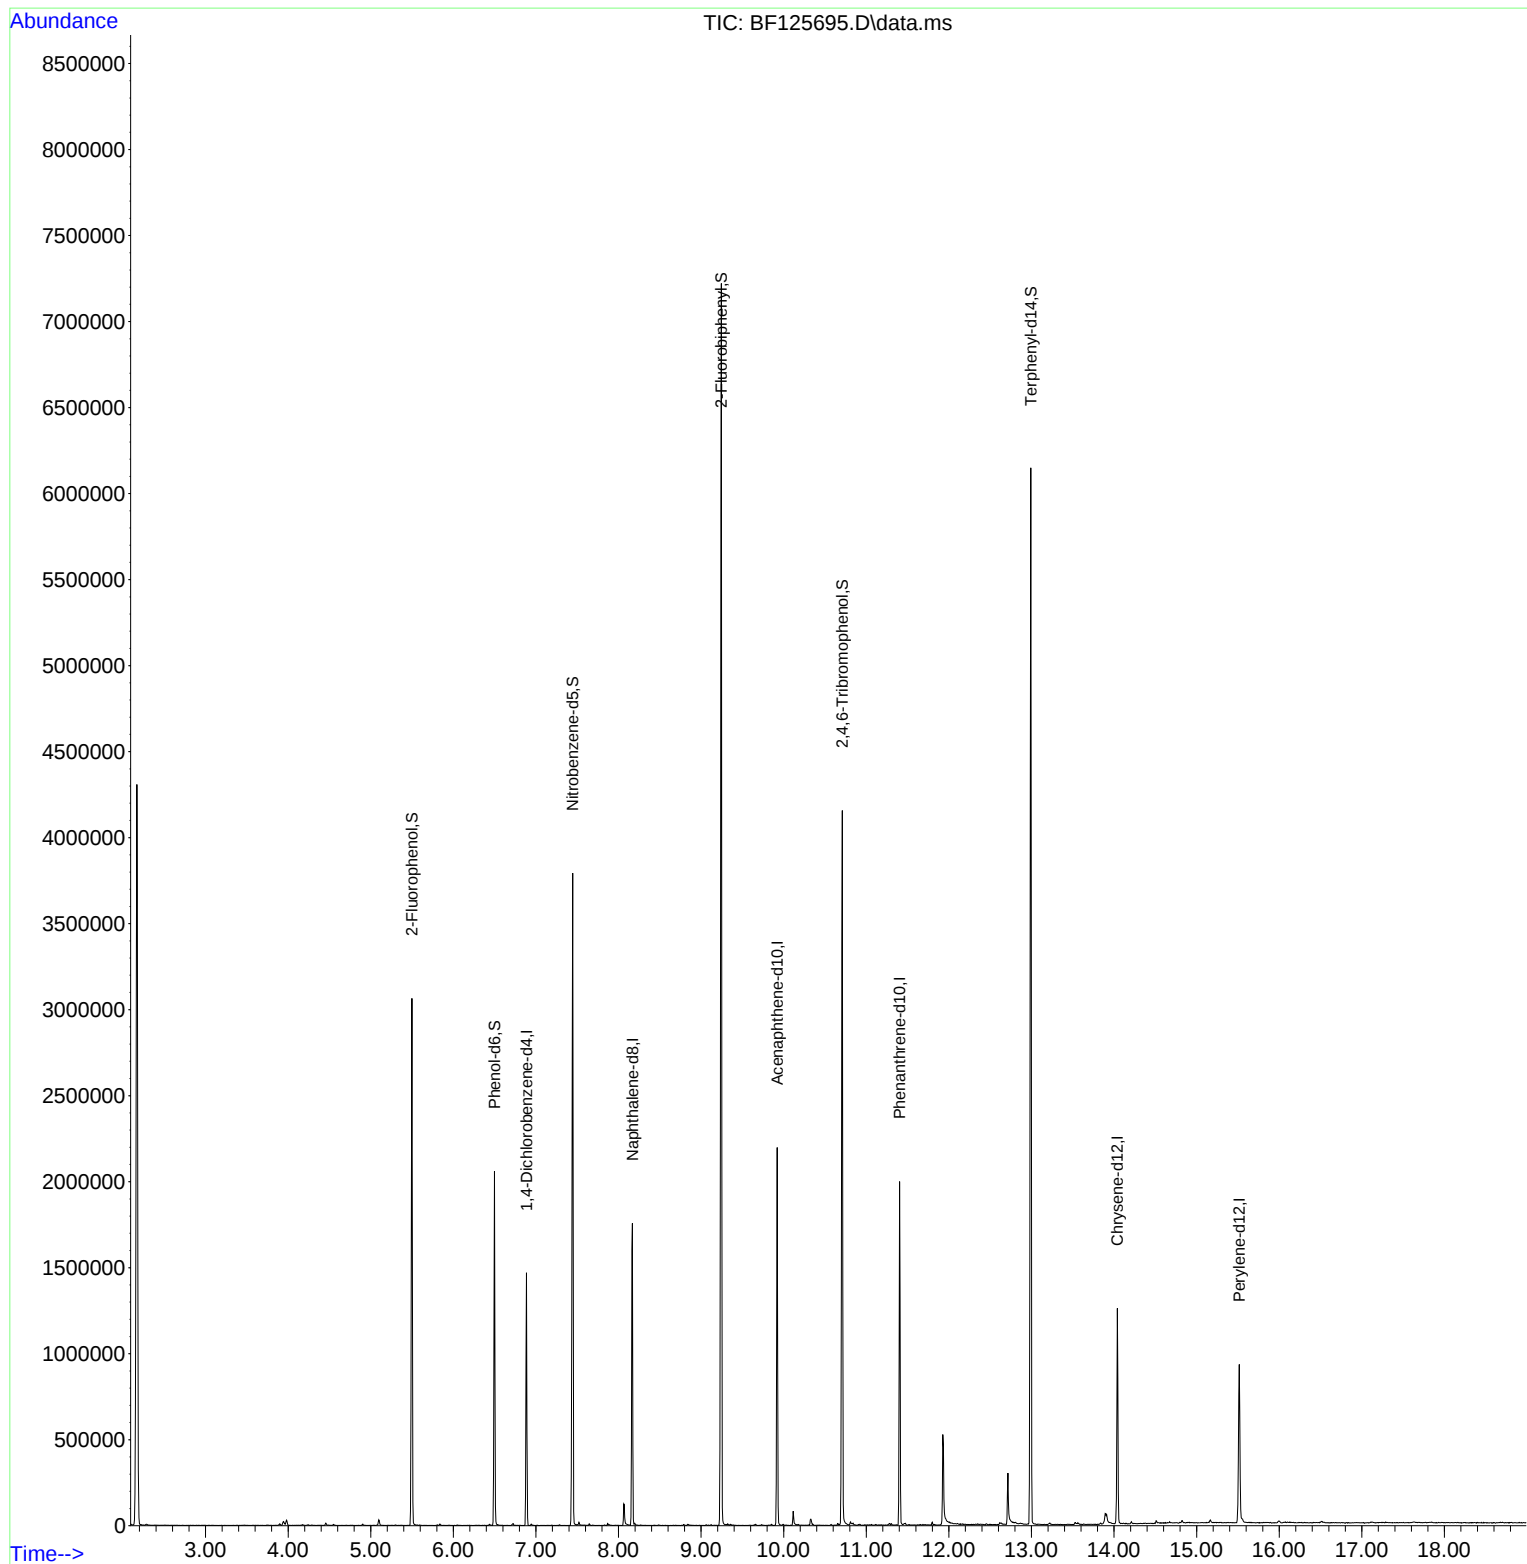




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.886 min Scan# 816
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33




Instrument :
BNA_F
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion:152 Resp: 201127
Ion Ratio Lower Upper
152 100
150 158.7 117.6 176.4
115 60.8 47.1 70.7

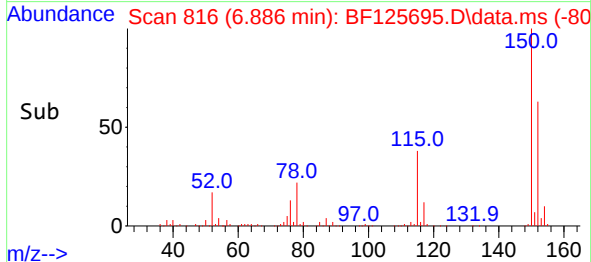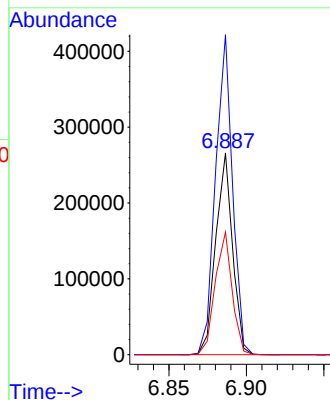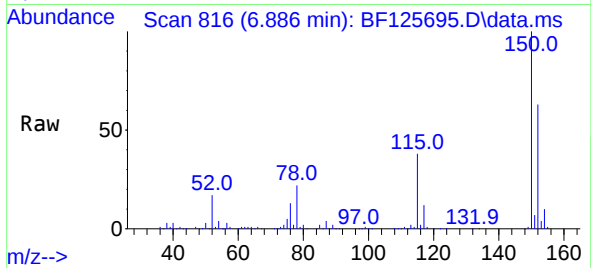

#5
2-Fluorophenol
Concen: 70.984 ng
RT: 5.498 min Scan# 580
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33

Tgt Ion:112 Resp: 866538
Ion Ratio Lower Upper
112 100
64 52.5 44.2 66.2
63 26.1 26.2 39.2#


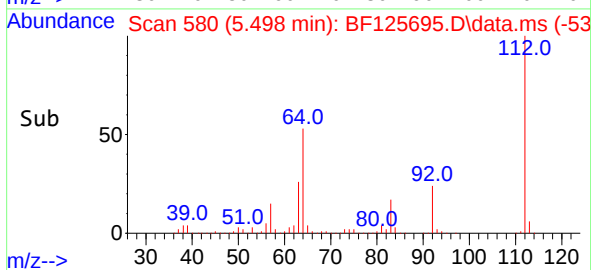
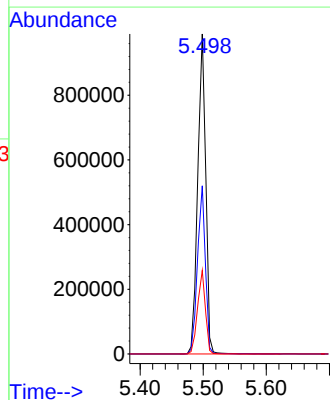
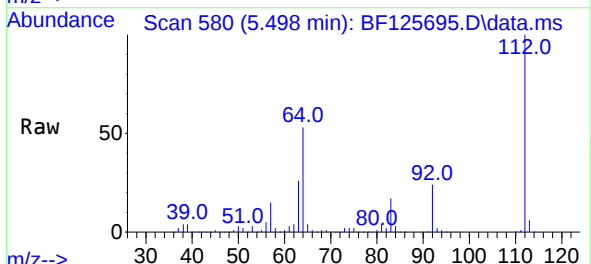




#7
Phenol-d6
Concen: 39.247 ng
RT: 6.498 min Scan# 750
Delta R.T. -0.012 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33




Instrument :
BNA_F
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion: 99 Resp: 644120
Ion Ratio Lower Upper
99 100
42 14.1 23.5 35.3#
71 28.6 25.6 38.4

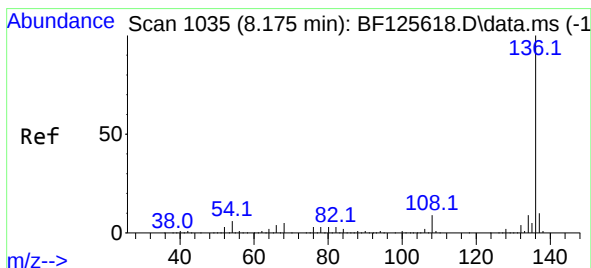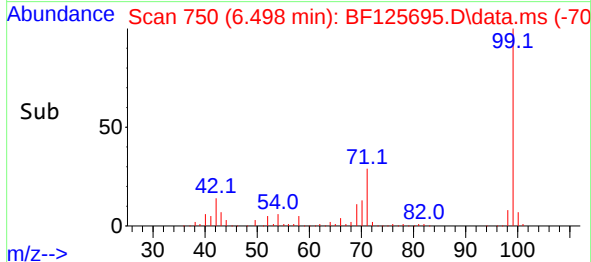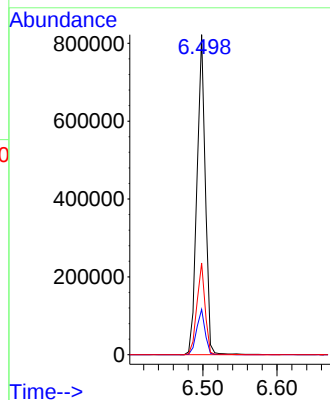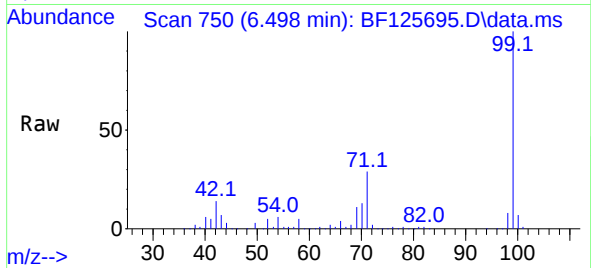

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33

Tgt Ion: 136 Resp: 817753
Ion Ratio Lower Upper
136 100
137 10.5 9.8 14.6
54 6.3 6.4 9.6#
68 5.1 3.3 4.9#


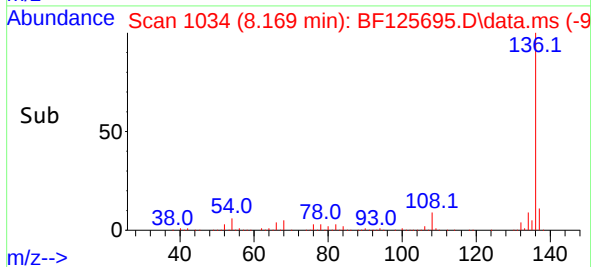
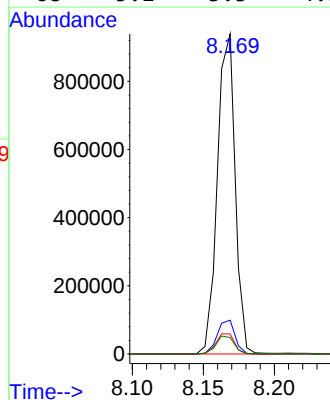
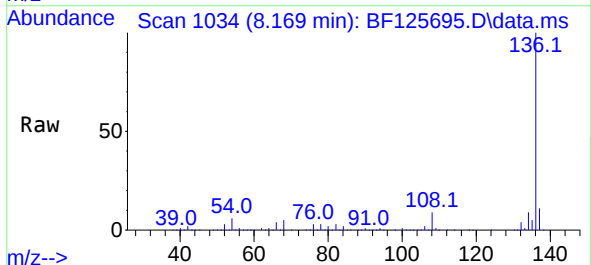




#23
Nitrobenzene-d5
Concen: 106.934 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33




Instrument :
BNA_F
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion: 82 Resp: 1253700
Ion Ratio Lower Upper
82 100
128 48.7 40.6 60.8
54 44.1 49.6 74.4#

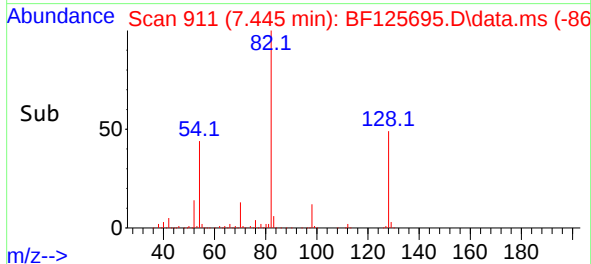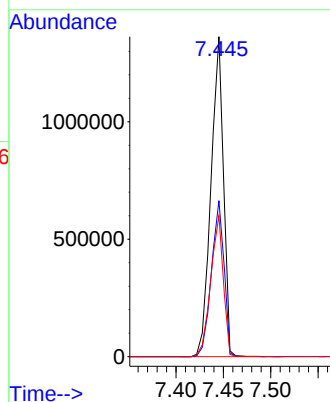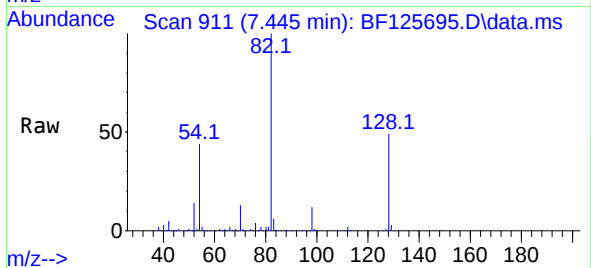

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.922 min Scan# 1332
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33

Tgt Ion:164 Resp: 413576
Ion Ratio Lower Upper
164 100
162 100.9 81.3 121.9
160 44.9 38.0 57.0


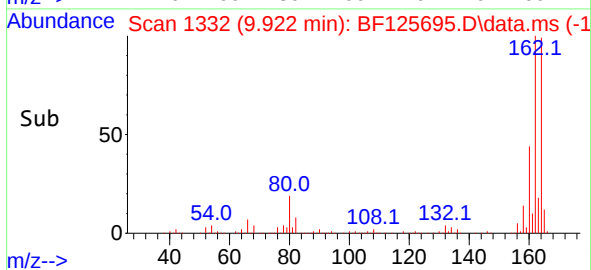
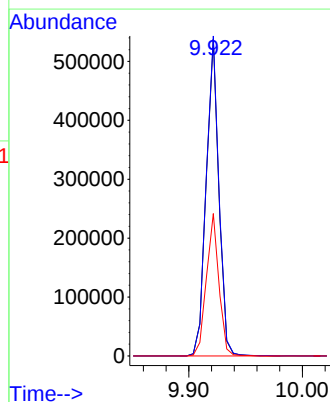
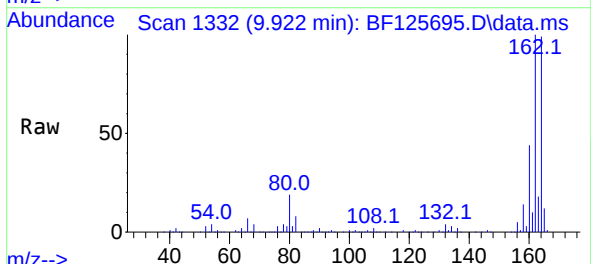




#42
2,4,6-Tribromophenol
Concen: 140.386 ng
RT: 10.710 min Scan# 1466
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33




Instrument :
BNA_F
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion:330 Resp: 541335
Ion Ratio Lower Upper
330 100
332 97.4 76.2 114.4
141 31.1 44.6 66.8#

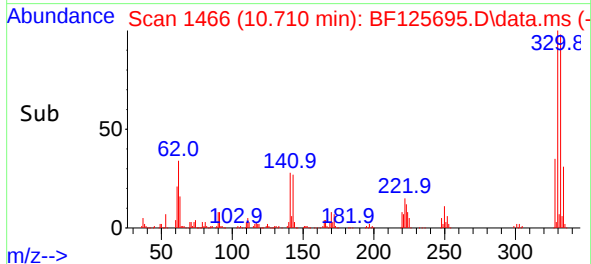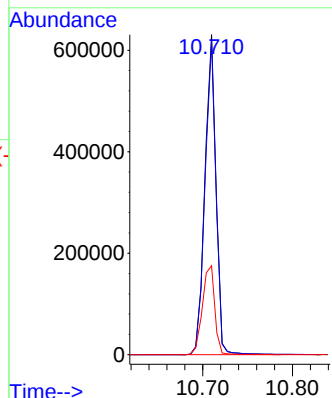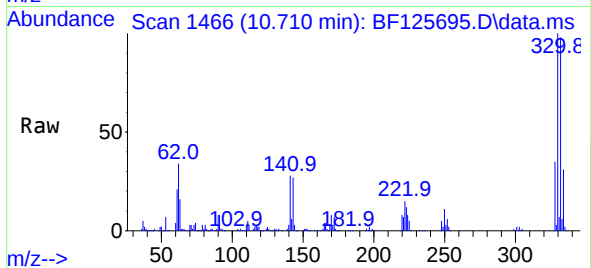

#45
2-Fluorobiphenyl
Concen: 100.731 ng
RT: 9.245 min Scan# 1217
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33

Tgt Ion:172 Resp: 2261552
Ion Ratio Lower Upper
172 100
171 38.5 26.5 39.7
170 25.9 18.8 28.2


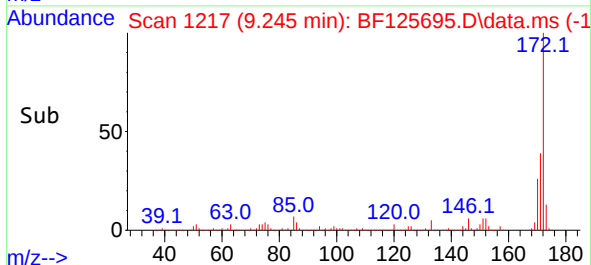
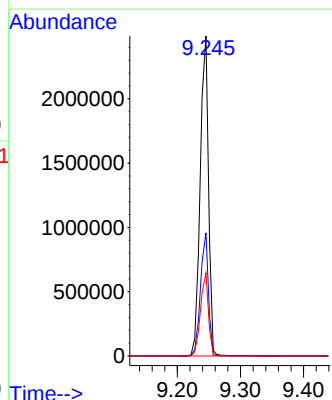
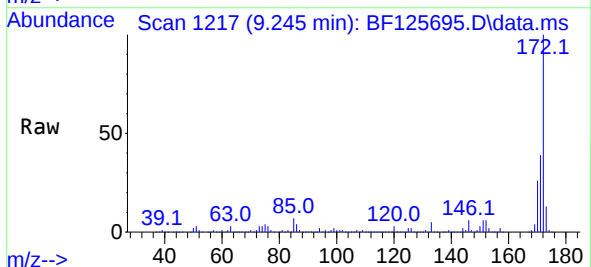




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 1584
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33




Instrument :
BNA_F
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion:188 Resp: 681482
Ion Ratio Lower Upper
188 100
94 10.4 6.7 10.1#
80 10.6 7.5 11.3

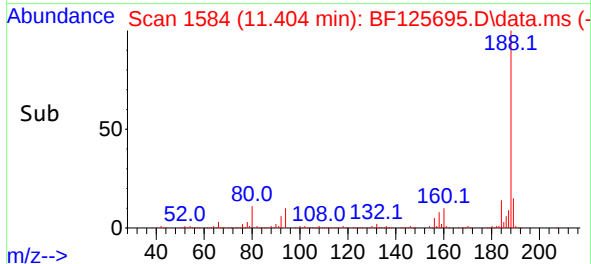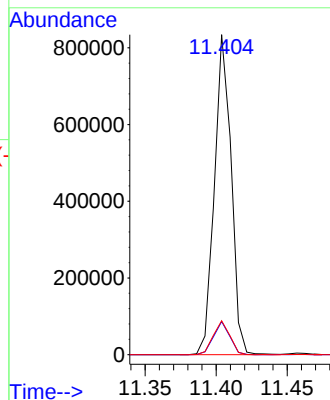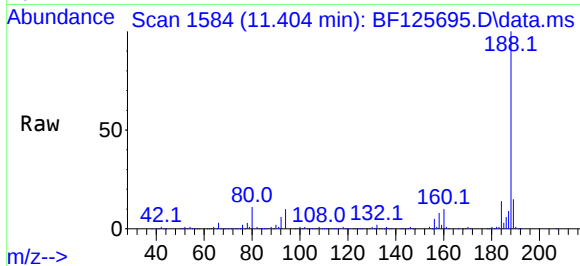

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33

Tgt Ion:240 Resp: 403828
Ion Ratio Lower Upper
240 100
120 13.5 10.8 16.2
236 26.5 21.6 32.4


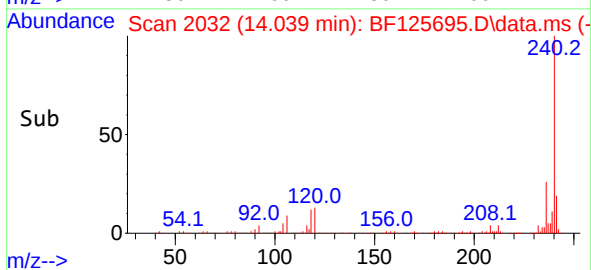
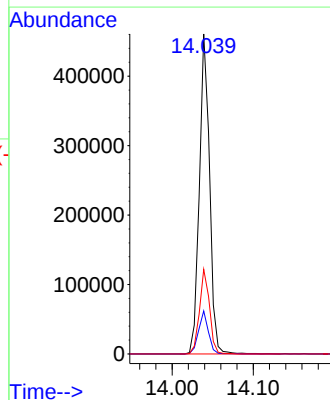
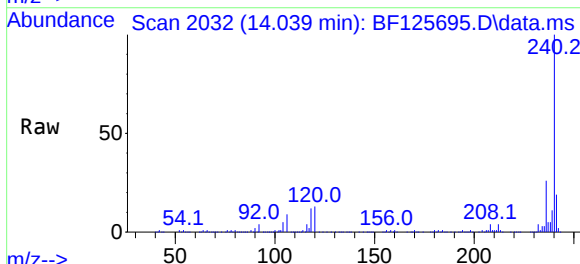


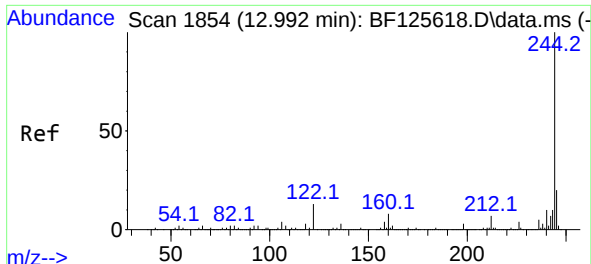

#79
Terphenyl-d14
Concen: 91.659 ng
RT: 12.992 min Scan# 1854
Delta R.T. 0.000 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33

Instrument :
BNA_F
ClientSampleId :
SW-RR-01-(2.0)

Tgt Ion:244 Resp: 2137379
Ion Ratio Lower Upper
244 100
212 6.8 5.9 8.9
122 12.5 9.0 13.4

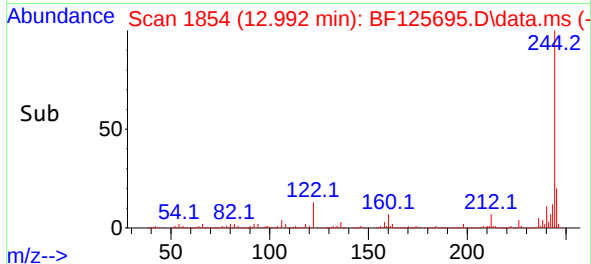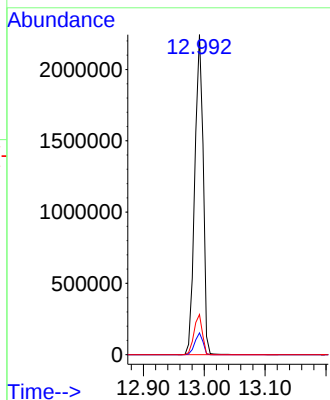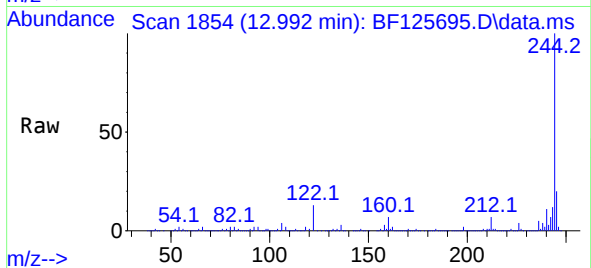

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.515 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BF125695.D
Acq: 28 Sep 2021 18:33

Tgt Ion:264 Resp: 409672
Ion Ratio Lower Upper
264 100
260 24.1 19.6 29.4
265 21.5 17.2 25.8

