

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
 Data File : BF125686.D
 Acq On : 28 Sep 2021 13:26
 Operator : JU/CG
 Sample : PB139432BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139432BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.251	19	28	34	rVB	138988	188350	2.37%	0.400%
2	5.516	577	583	586	rBV	6092800	6423516	80.90%	13.627%
3	6.510	746	752	755	rBV	5427182	6408601	80.71%	13.595%
4	6.886	812	816	820	rBV	1870346	1460790	18.40%	3.099%
5	7.445	906	911	914	rBV	3780323	4210445	53.02%	8.932%
6	8.169	1029	1034	1037	rBV	2341351	2044066	25.74%	4.336%
7	9.245	1211	1217	1220	rBV	7955245	7940547	100.00%	16.845%
8	9.922	1327	1332	1336	rBV	2753198	2332620	29.38%	4.949%
9	10.710	1461	1466	1469	rBV	4746074	4388595	55.27%	9.310%
10	11.404	1581	1584	1588	rBV	2412824	2172499	27.36%	4.609%
11	12.998	1850	1855	1858	rBV	6416103	6789826	85.51%	14.404%
12	14.045	2029	2033	2044	rVB	1414301	1387697	17.48%	2.944%
13	15.351	2245	2255	2269	rBV5	20810	87610	1.10%	0.186%
14	15.521	2278	2284	2289	rBV	1009368	1302678	16.41%	2.764%




Sum of corrected areas: 47137840

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
Data File : BF125686.D
Acq On : 28 Sep 2021 13:26
Operator : JU/CG
Sample : PB139432BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139432BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

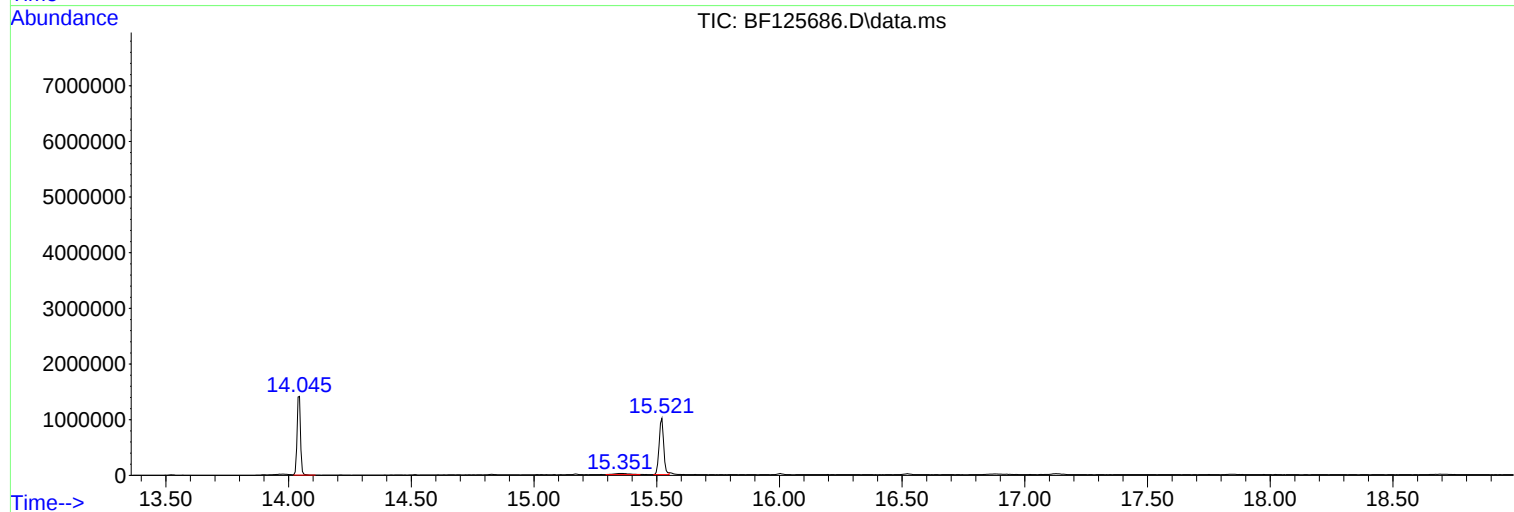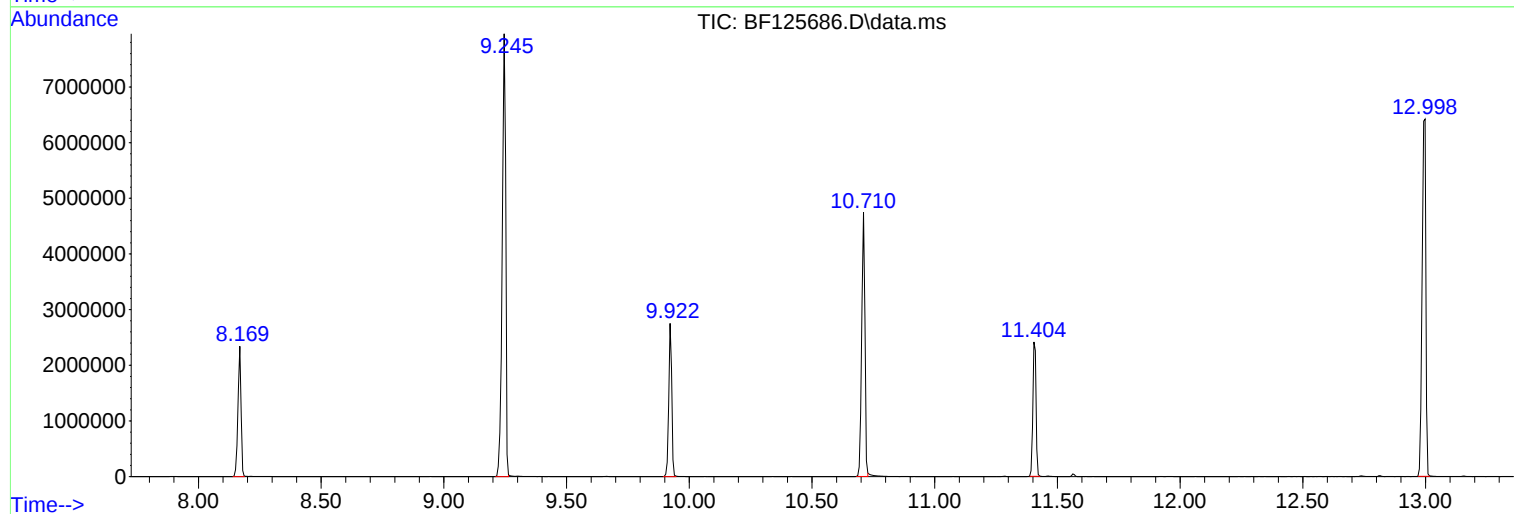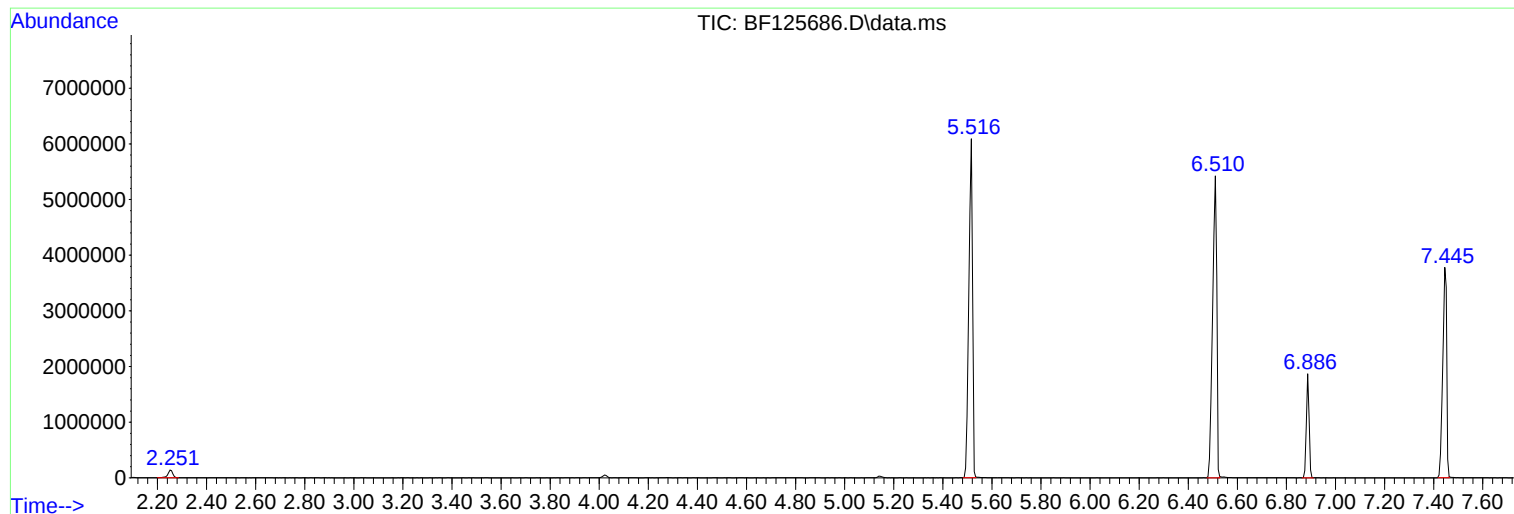

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
Data File : BF125686.D
Acq On : 28 Sep 2021 13:26
Operator : JU/CG
Sample : PB139432BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139432BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.251	2.58 ng	188350	1,4-Dichlorobenzene-d4	6.886

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	10
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

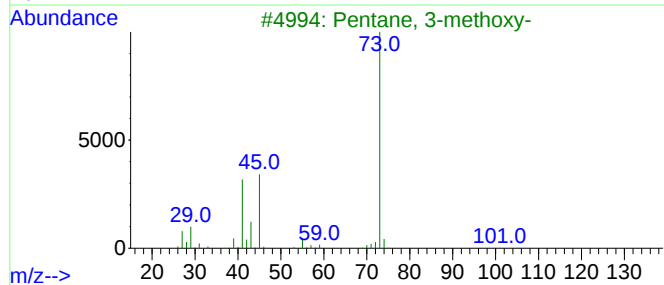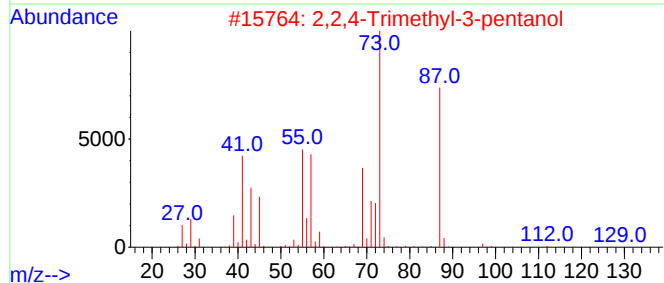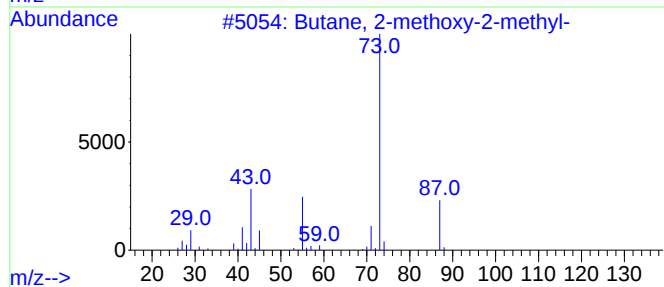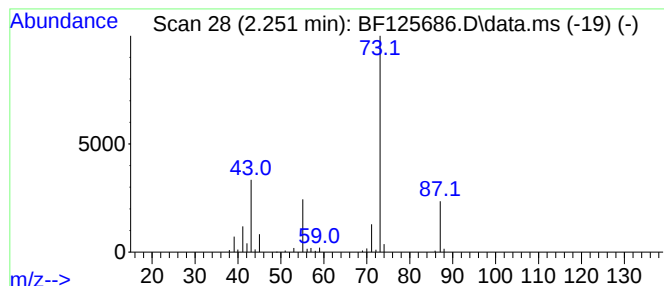

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
Data File : BF125686.D
Acq On : 28 Sep 2021 13:26
Operator : JU/CG
Sample : PB139432BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139432BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.251	2.6	ng	188350	1	6.886	1460790	20.0