
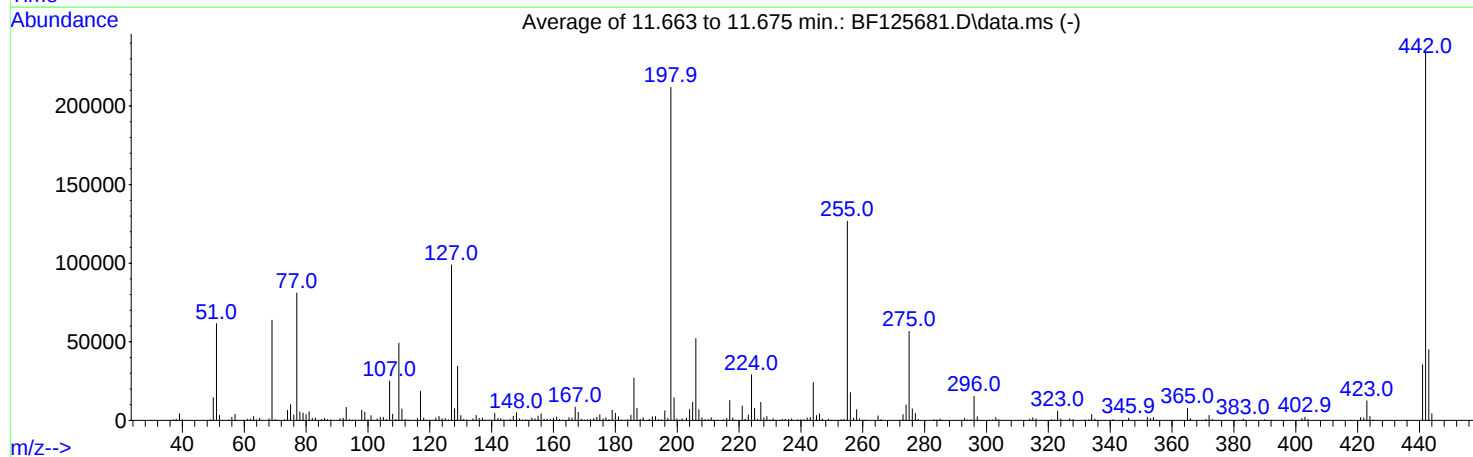


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
 Data File : BF125681.D
 Acq On : 28 Sep 2021 10:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 15:38:32 2021

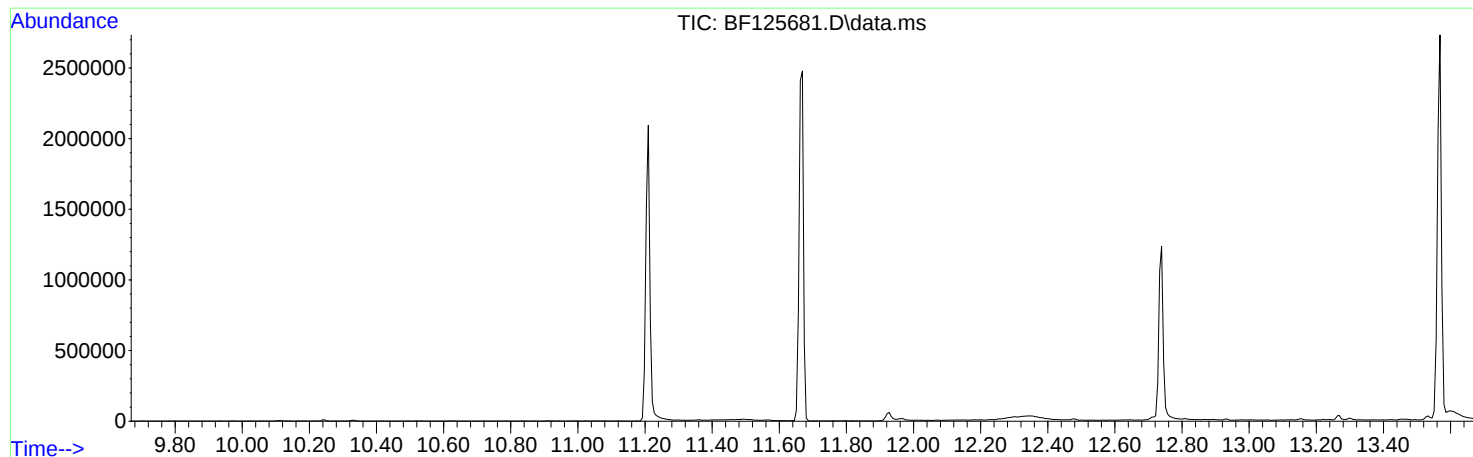




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	61464	PASS
68	69	0.00	2	1.7	1070	PASS
69	198	0.00	100	30.1	63760	PASS
70	69	0.00	2	0.6	409	PASS
127	198	10	80	46.7	98869	PASS
197	198	0.00	2	0.6	1311	PASS
198	198	100	100	100.0	211936	PASS
199	198	5	9	6.8	14368	PASS
275	198	10	60	26.7	56651	PASS
365	198	1	100	3.7	7743	PASS
441	198	0.01	100	16.7	35451	PASS
442	442	50	100	100.0	234048	PASS
443	442	15	24	19.2	44997	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
Data File : BF125681.D
Acq On : 28 Sep 2021 10:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 28 10:51:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

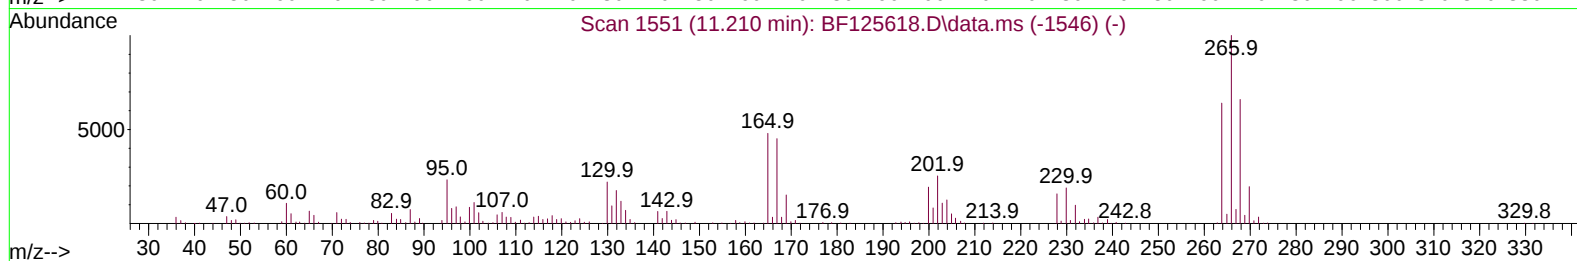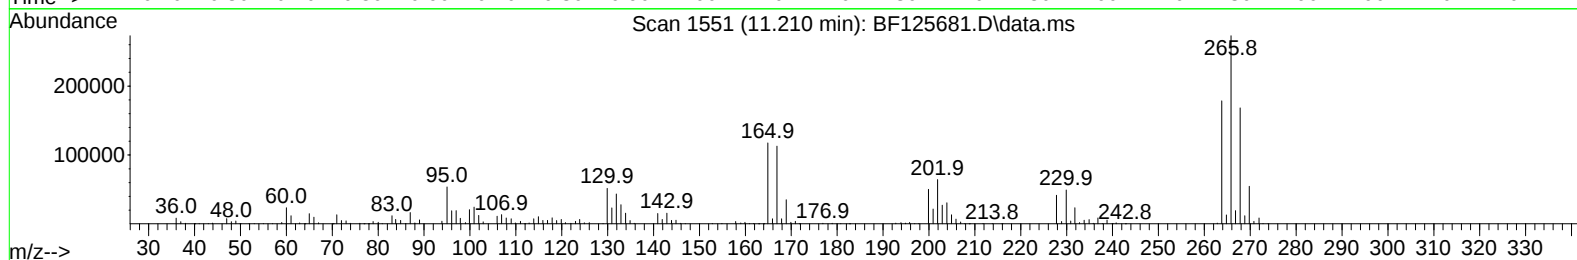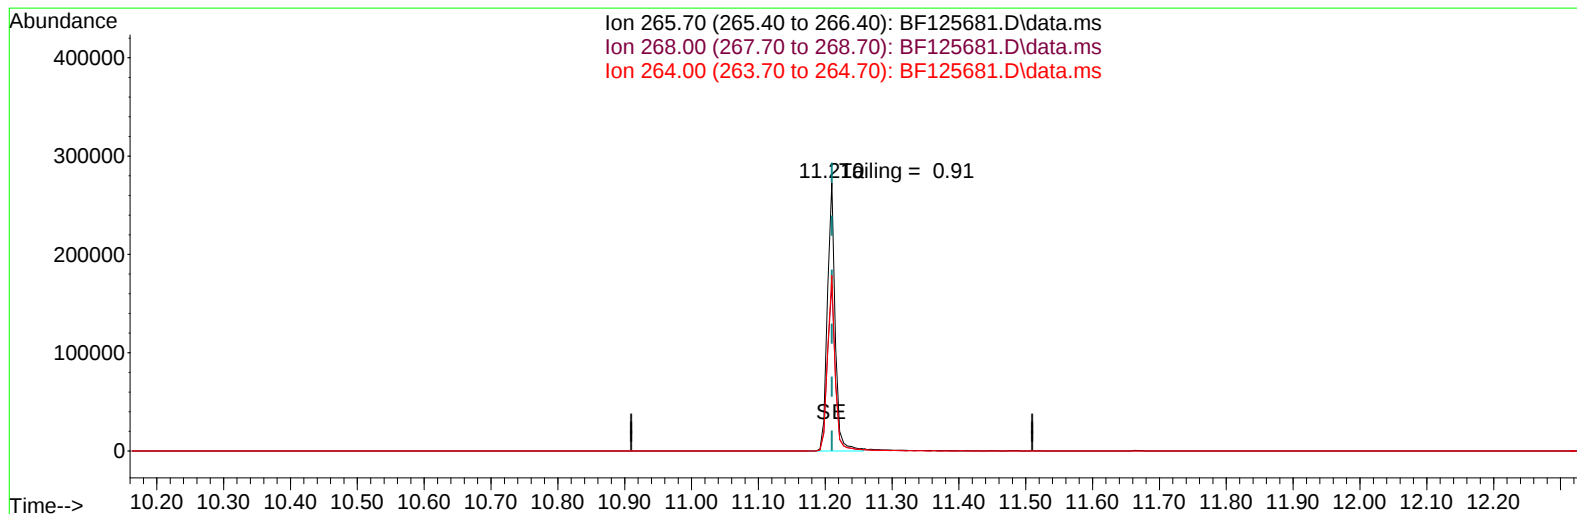

TIC: BF125681.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 35858.83 ng




response 224798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.70
264.00	69.90	65.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092821\
Data File : BF125681.D
Acq On : 28 Sep 2021 10:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 28 10:51:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

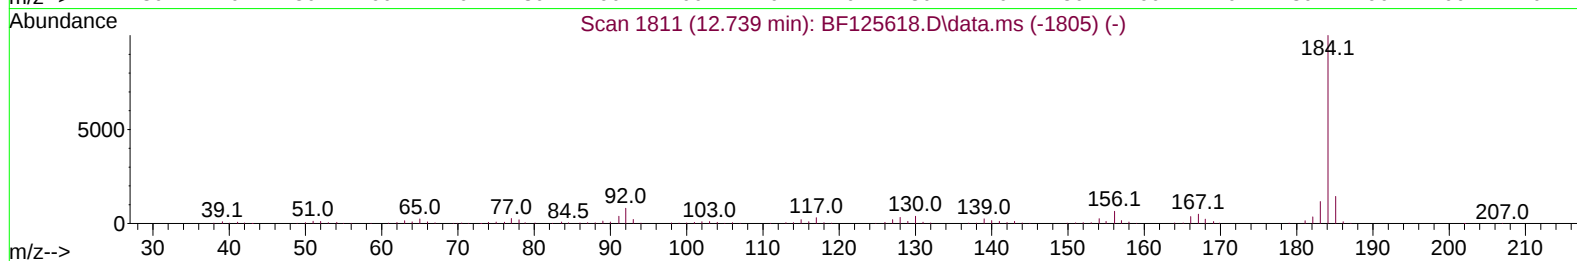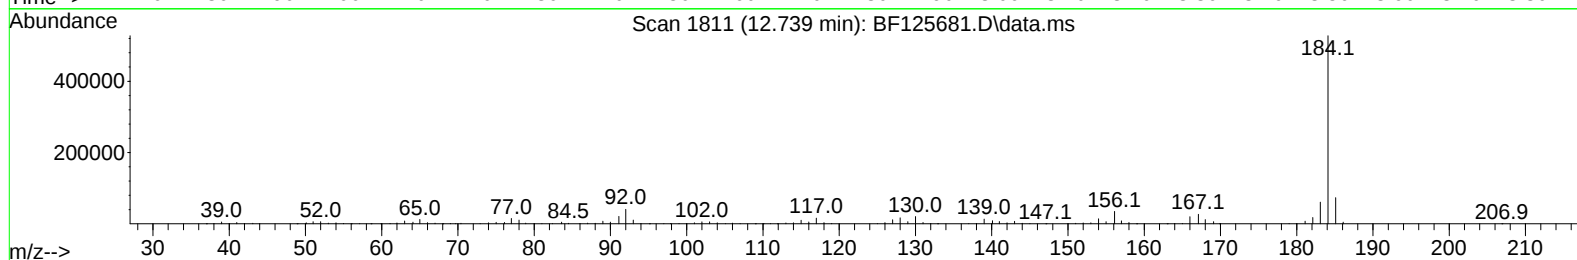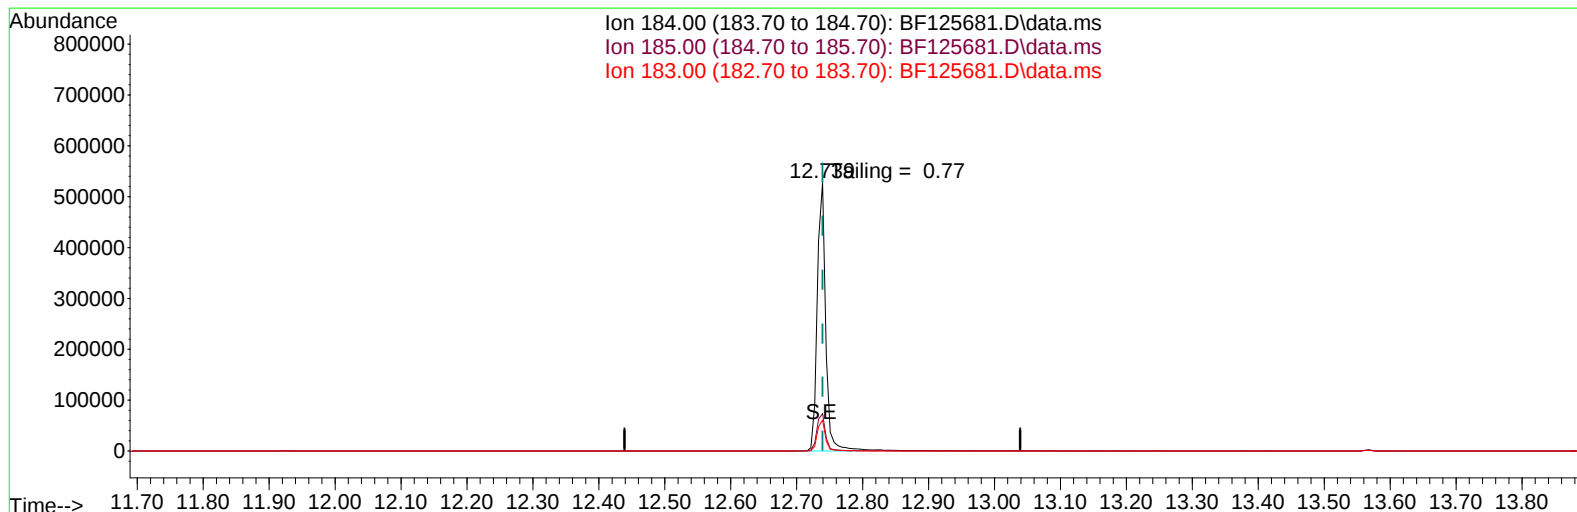

TIC: BF125681.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 0.00 ng

response 472793

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.96
183.00	10.10	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/28/2021	BNA_F	<u>BF125681.D</u>
Compound Name	Response	Retention Time
DDT	441795	13.56
DDD	6010	13.26
DDE	1489	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7499	449294	1.67