
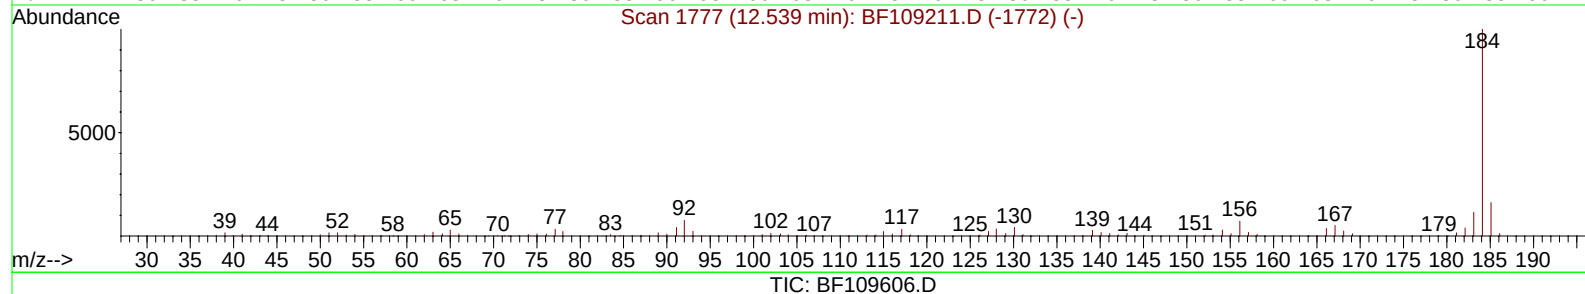
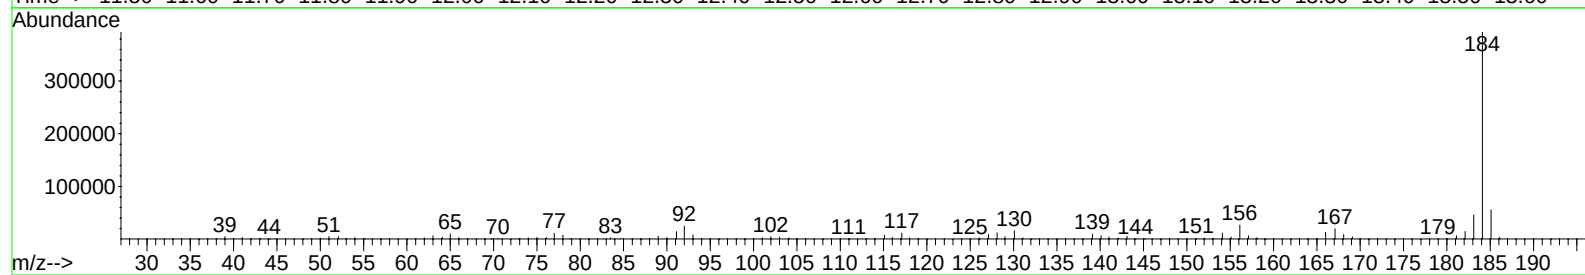


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100518\
 Data File : BF109606.D
 Acq On : 5 Oct 2018 11:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 15:38:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration

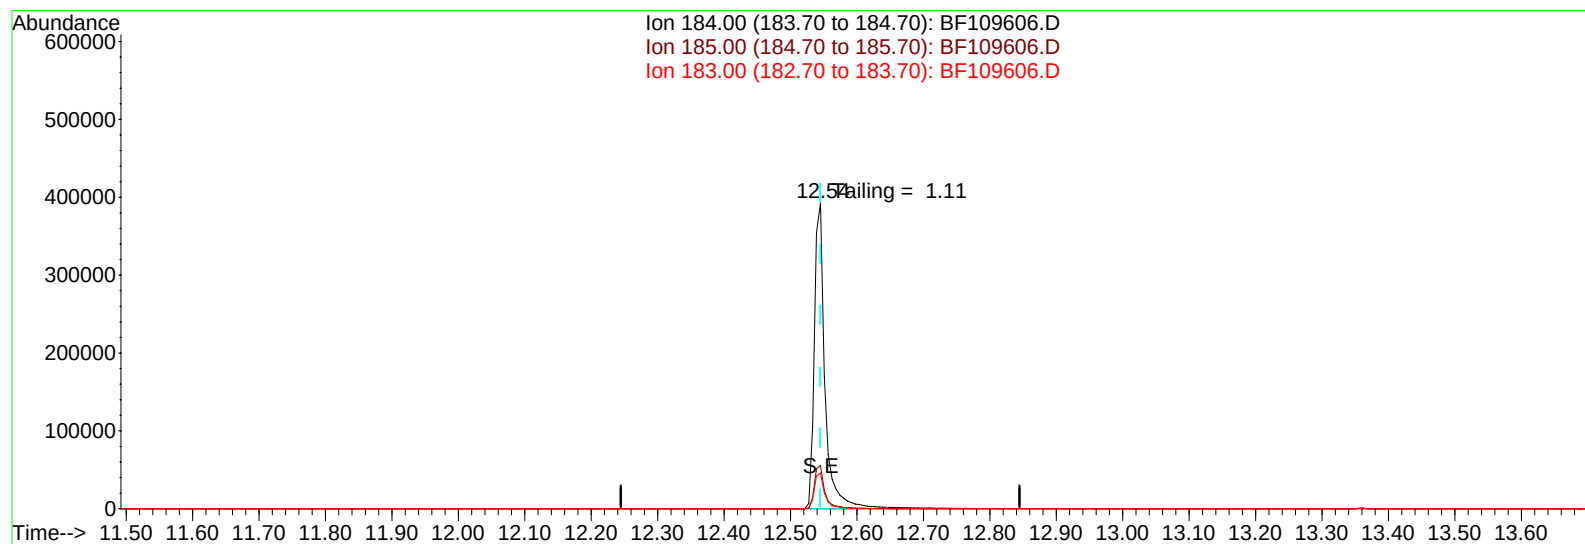

(76) Benzidine




12.545min (-0.000) 0.00ng

response 441892

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.17
183.00	11.60	11.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100518\
Data File : BF109606.D
Acq On : 5 Oct 2018 11:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 15:38:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

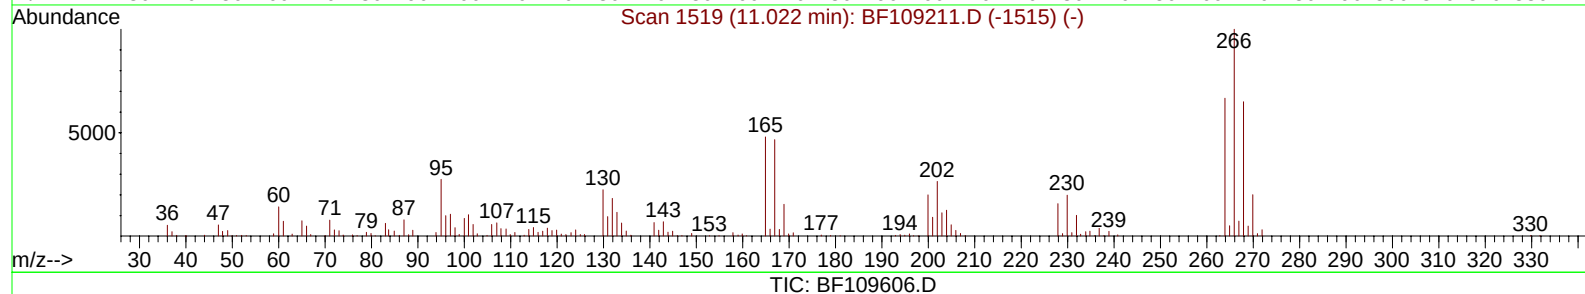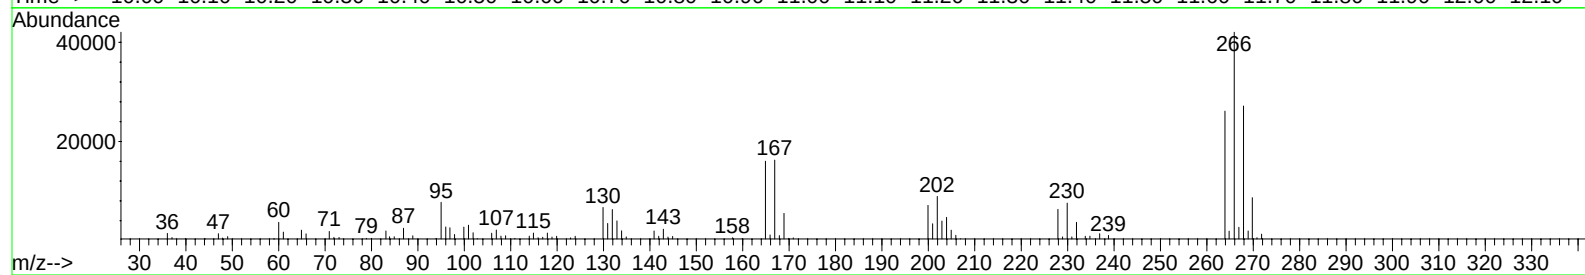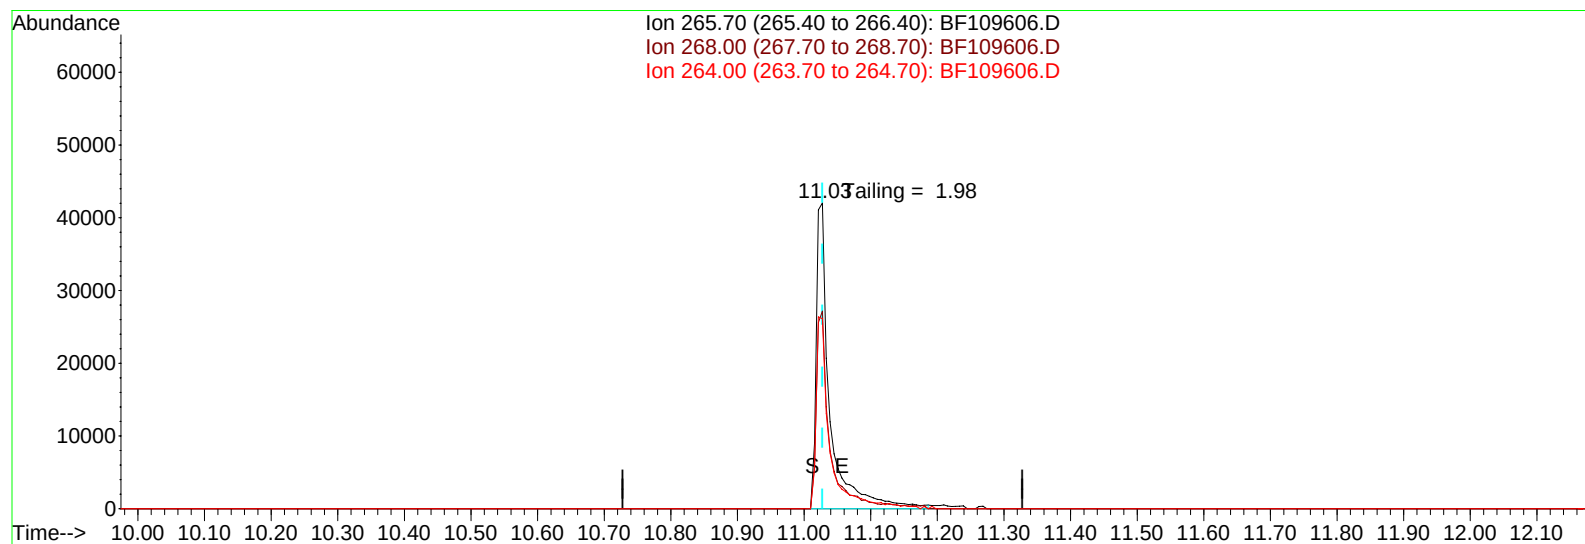

(69) Pentachlorophenol (C)

11.027min (-0.000) 38702.56ng

response 60375

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.62
264.00	61.90	62.16
0.00	0.00	0.00