
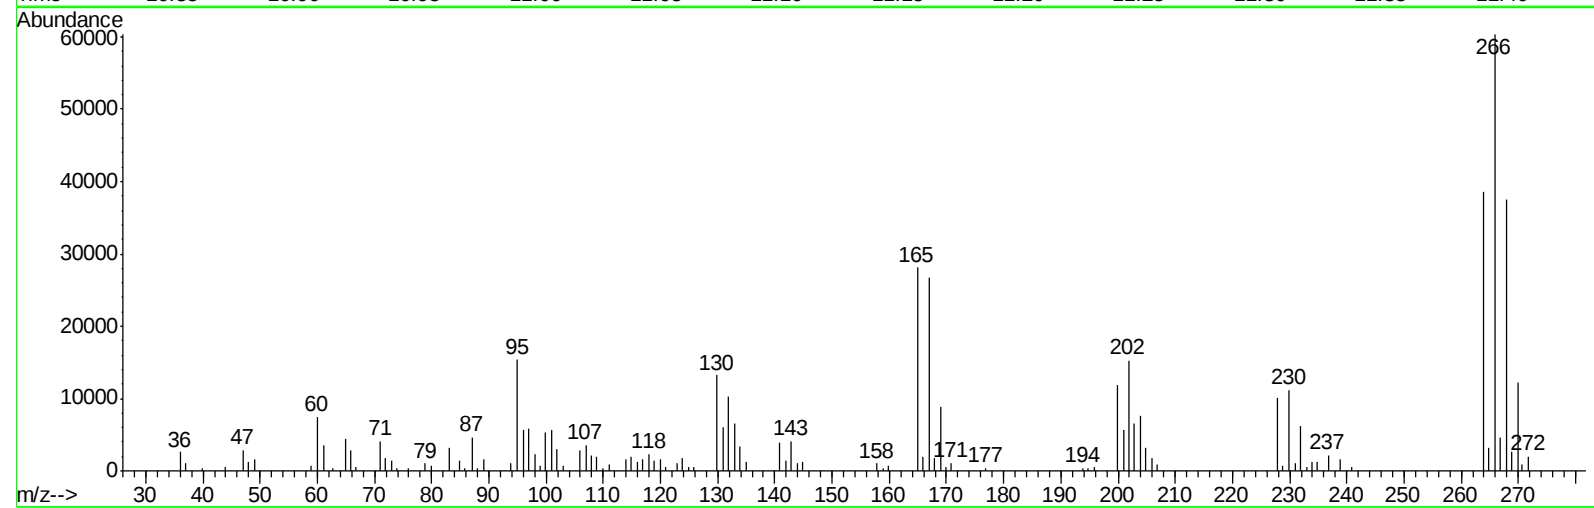


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100518\
Data File : BF109615.D
Acq On : 5 Oct 2018 18:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 08:06:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

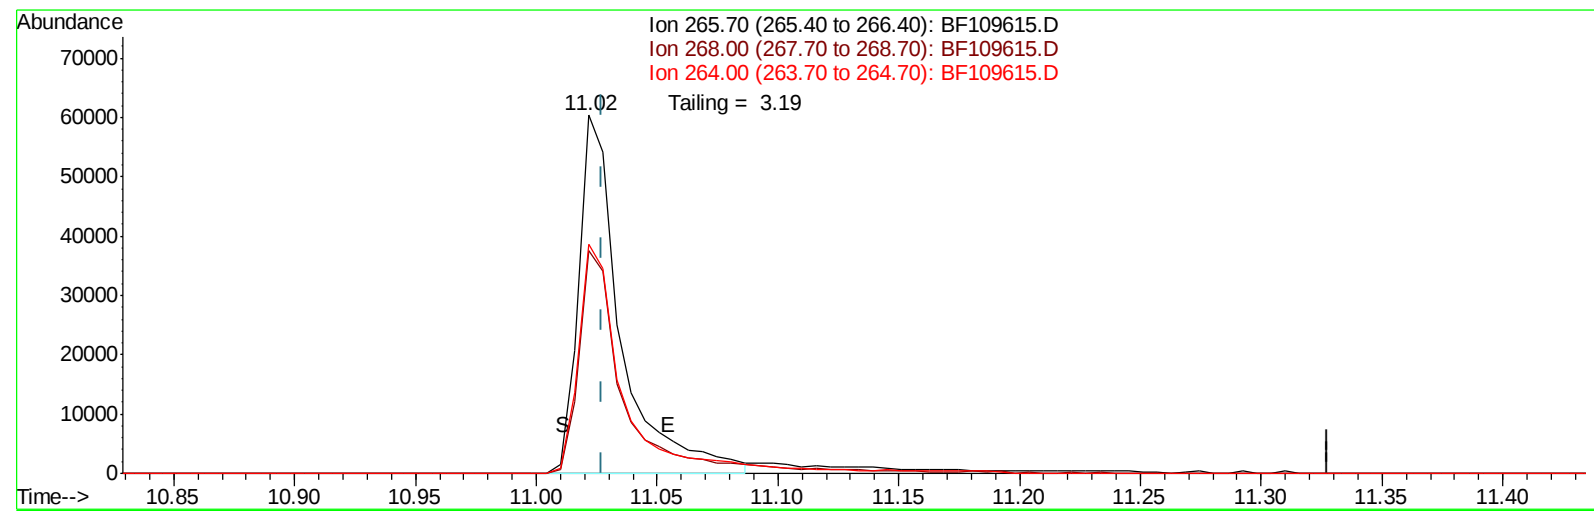

TIC: BF109615.D

(69) Pentachlorophenol (C)



11.022min (-0.006) 36325.92ng

response 80514

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.10
264.00	61.90	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100518\
 Data File : BF109615.D
 Acq On : 5 Oct 2018 18:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 08:06:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration

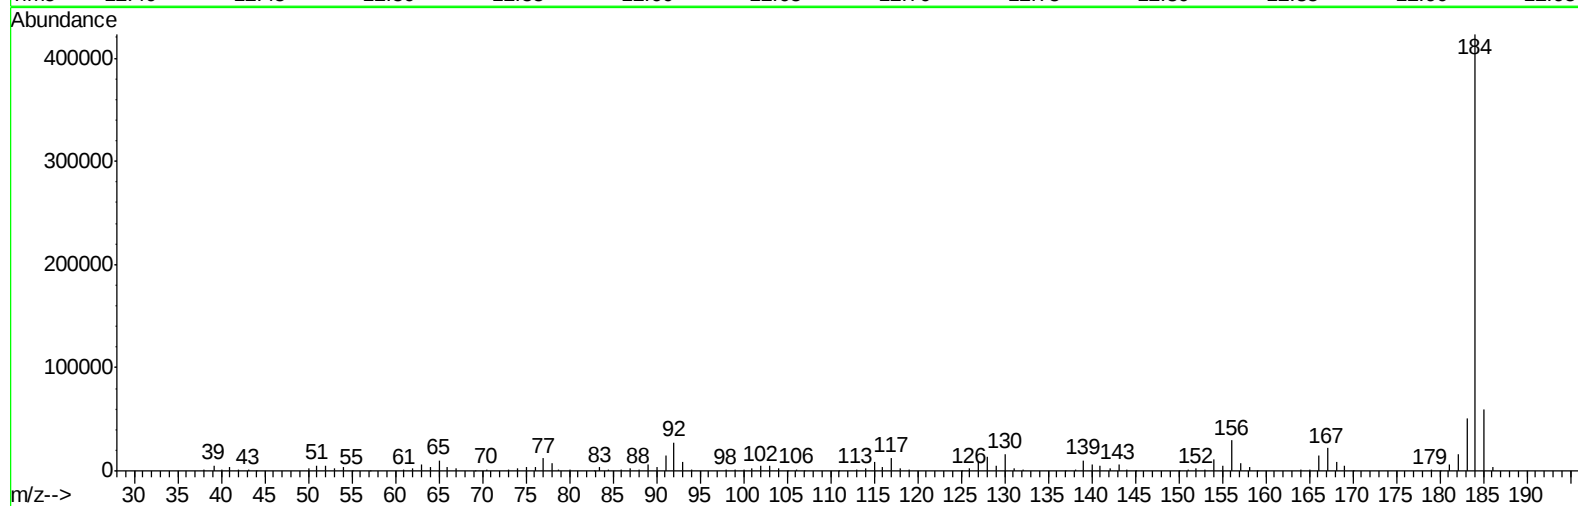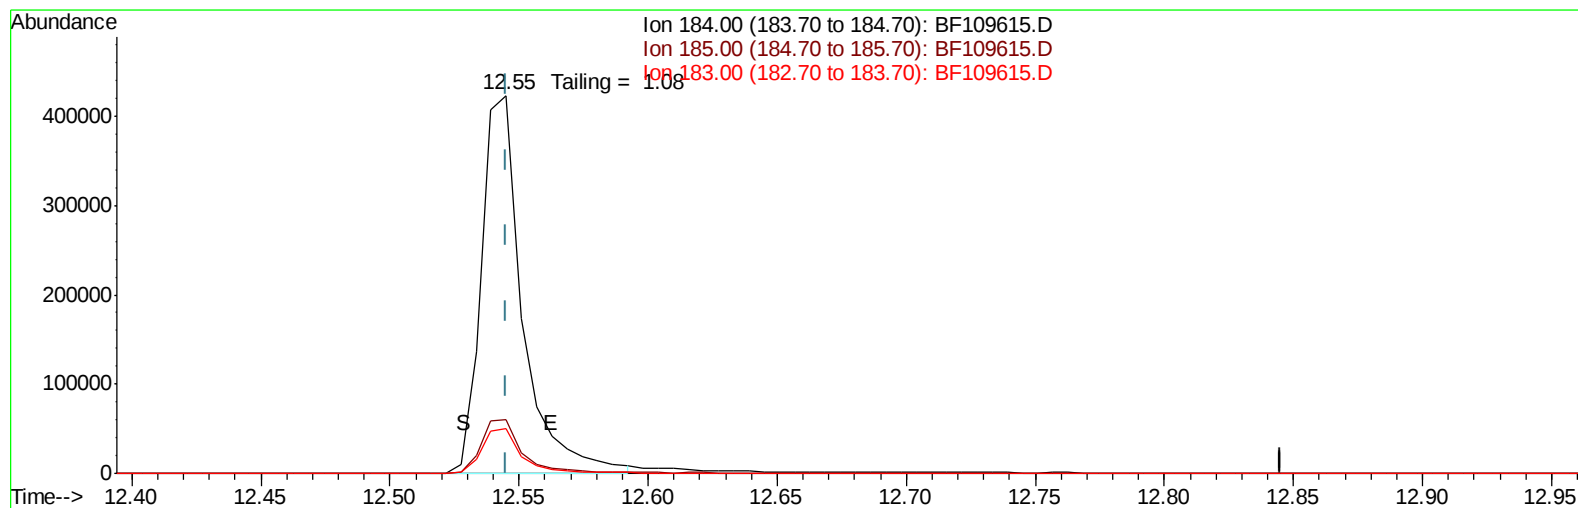

TIC: BF109615.D

(76) Benzidine

12.545min (+0.000) 0.00ng

response 492713

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.11
183.00	11.60	11.89
0.00	0.00	0.00