
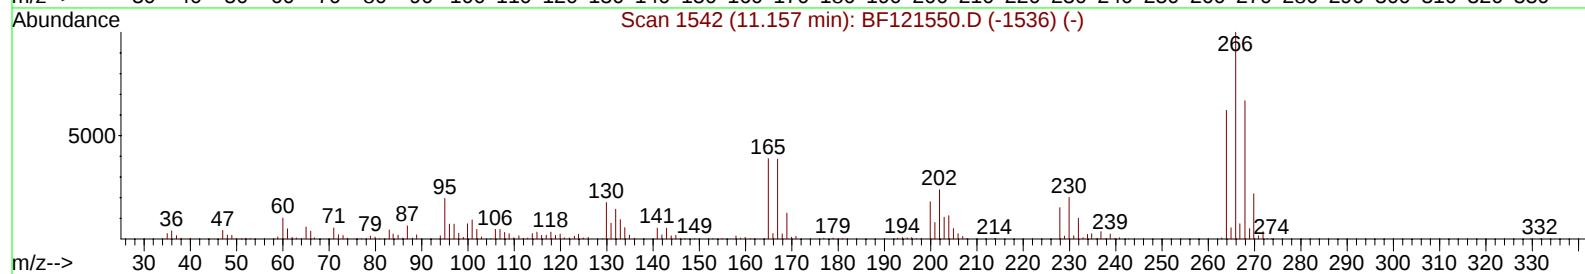
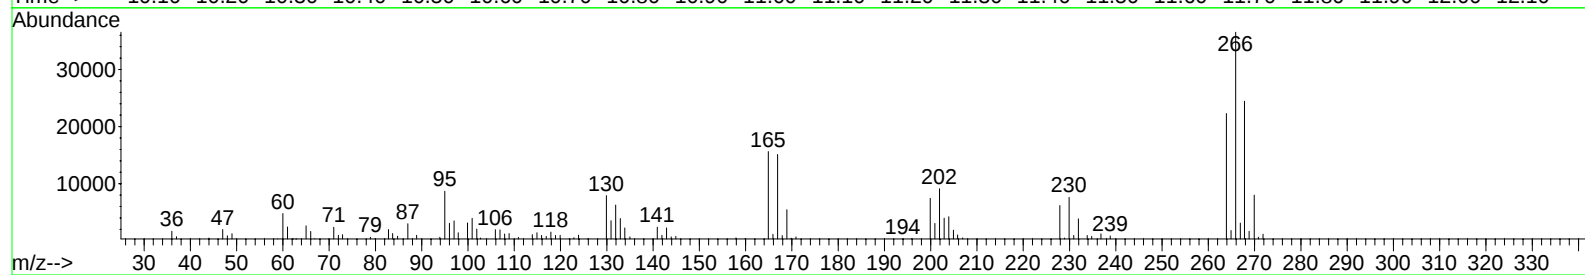


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100620\
 Data File : BF121840.D
 Acq On : 6 Oct 2020 8:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 19:11:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 14:29:14 2020
 Response via : Initial Calibration

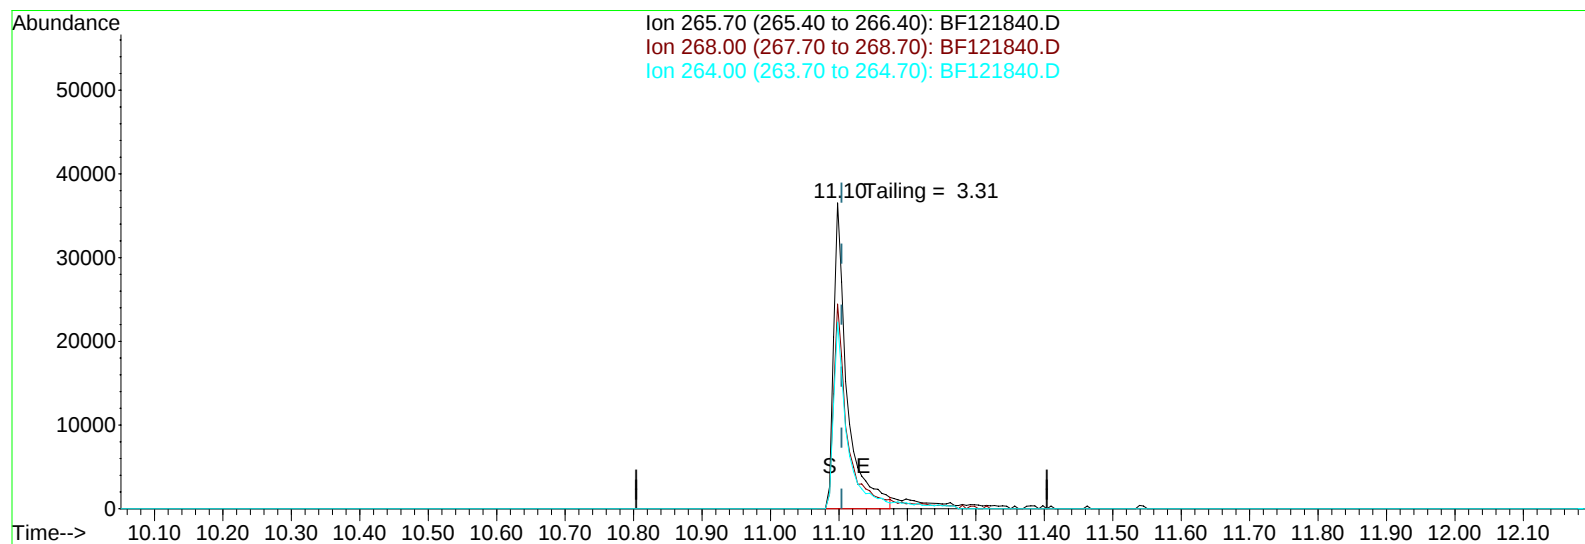

TIC: BF121840.D

(70) Pentachlorophenol (C)




11.098min (-0.006) 16495.79ng

response 51682

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	66.95
264.00	62.40	60.99
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100620\
 Data File : BF121840.D
 Acq On : 6 Oct 2020 8:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 19:11:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 14:29:14 2020
 Response via : Initial Calibration

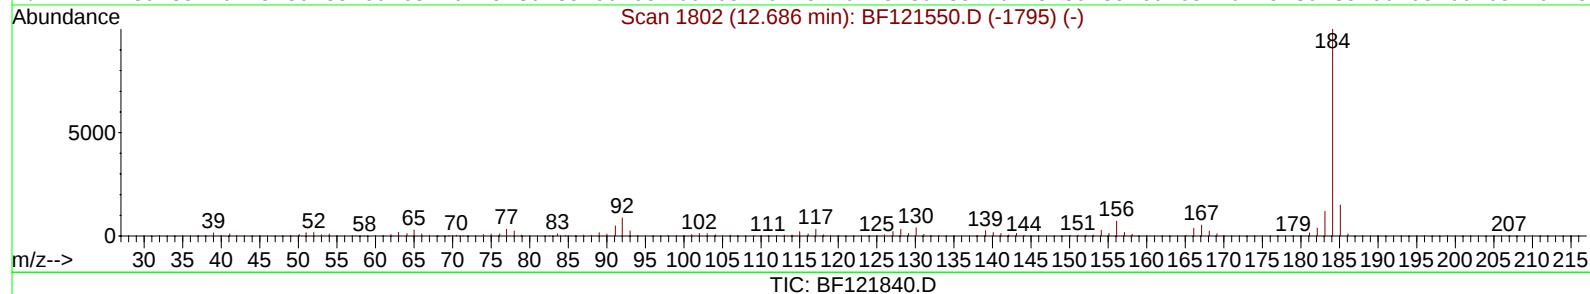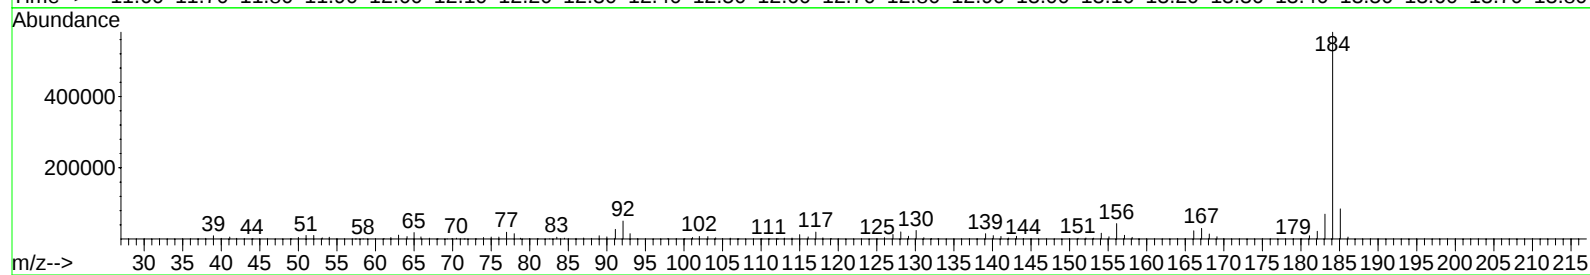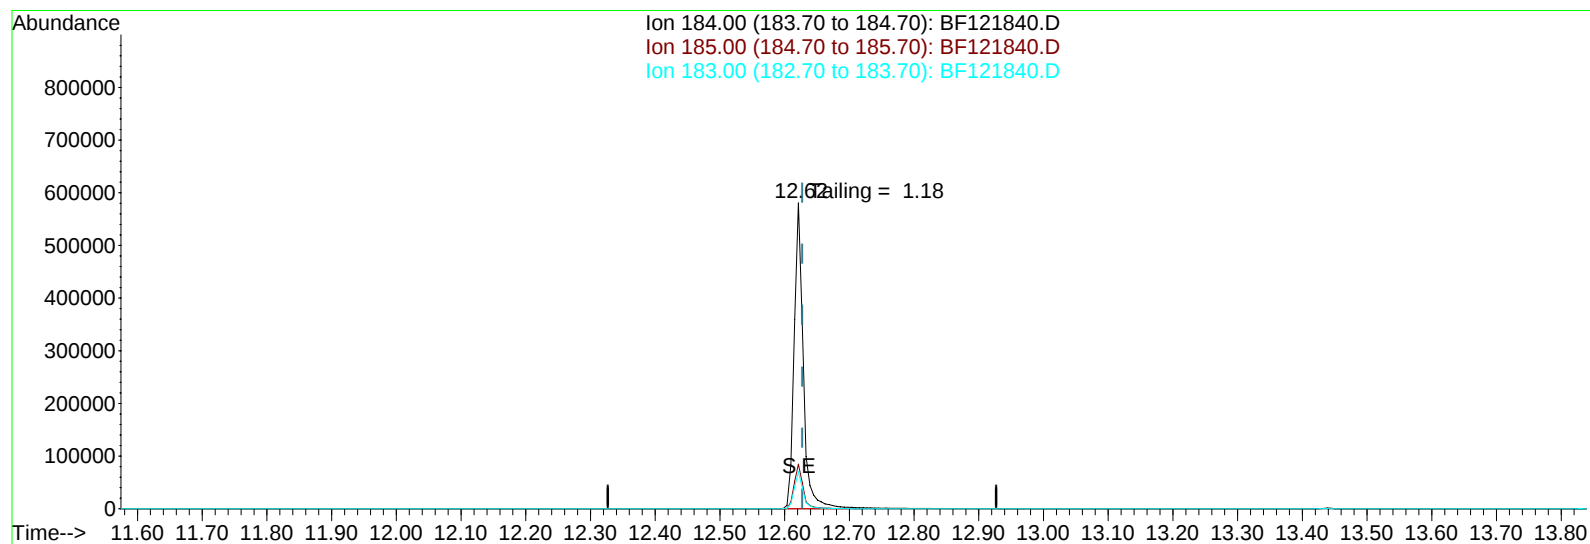

(77) Benzidine

12.621min (-0.006) 0.00ng

response 580814

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.61
183.00	11.70	12.07
0.00	0.00	0.00