

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100620\
 Data File : BF121842.D
 Acq On : 6 Oct 2020 9:33
 Operator : JU/CG
 Sample : PB132042BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB132042BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.010	493	497	506	rBV	44660	67946	1.29%	0.224%
2	5.398	558	563	566	rBV	3598540	3654329	69.23%	12.045%
3	6.410	729	735	738	rBV	3313714	3685603	69.83%	12.148%
4	6.763	791	795	798	rBV	1057833	839530	15.91%	2.767%
5	7.334	886	892	895	rBV	2306987	2695354	51.07%	8.884%
6	8.045	1008	1013	1035	rBV	1170025	1128593	21.38%	3.720%
7	9.122	1190	1196	1207	rBV	4049482	4675699	88.58%	15.411%
8	9.798	1305	1311	1321	rBV	1404285	1299880	24.63%	4.284%
9	10.592	1439	1446	1474	rBV	2820034	3004548	56.92%	9.903%
10	11.286	1557	1564	1572	rBV	1359927	1366585	25.89%	4.504%
11	12.874	1826	1834	1837	rBV	5040887	5278245	100.00%	17.397%
12	13.921	2008	2012	2024	rVB	1380216	1345701	25.50%	4.435%
13	15.362	2251	2257	2274	rVB	913486	1297533	24.58%	4.277%


Sum of corrected areas: 30339546

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100620\
Data File : BF121842.D
Acq On : 6 Oct 2020 9:33
Operator : JU/CG
Sample : PB132042BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132042BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

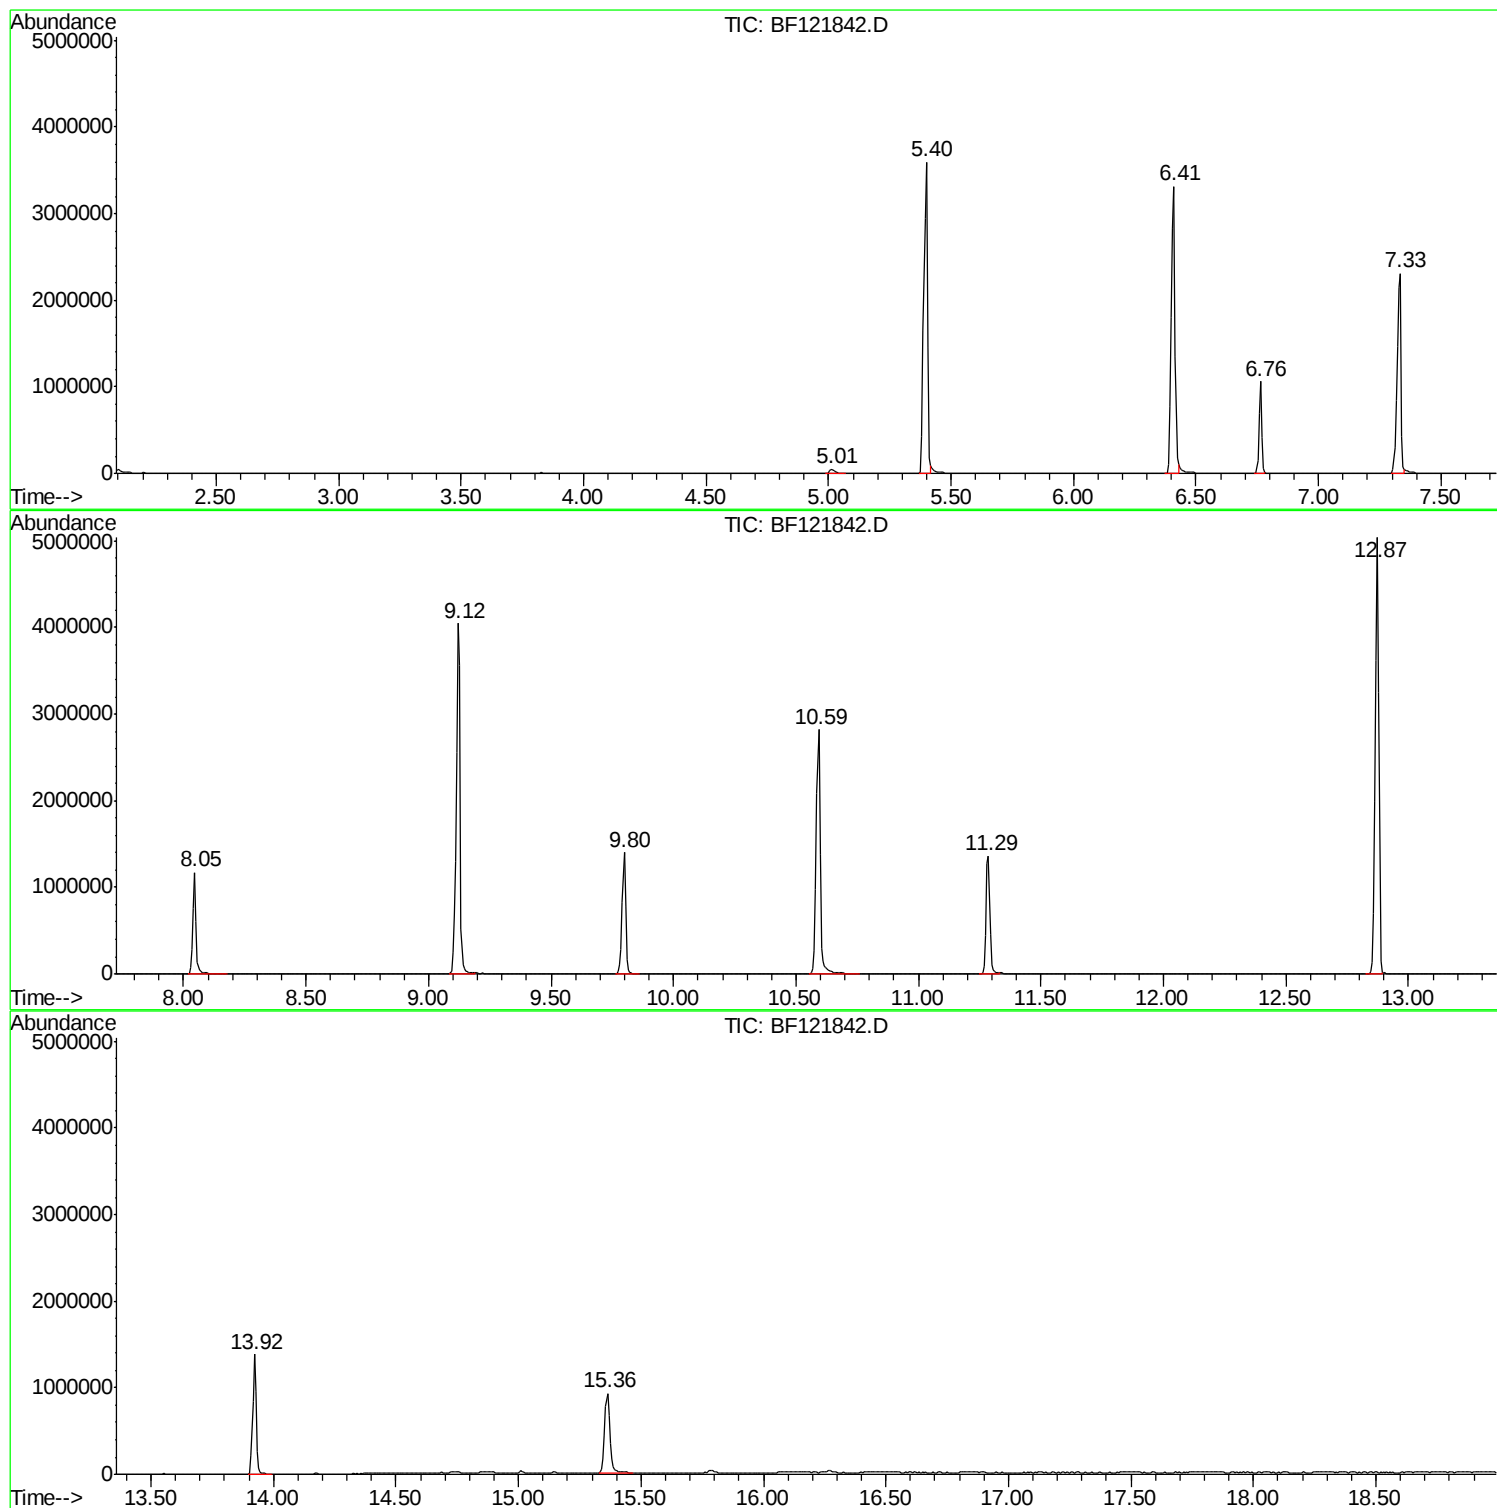

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100620\
Data File : BF121842.D
Acq On : 6 Oct 2020 9:33
Operator : JU/CG
Sample : PB132042BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132042BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100620\
Data File : BF121842.D
Acq On : 6 Oct 2020 9:33
Operator : JU/CG
Sample : PB132042BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132042BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc