


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100620\
 Data File : BF121840.D
 Acq On : 6 Oct 2020 8:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 14:29:14 2020

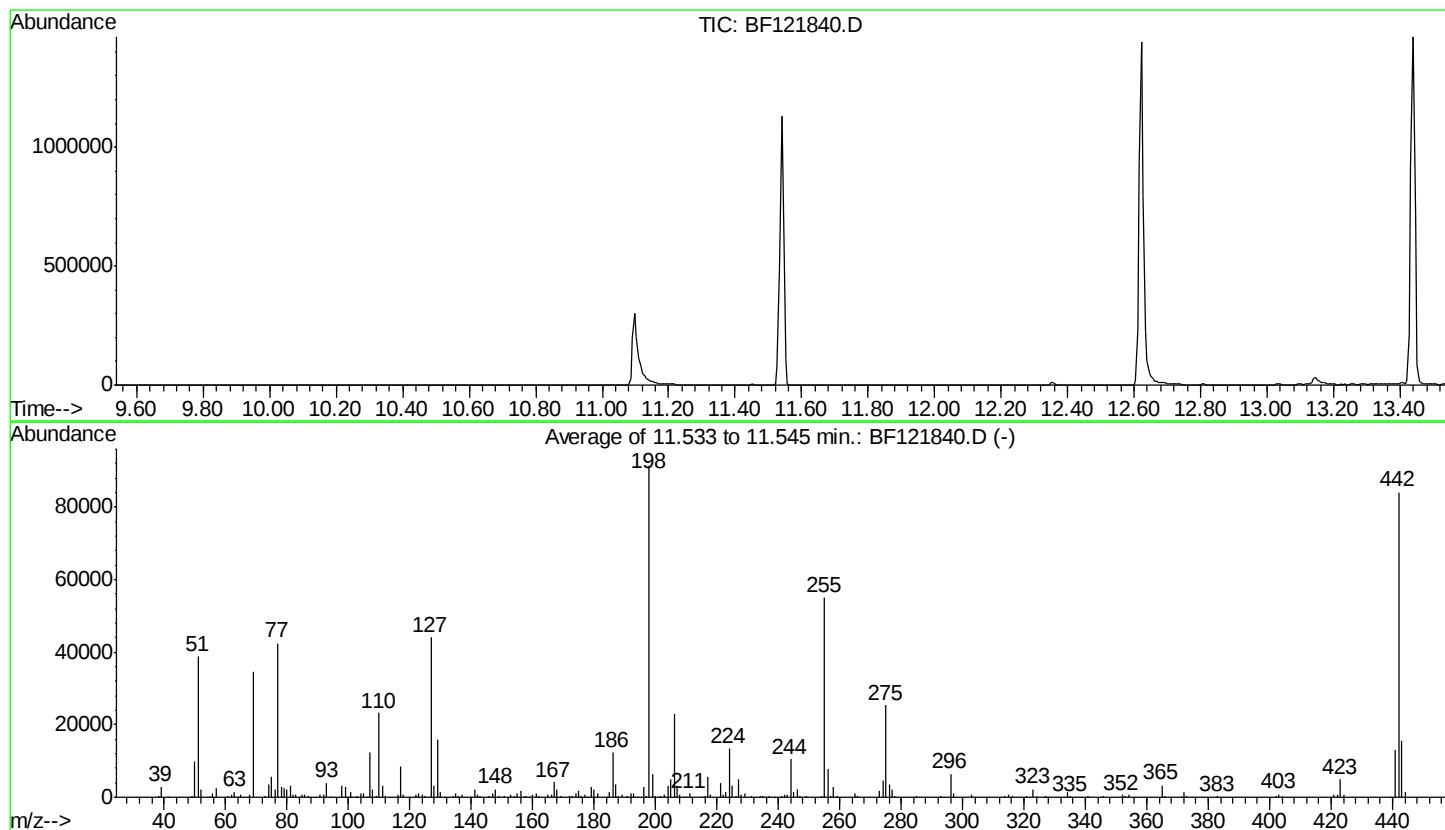

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	38688	PASS
68	69	0.00	2	1.7	588	PASS
69	198	0.00	100	37.9	34658	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	43981	PASS
197	198	0.00	2	0.4	321	PASS
198	198	100	100	100.0	91466	PASS
199	198	5	9	7.0	6447	PASS
275	198	10	60	27.7	25307	PASS
365	198	1	100	3.5	3202	PASS
441	198	0.01	100	14.4	13159	PASS
442	198	50	100	92.1	84210	PASS
443	442	15	24	18.4	15482	PASS